

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006922.D
 Acq On : 19 Jul 2019 13:51
 Operator : HP/JU
 Sample : PB121403BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 23:33:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2598	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	9674	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	5011	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	717924	0.40	ng/ul	0.08
16) Chrysene-d12	21.25	240	7617	0.40	ng/ul	0.02
20) Perylene-d12	23.32	264	664790	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	3359	0.23	ng/ul	0.02
14) Fluoranthene-d10	19.06	212	5791	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.23	166	1219	0.056	ng/ul#	15
17) Pyrene	19.41	202	1283	0.037	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006922.D
Acq On : 19 Jul 2019 13:51
Operator : HP/JU
Sample : PB121403BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 23:33:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

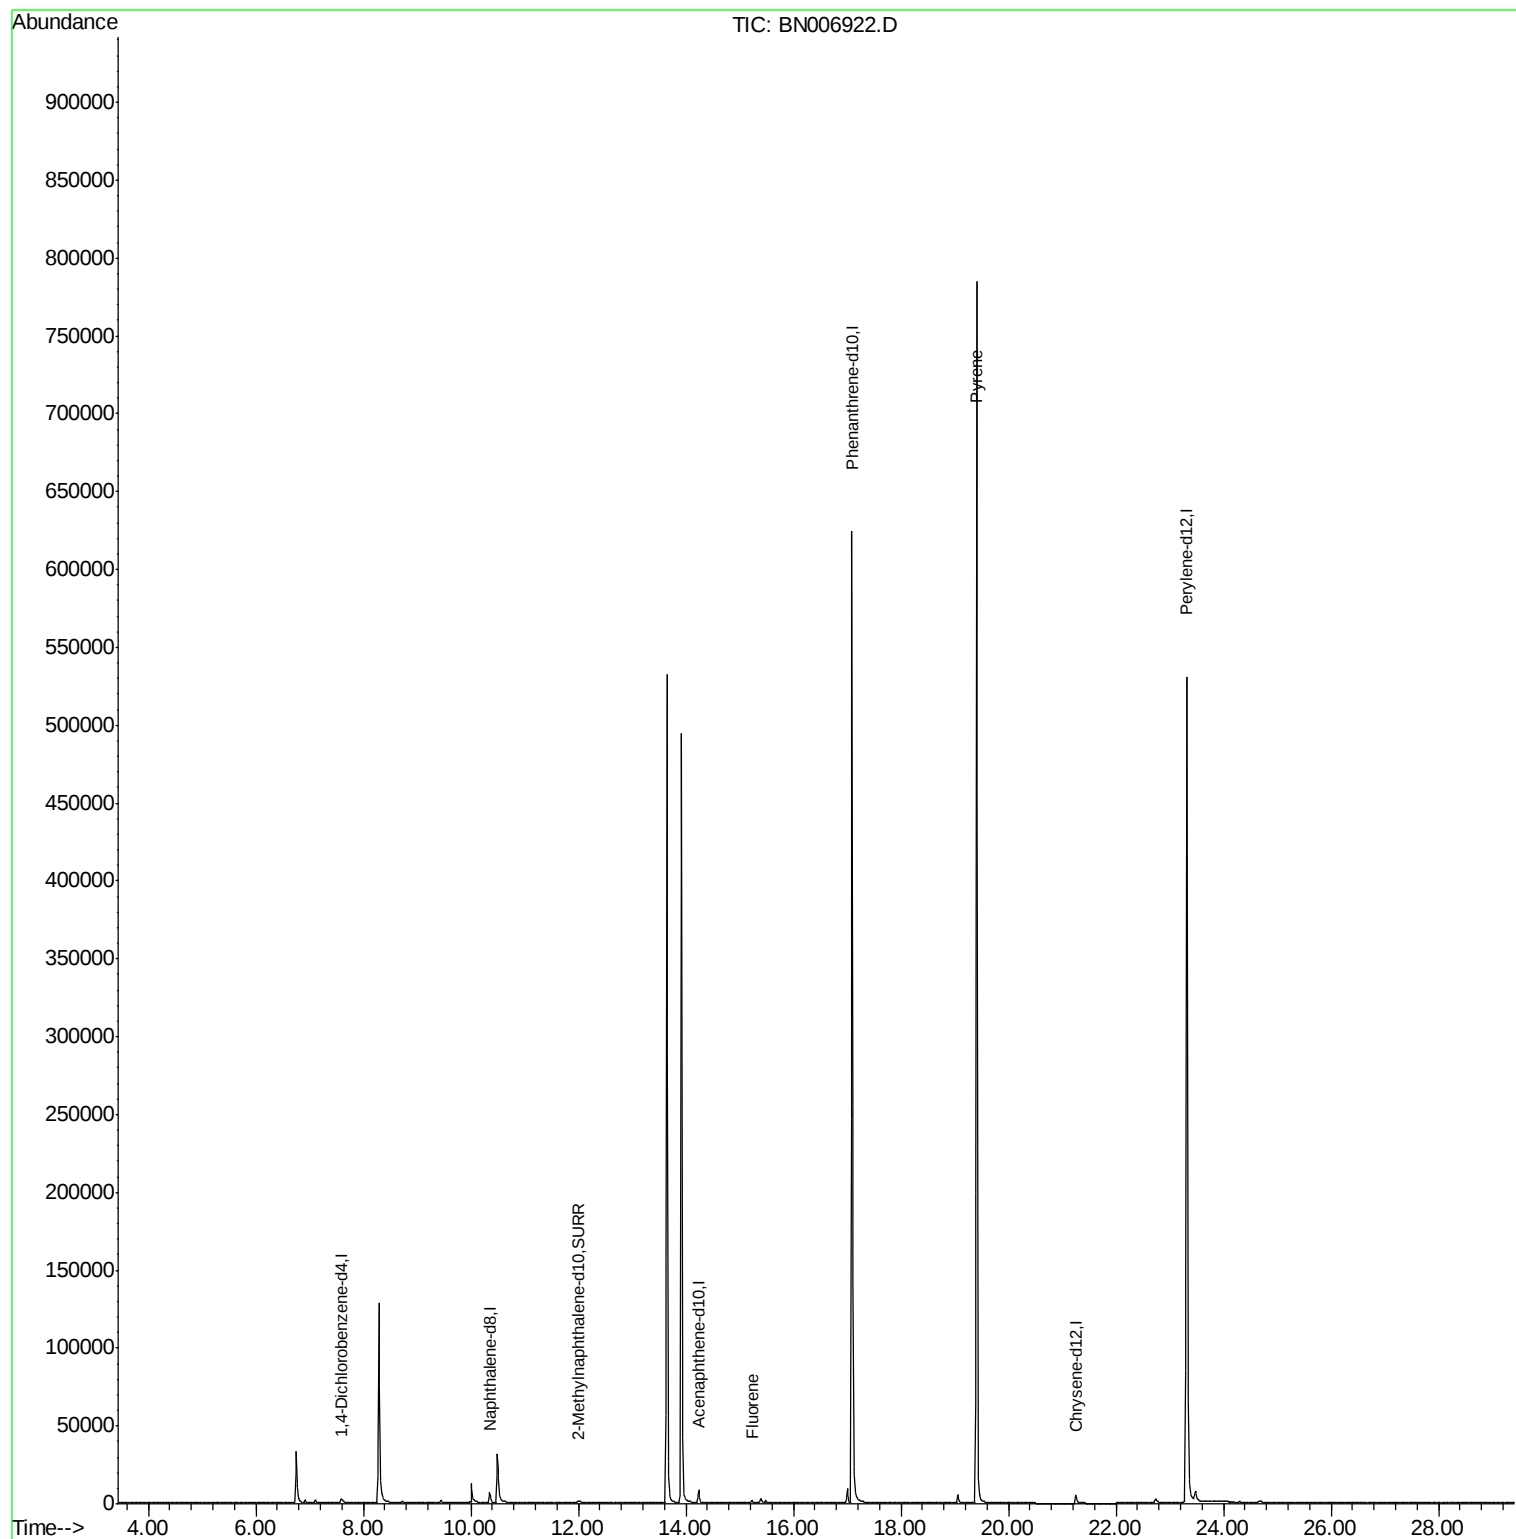

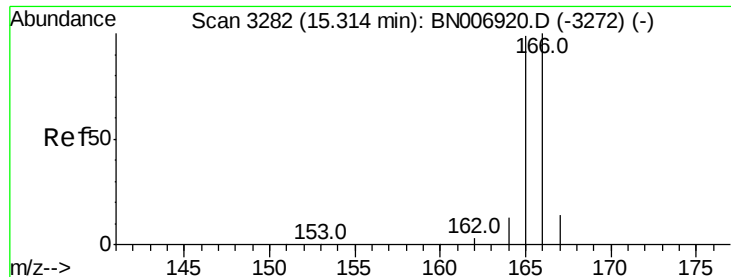

#9

Fluorene

Concen: 0.056 ng/ul

RT: 15.23 min Scan# 3264

Delta R.T. -0.08 min

Lab File: BN006922.D

Acq: 19 Jul 2019 13:51

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 1219

Ion Ratio Lower Upper

166 100

165 9.8 78.2 117.4#




167 36.2 11.3 16.9#

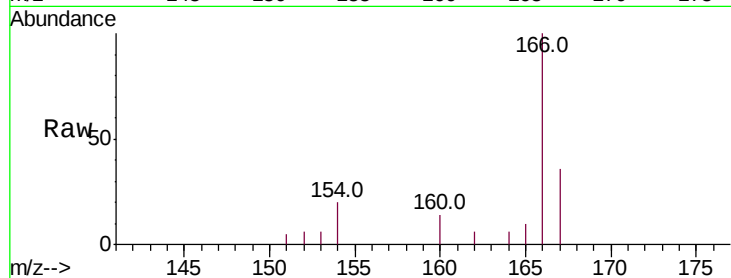

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

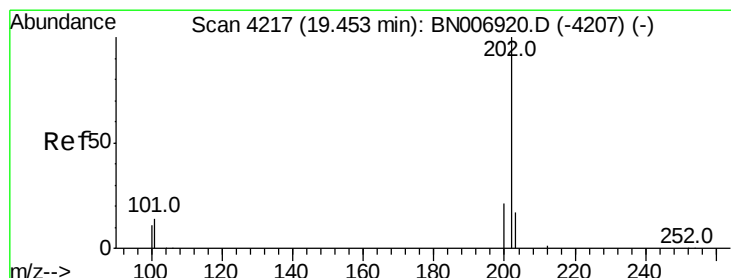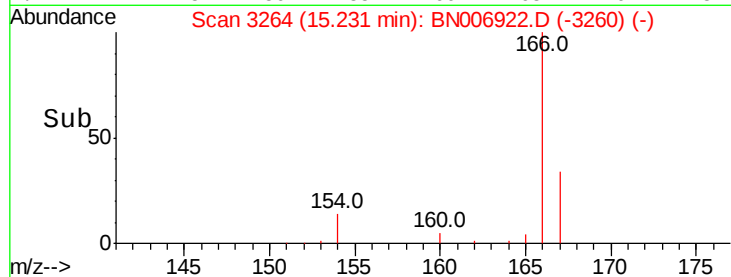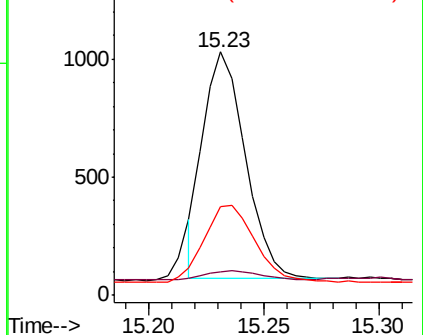

#17

Pyrene

Concen: 0.037 ng/ul

RT: 19.41 min Scan# 4207

Delta R.T. -0.05 min

Lab File: BN006922.D

Acq: 19 Jul 2019 13:51


Tgt Ion:202 Resp: 1283

Ion Ratio Lower Upper

202 100

101 177.4 12.2 18.2#

100 1211.7 9.8 14.8#

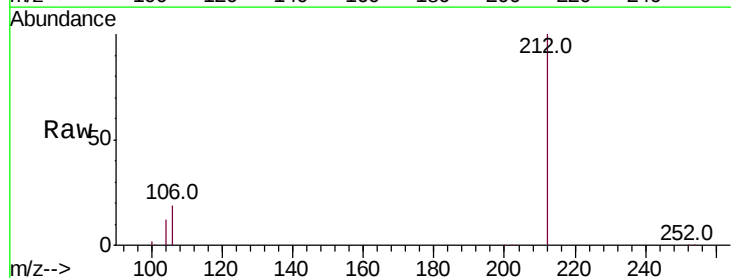

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

