

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006924.D
 Acq On : 19 Jul 2019 15:01
 Operator : HP/JU
 Sample : K3764-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 23:33:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2275	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.36	136	8080	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	4046	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	8535	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	6198	0.40	ng/ul	0.01
20) Perylene-d12	23.48	264	9288	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	1603	0.13	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	3719	0.15	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.32	252	934	0.025	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006924.D
Acq On : 19 Jul 2019 15:01
Operator : HP/JU
Sample : K3764-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 23:33:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

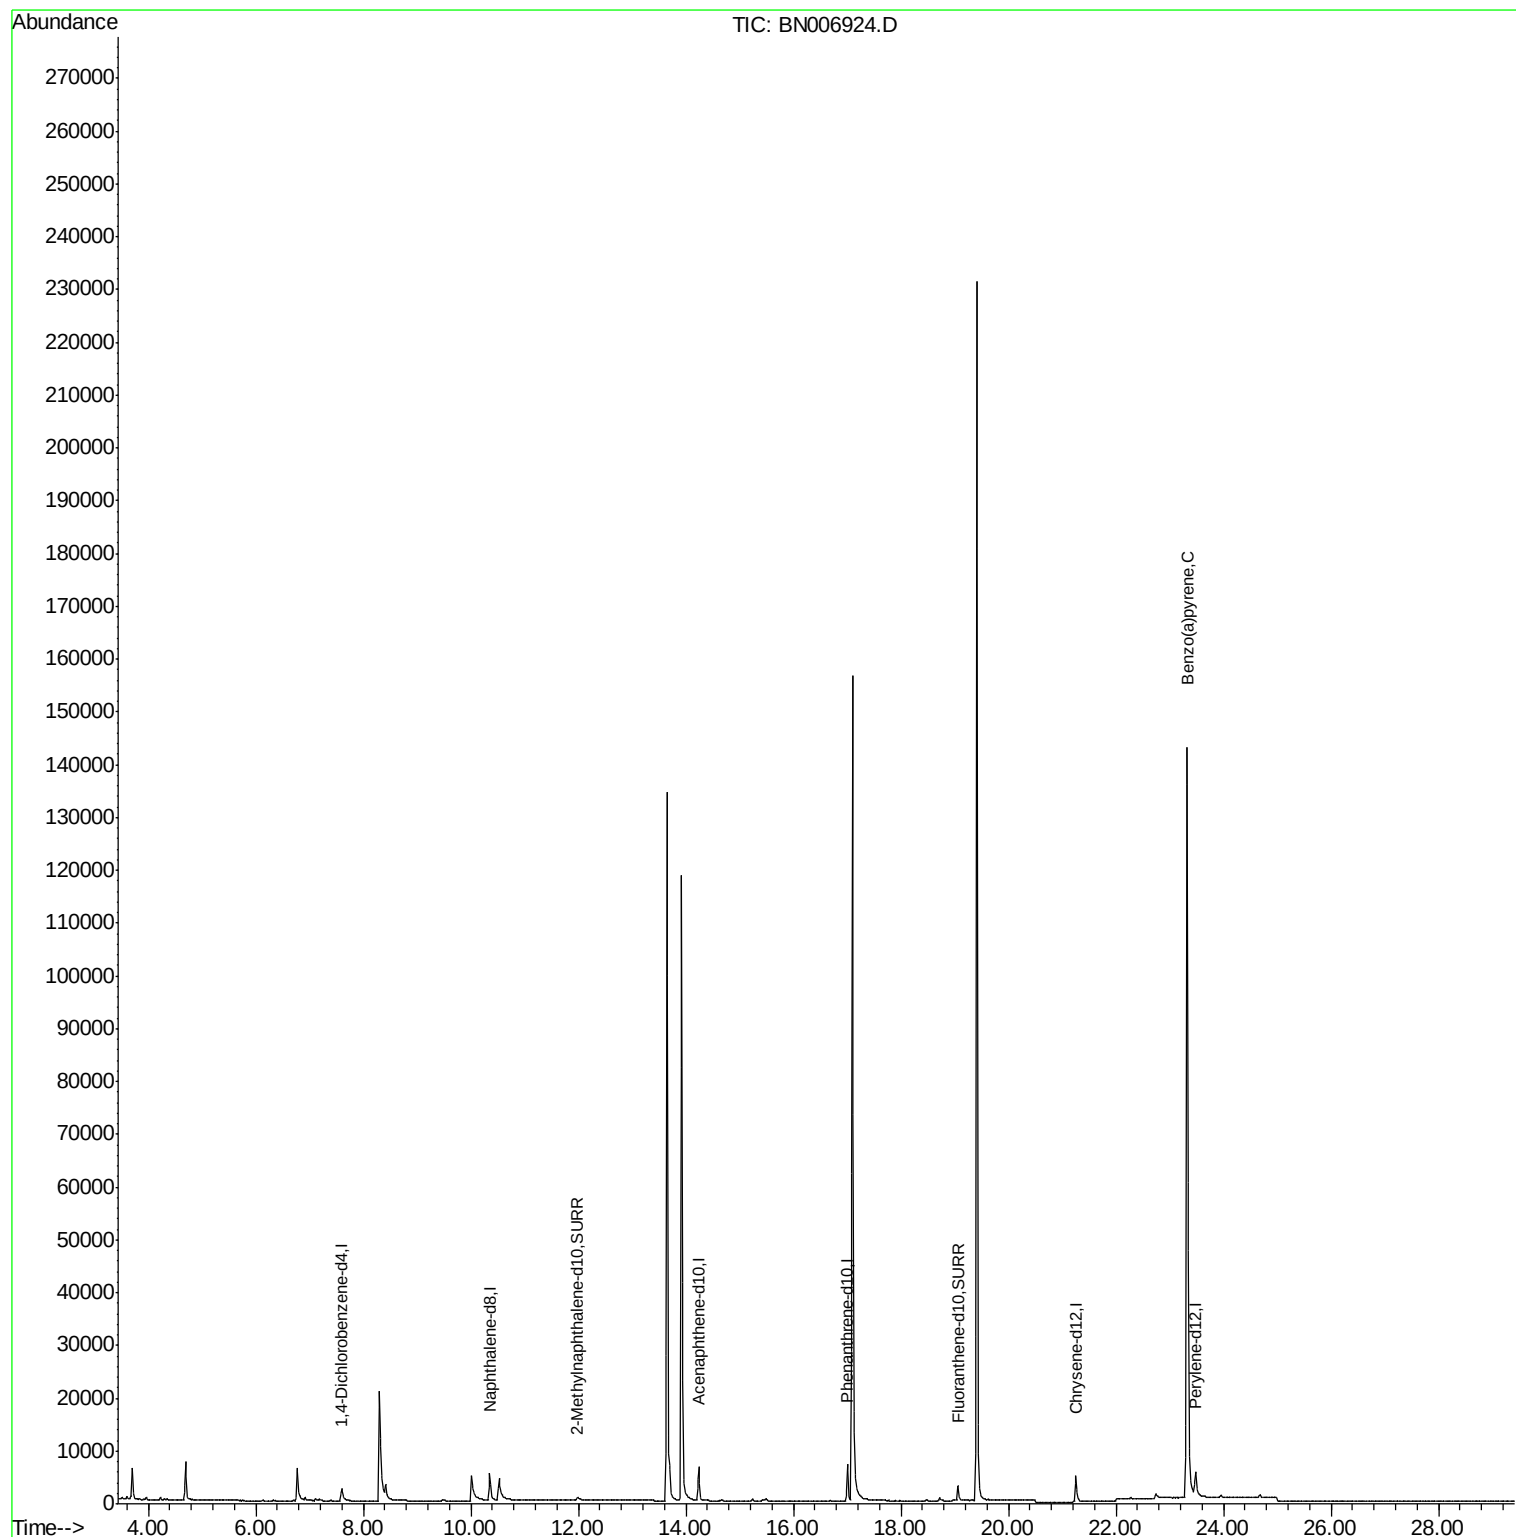

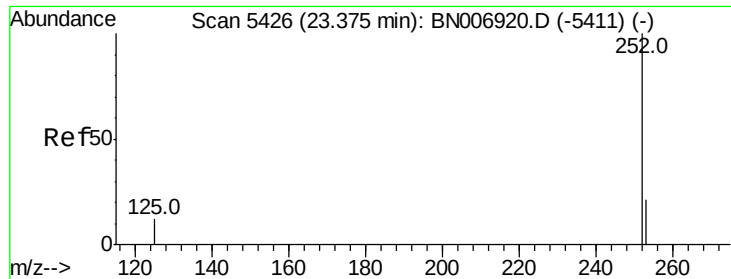

#23

Benzo(a)pyrene

Concen: 0.025 ng/ul

RT: 23.32 min Scan# 5407

Delta R.T. -0.06 min

Lab File: BN006924.D

Acq: 19 Jul 2019 15:01

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 934

Ion Ratio Lower Upper

252 100

253 69.6 19.4 29.2#

125 121.2 12.6 19.0#

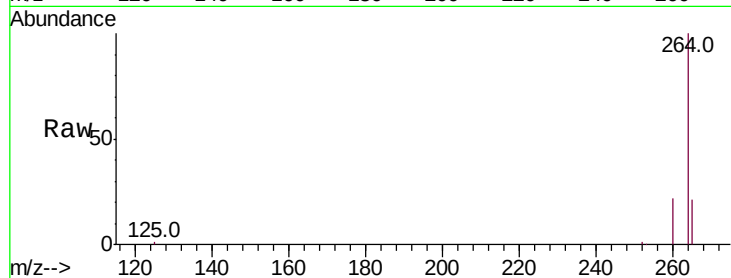

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

