

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006928.D
 Acq On : 19 Jul 2019 17:28
 Operator : HP/JU
 Sample : K3823-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 23:33:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2156	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	7658	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	3815	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	761845	0.40	ng/ul	0.08
16) Chrysene-d12	21.25	240	5634	0.40	ng/ul	0.01
20) Perylene-d12	23.31	264	734127	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	2952	0.25	ng/ul	0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.40	128	832	0.038	ng/ul#	67
17) Pyrene	19.41	202	1513	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006928.D
Acq On : 19 Jul 2019 17:28
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 23:33:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

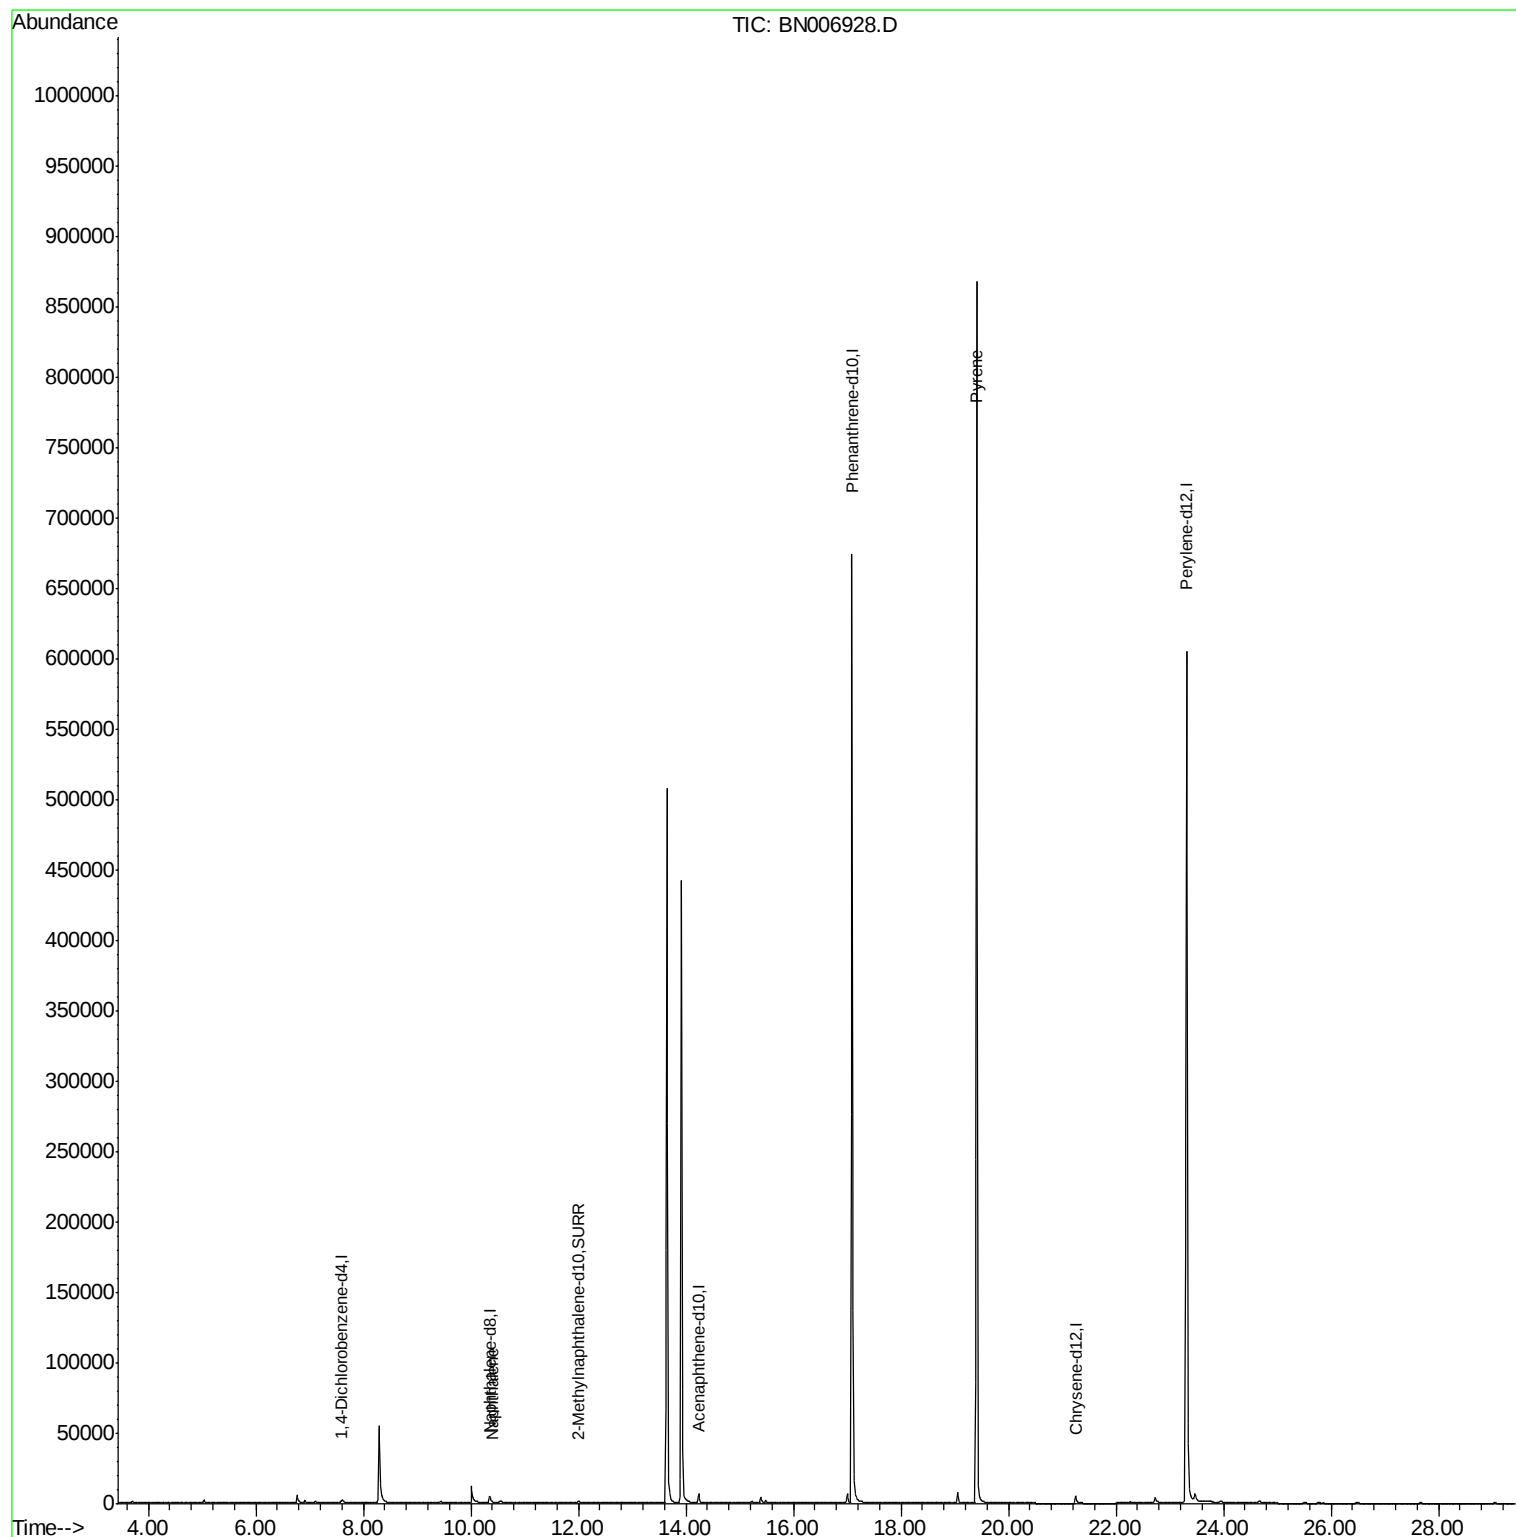

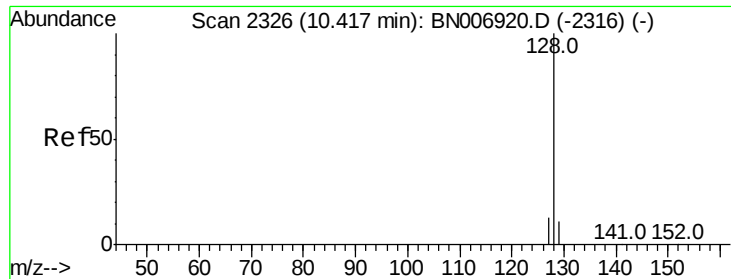

#3

Naphthalene

Concen: 0.038 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006928.D

Acq: 19 Jul 2019 17:28

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 832

Ion Ratio Lower Upper

128 100

129 27.5 9.4 14.0#




127 23.8 10.6 16.0#

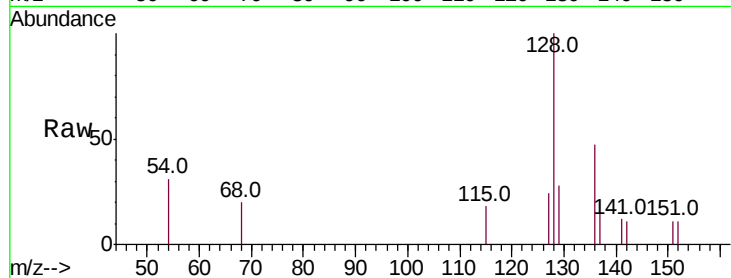

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

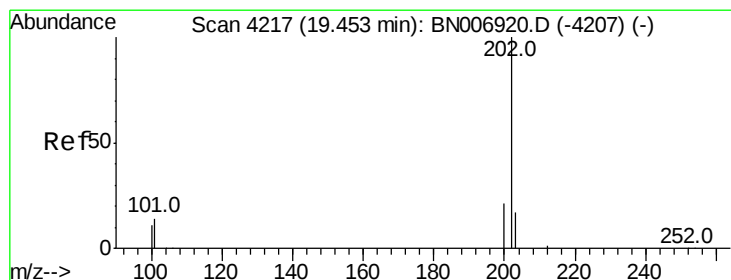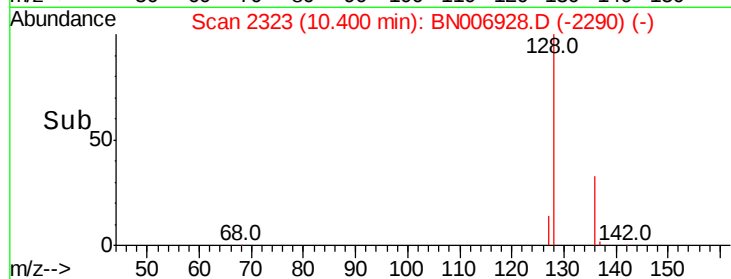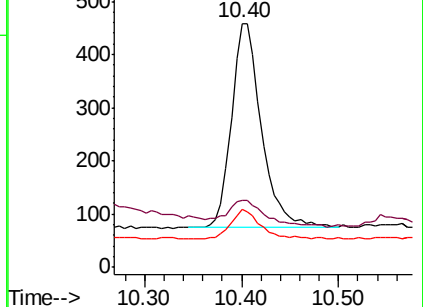

#17

Pyrene

Concen: 0.059 ng/ul

RT: 19.41 min Scan# 4207

Delta R.T. -0.05 min

Lab File: BN006928.D

Acq: 19 Jul 2019 17:28


Tgt Ion:202 Resp: 1513

Ion Ratio Lower Upper

202 100

101 174.6 12.2 18.2#

100 1202.5 9.8 14.8#

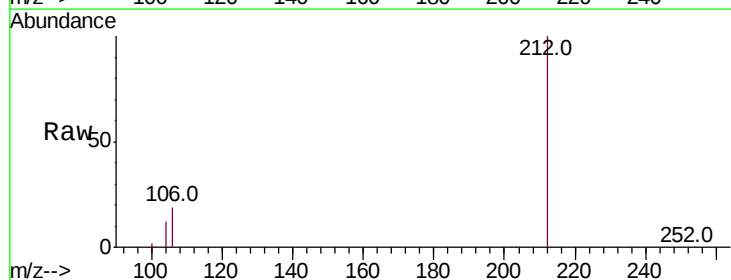

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

