

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006932.D
 Acq On : 19 Jul 2019 19:48
 Operator : HP/JU
 Sample : PB121511BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 23:33:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2482	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8870	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4361	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	761735	0.40	ng/ul	0.08
16) Chrysene-d12	21.24	240	5665	0.40	ng/ul	0.00
20) Perylene-d12	23.29	264	566346	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	3612	0.26	ng/ul	0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
9) Fluorene	15.23	166	1312	0.069	ng/ul#	16
17) Pyrene	19.40	202	1350	0.052	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006932.D
Acq On : 19 Jul 2019 19:48
Operator : HP/JU
Sample : PB121511BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 23:33:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

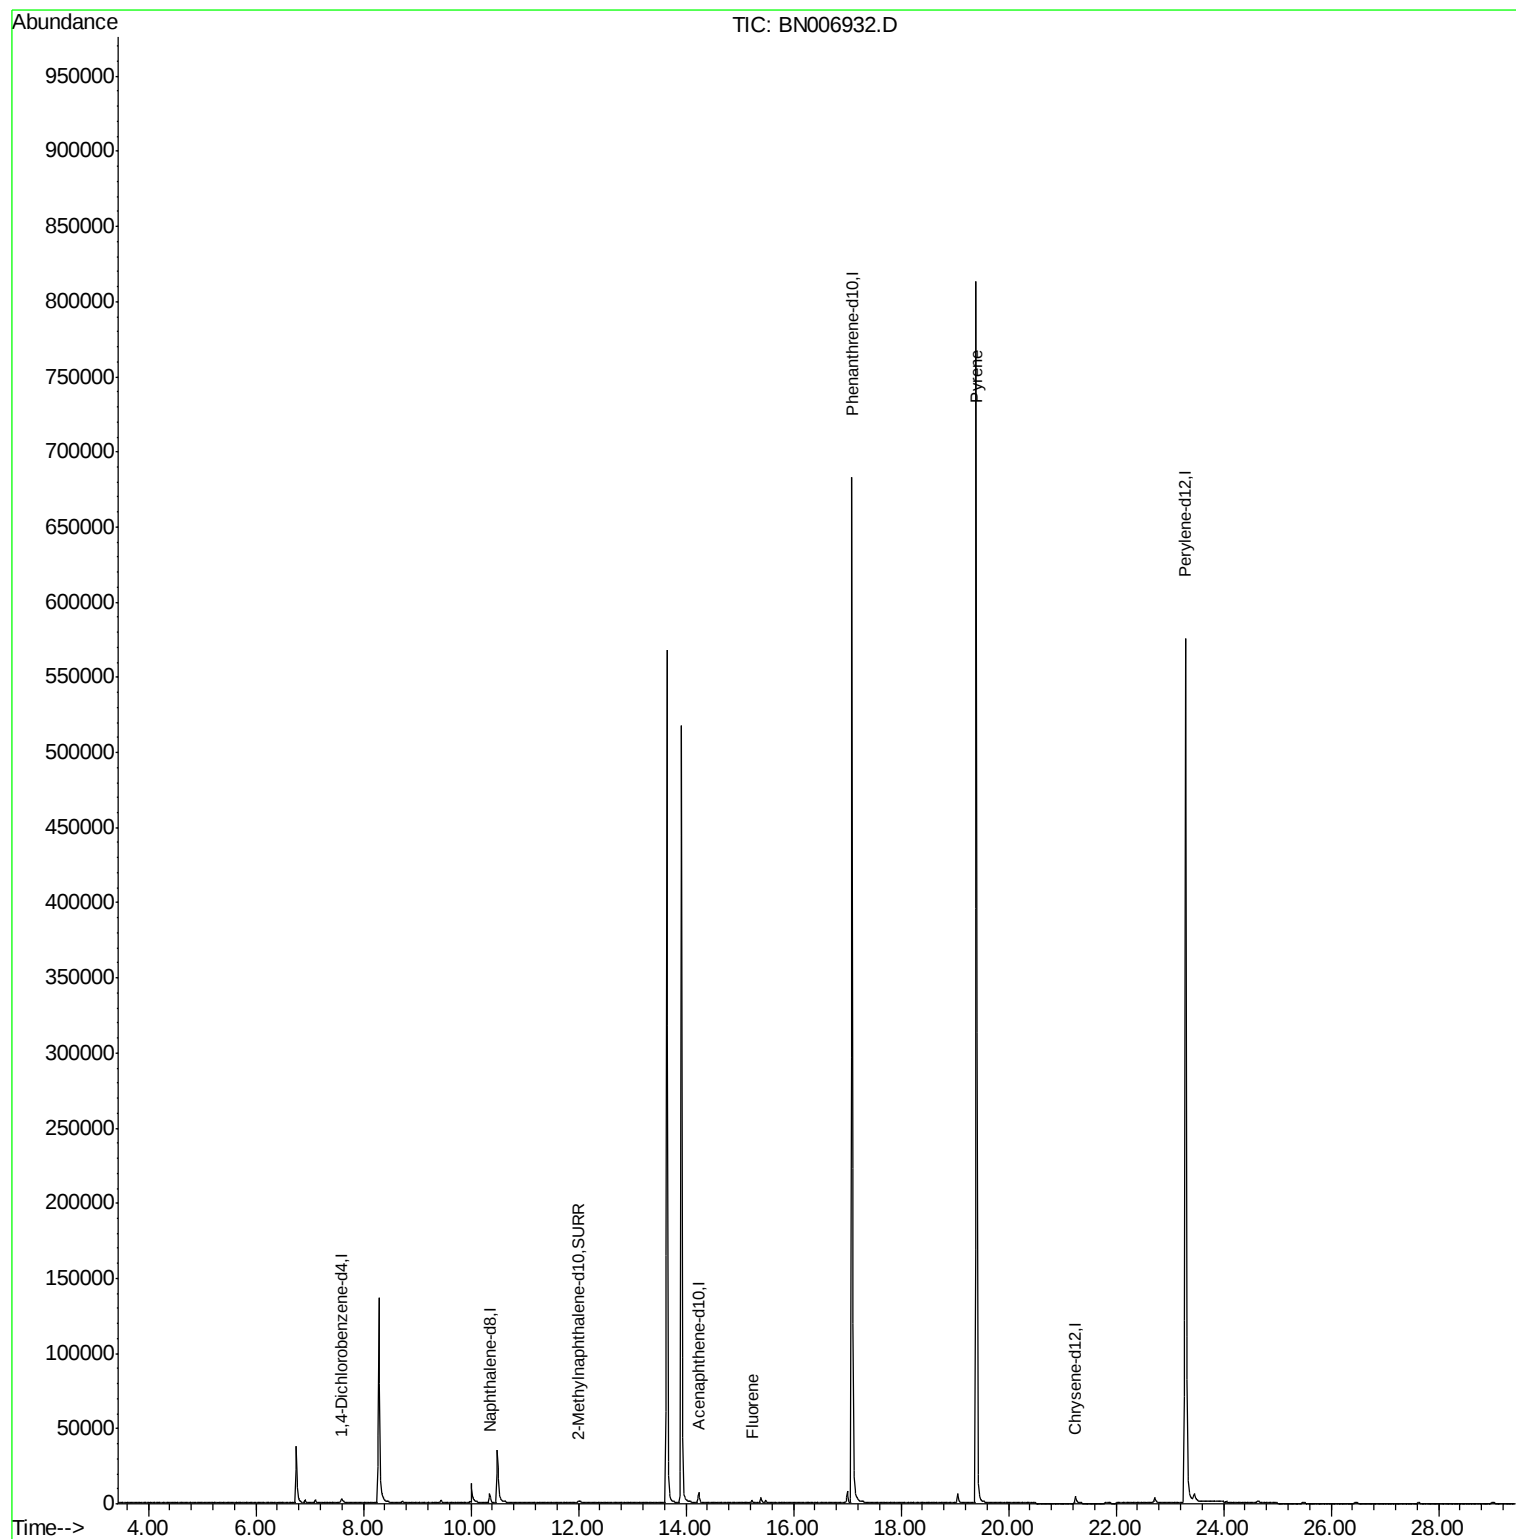

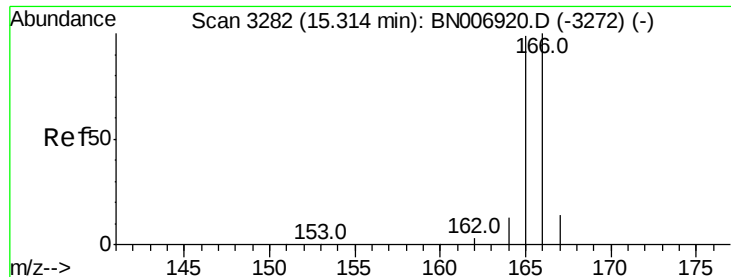

#9

Fluorene

Concen: 0.069 ng/ul

RT: 15.23 min Scan# 3264

Delta R.T. -0.08 min

Lab File: BN006932.D

Acq: 19 Jul 2019 19:48

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 1312

Ion Ratio Lower Upper




166 100

165 9.8 78.2 117.4#

167 35.3 11.3 16.9#

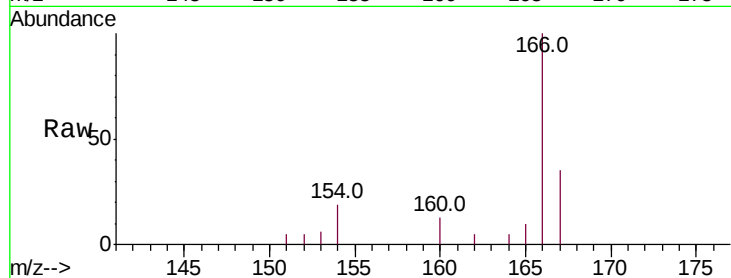

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

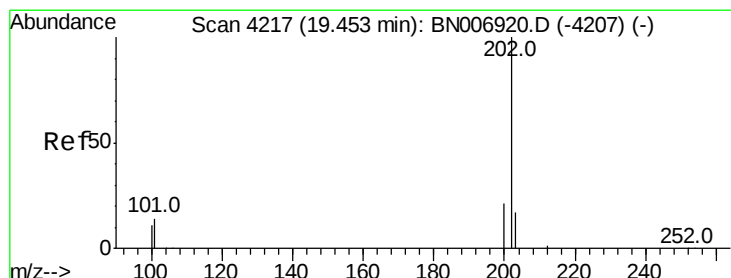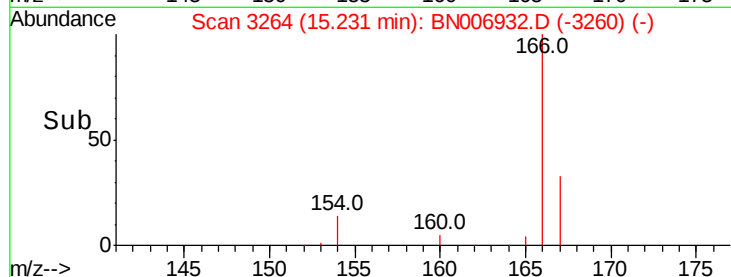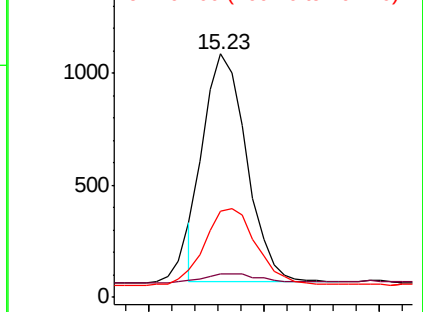

#17

Pyrene

Concen: 0.052 ng/ul

RT: 19.40 min Scan# 4206

Delta R.T. -0.05 min

Lab File: BN006932.D

Acq: 19 Jul 2019 19:48


Tgt Ion:202 Resp: 1350

Ion Ratio Lower Upper

202 100

101 181.2 12.2 18.2#

100 1261.2 9.8 14.8#

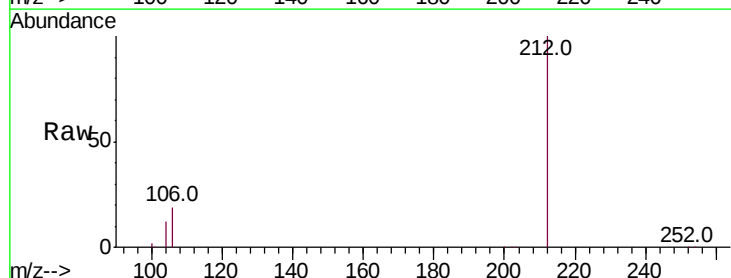

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

