

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006936.D
 Acq On : 19 Jul 2019 22:08
 Operator : HP/JU
 Sample : K3823-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 23:33:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2410	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8535	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4340	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	780456	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.29	264	628171	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	3157	0.24	ng/ul	0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.41	128	862	0.035	ng/ul#	Ovalue 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006936.D
Acq On : 19 Jul 2019 22:08
Operator : HP/JU
Sample : K3823-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 23:33:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

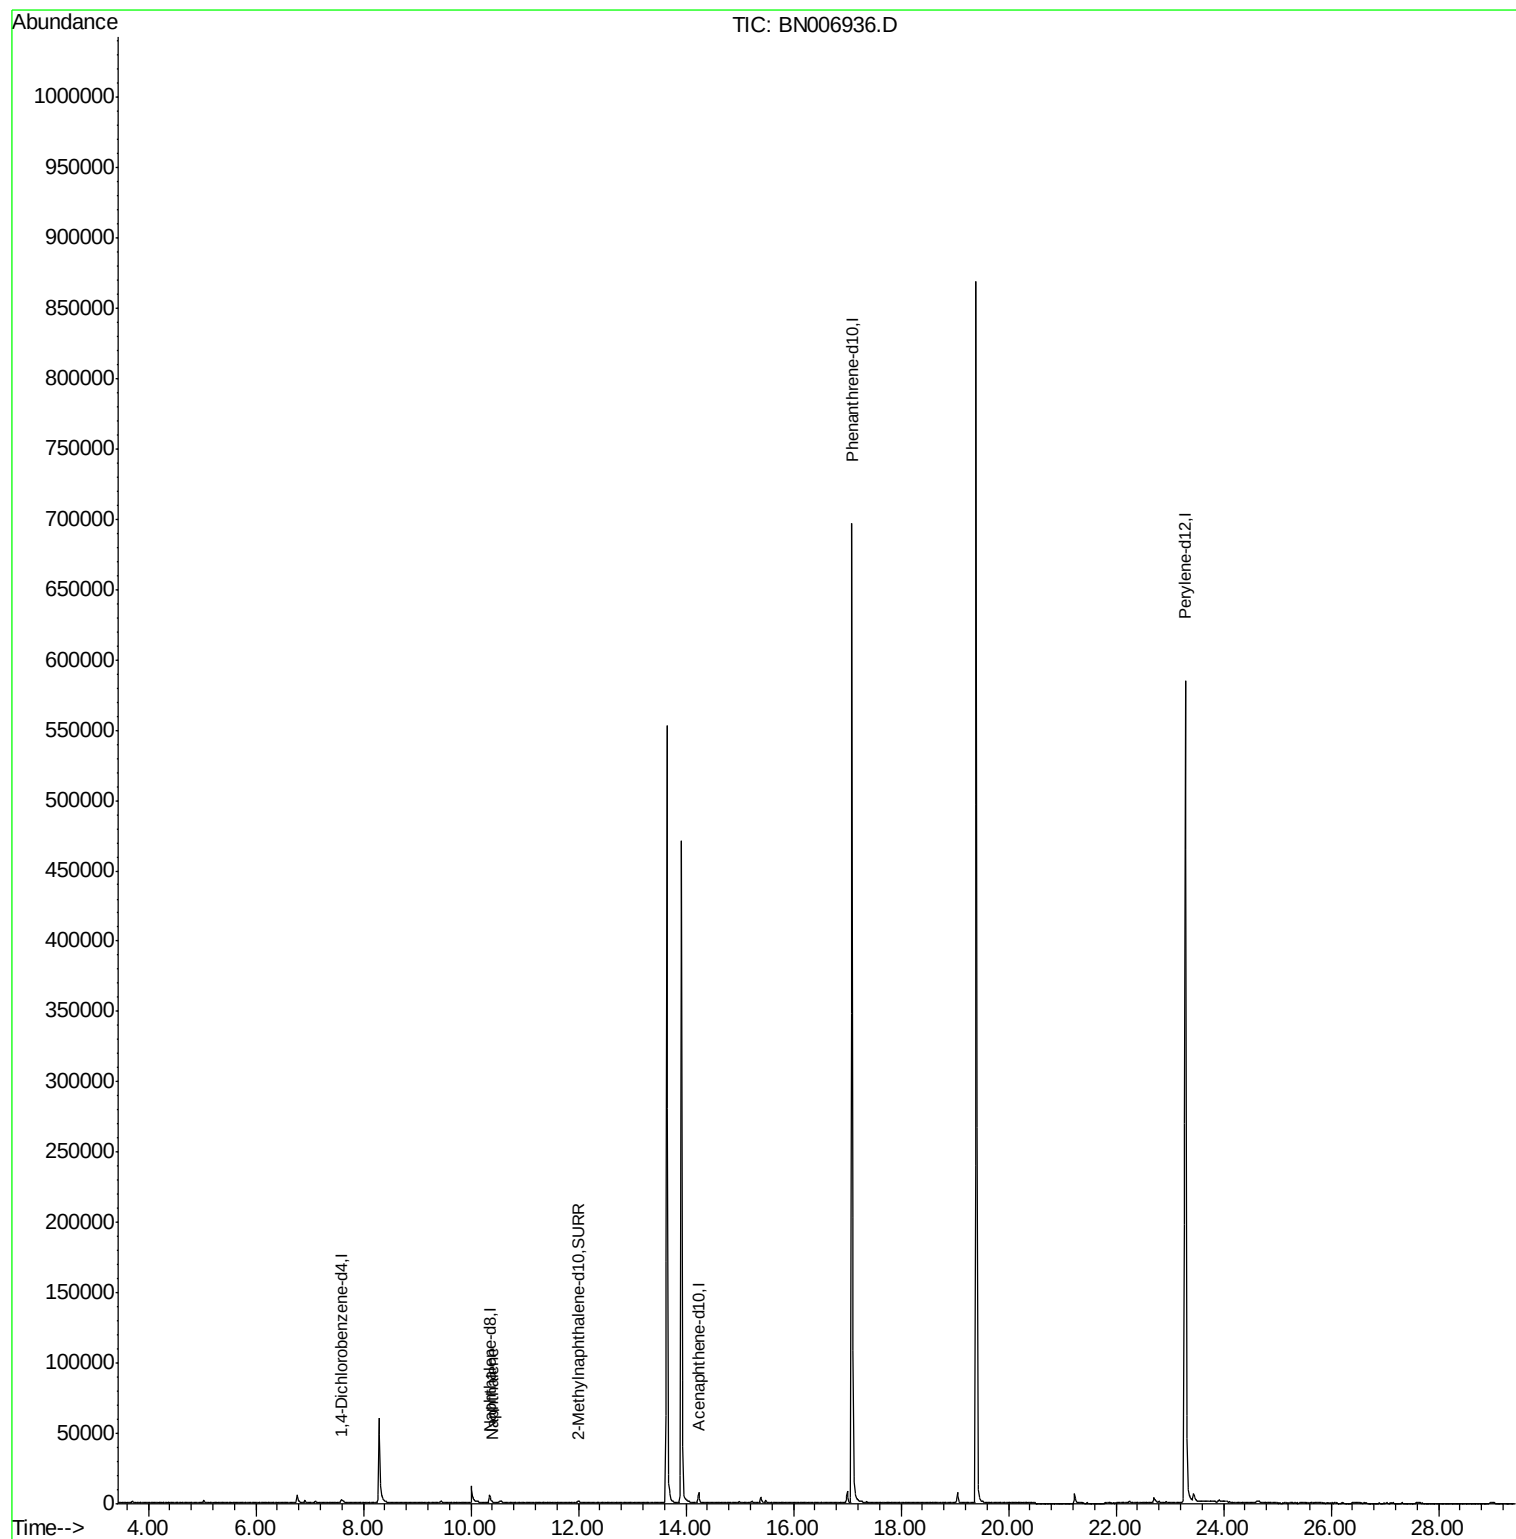

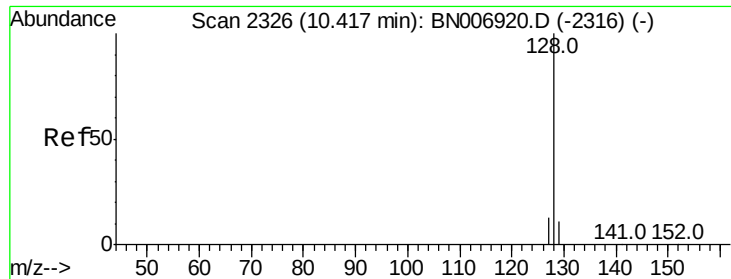

#3

Naphthalene

Concen: 0.035 ng/ul

RT: 10.41 min Scan# 2324

Delta R.T. -0.01 min

Lab File: BN006936.D

Acq: 19 Jul 2019 22:08

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 862

Ion Ratio Lower Upper

128 100

129 28.1 9.4 14.0#

127 23.2 10.6 16.0#

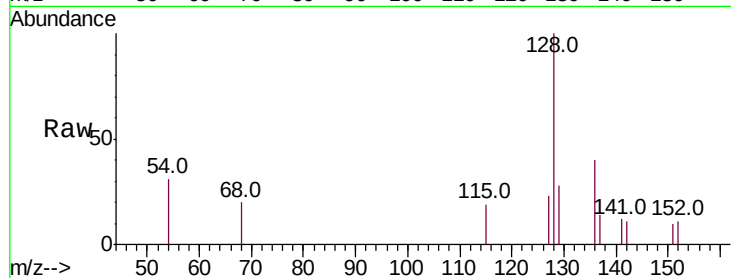

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

