

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
 Data File : BN006938.D
 Acq On : 19 Jul 2019 23:18
 Operator : HP/JU
 Sample : K3823-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A52L2

Manual Integrations
 APPROVED

mohammad
 7/22/2019 10:03:27 AM

Quant Time: Jul 20 00:52:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 23:29:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2442	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8645	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4367	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	8977m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	7114m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	6019m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	3639	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	8785m	0.33	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.40	128	1376	0.055	ng/ul#	Ovalue 79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071919\
Data File : BN006938.D
Acq On : 19 Jul 2019 23:18
Operator : HP/JU
Sample : K3823-09
Misc :
ALS Vial : 19 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A52L2

Manual Integrations
APPROVED

mohammad
7/22/2019 10:03:27 AM

Quant Time: Jul 20 00:52:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 23:29:55 2019
Response via : Initial Calibration

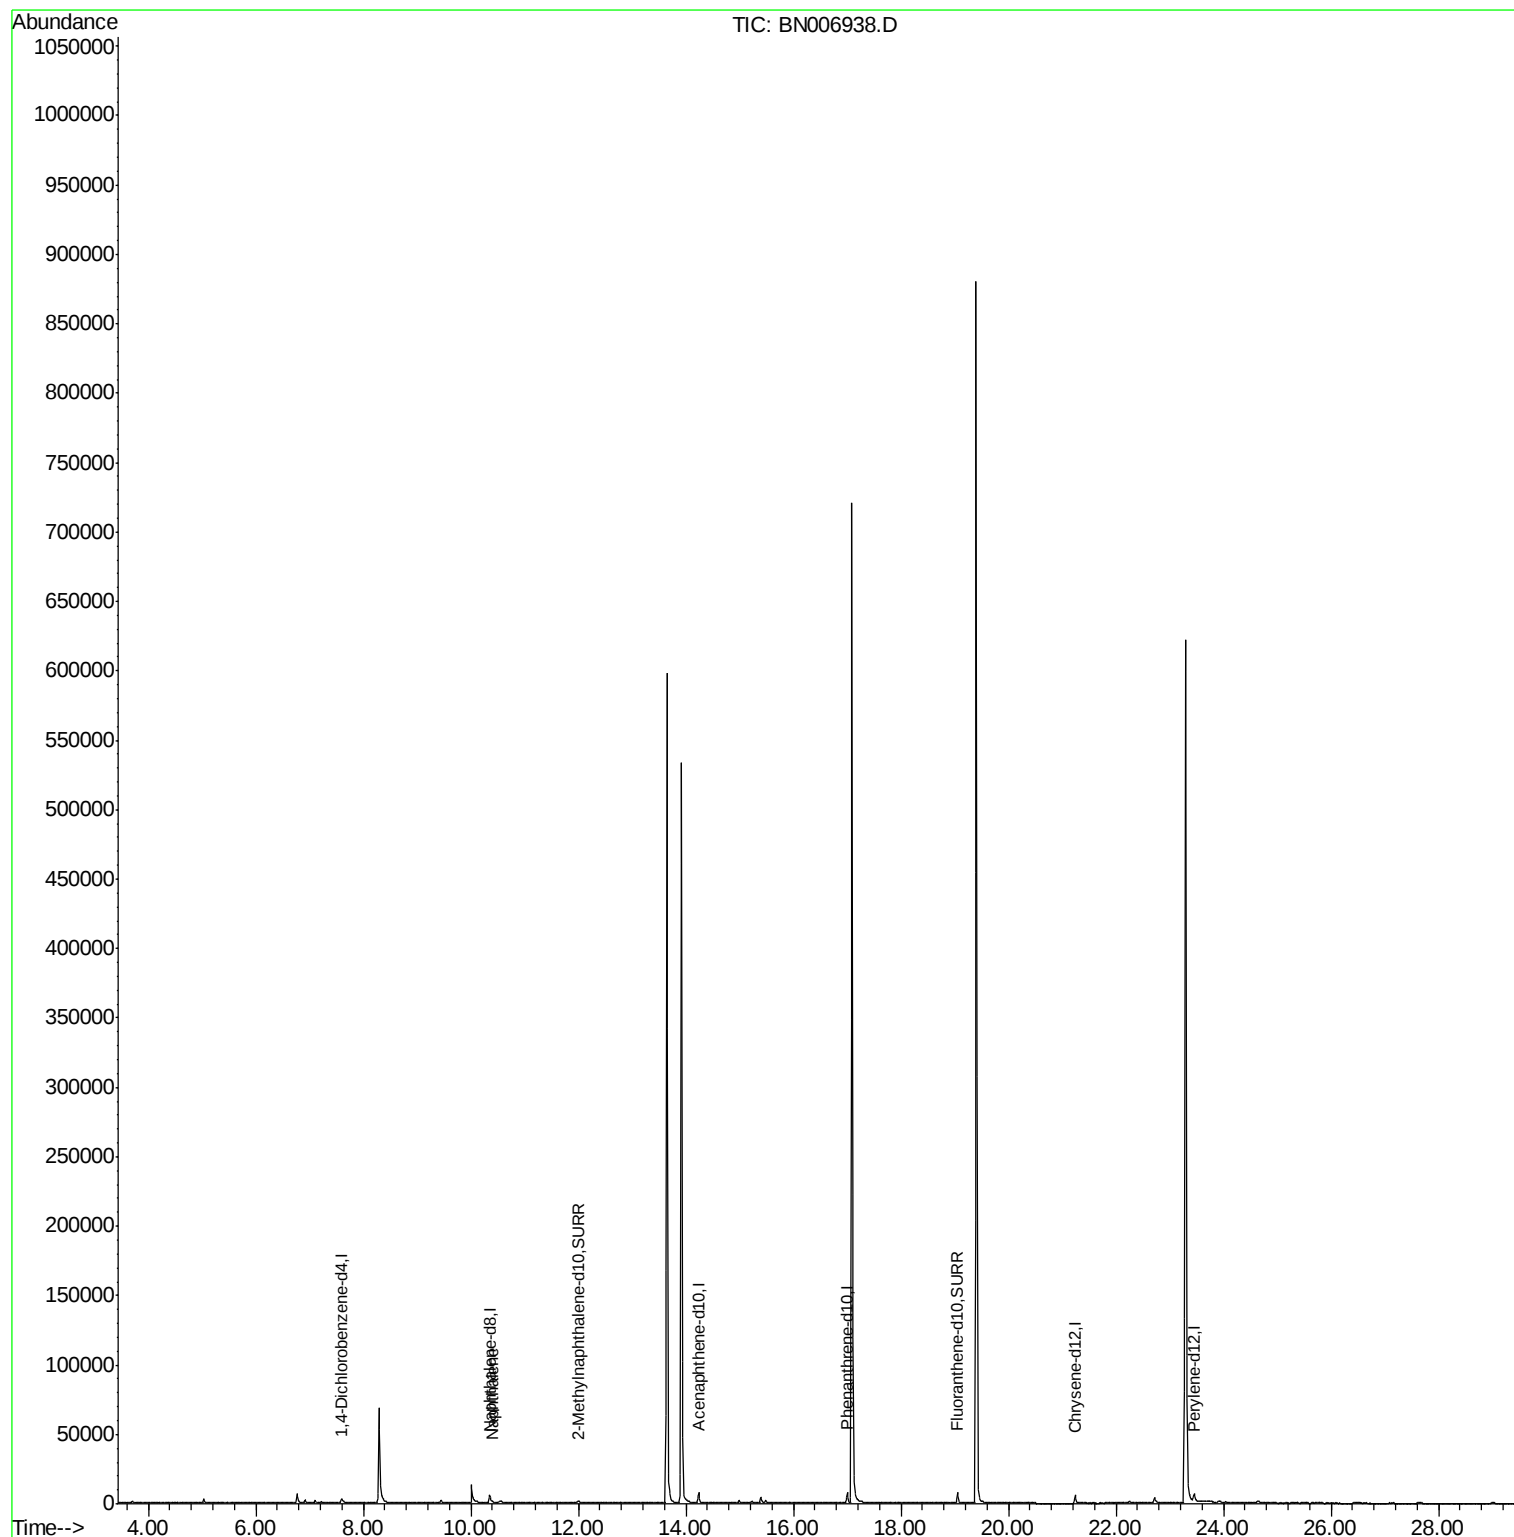

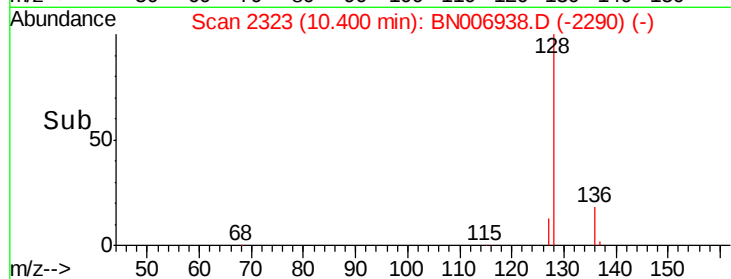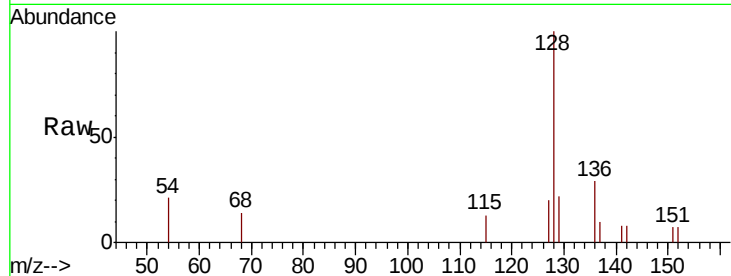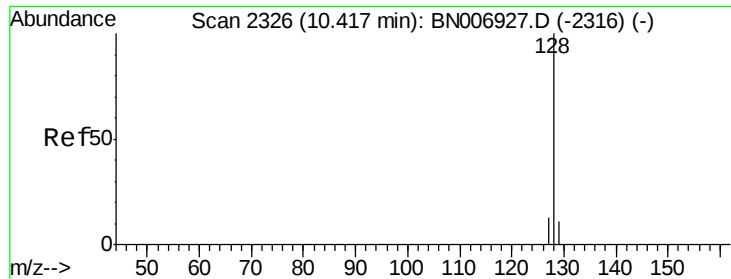

#3

Naphthalene

Concen: 0.055 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006938.D

Acq: 19 Jul 2019 23:18

Instrument :

BNA_N

ClientSampleId :

A52L2

Tot Ion:128 Resp: 1376

Ion Ratio Lower Upper

128 100

129 21.7 9.4 14.0#

127 19.8 10.6 16.0#

Manual Integrations

APPROVED

mohammad

7/22/2019 10:03:27 AM

