

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072018\
 Data File : BN002097.D
 Acq On : 20 Jul 2018 13:41
 Operator : JU/SJ
 Sample : J4039-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 20 23:56:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 20 23:55:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	268682	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	1239442	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	765231	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1734568	20.00	ng/ul	0.00
77) Chrysene-d12	21.28	240	1778530	20.00	ng/ul	0.00
85) Perylene-d12	23.52	264	1639658	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	31465	5.28	ng/uL	0.00
5) Phenol-d5	6.88	99	158214	6.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	443434	28.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	466739	23.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	306459	15.04	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	309641	30.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	354145	30.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	580726	27.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	5885	0.24	ng/ul	0.01
43) Dimethylphthalate-d6	13.75	166	2041826	31.48	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	2217983	27.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	71900	5.80	ng/ul	0.00
57) Fluorene-d10	15.33	176	1755607	31.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	327436	28.98	ng/ul	0.00
70) Anthracene-d10	17.18	188	2687589	31.78	ng/ul	0.00
78) Pyrene-d10	19.48	212	3055391	33.05	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	2992824	33.80	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.79	163	297979	4.690	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072018\
Data File : BN002097.D
Acq On : 20 Jul 2018 13:41
Operator : JU/SJ
Sample : J4039-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 20 23:56:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 20 23:55:09 2018
Response via : Initial Calibration

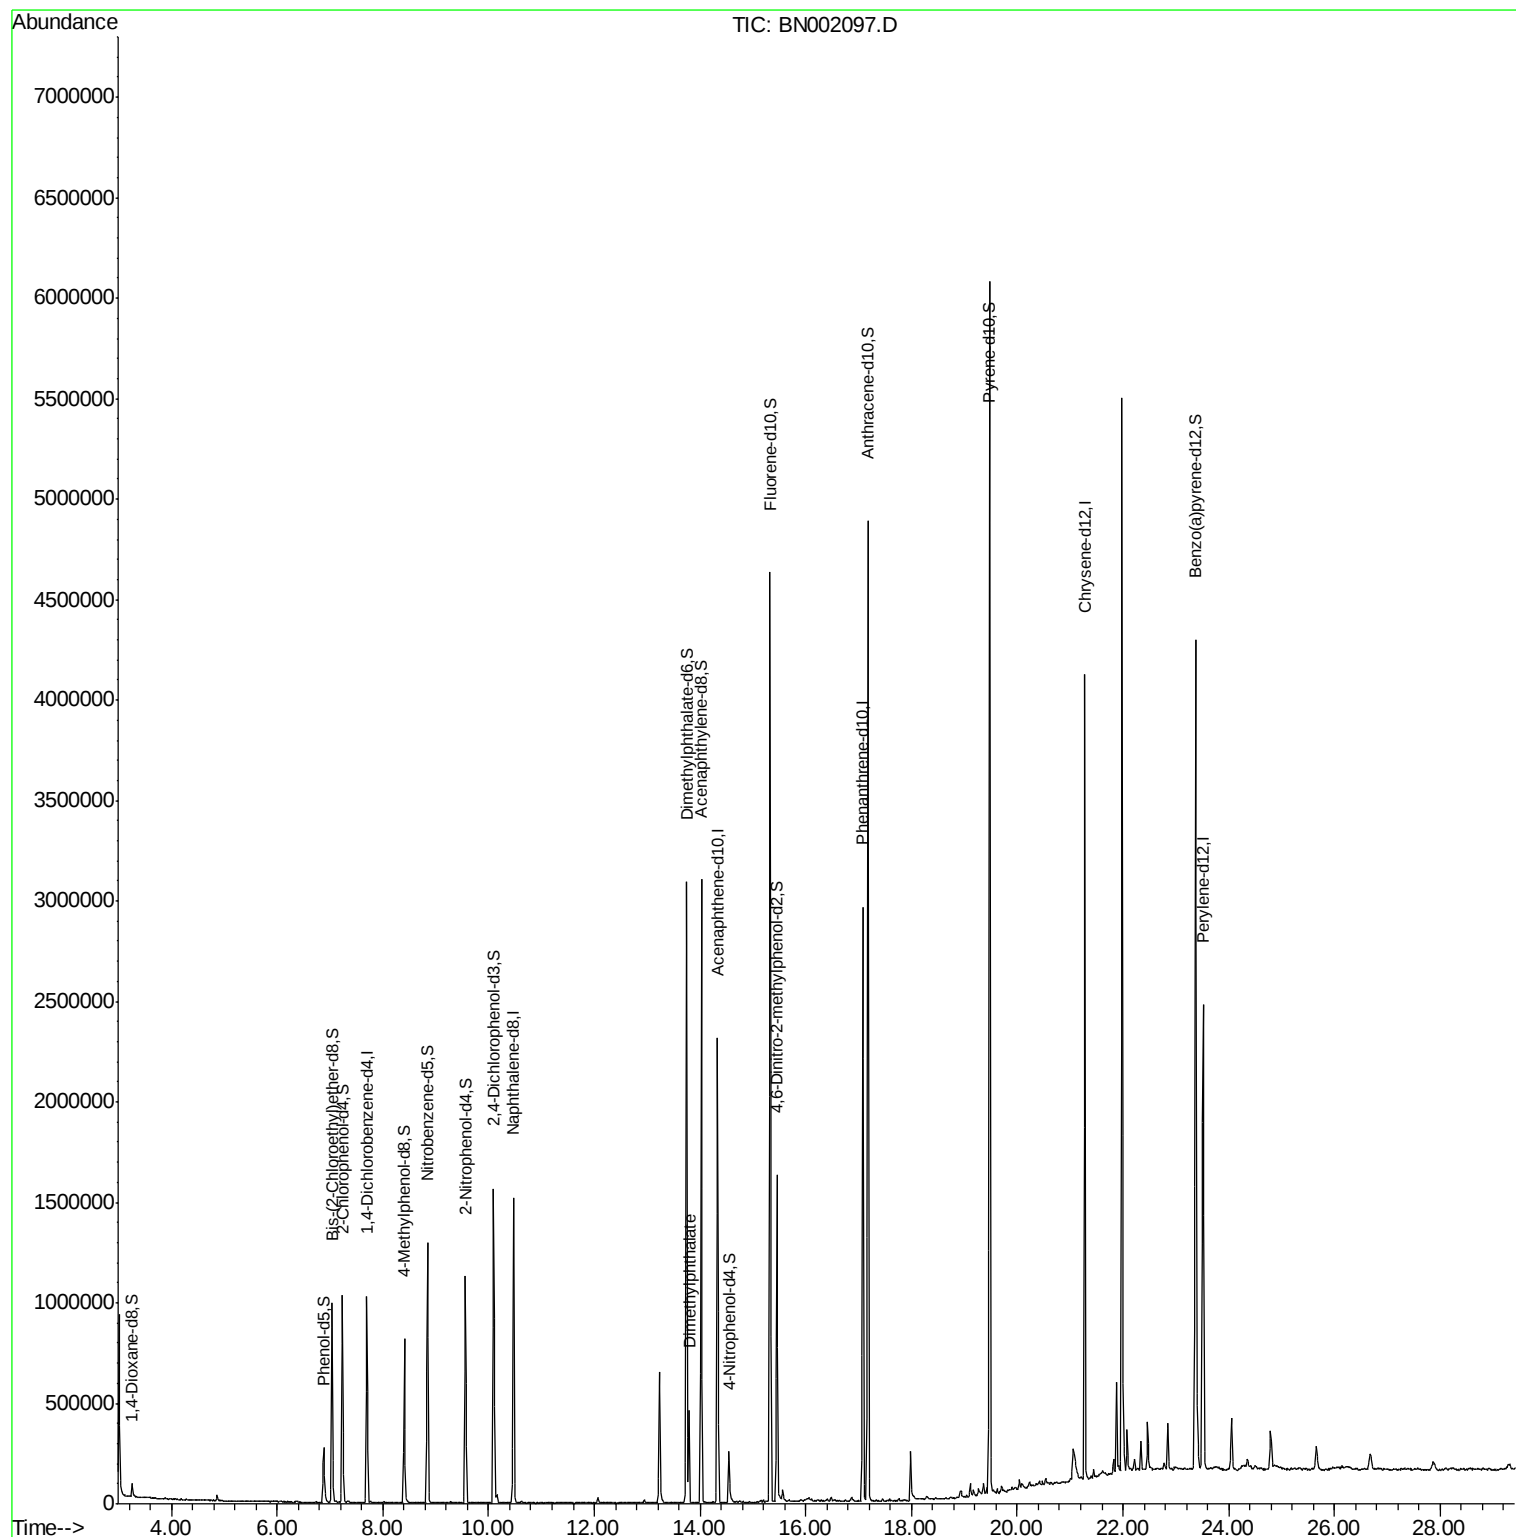

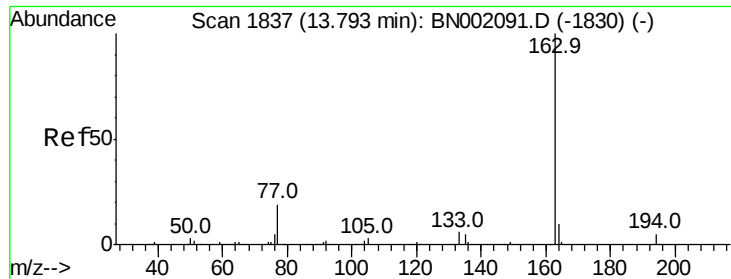

#44

Dimethylphthalate

Concen: 4.690 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BN002097.D

Acq: 20 Jul 2018 13:41

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 297979

Ion Ratio Lower Upper

163 100

194 4.5 3.2 4.8

164 9.4 7.8 11.8

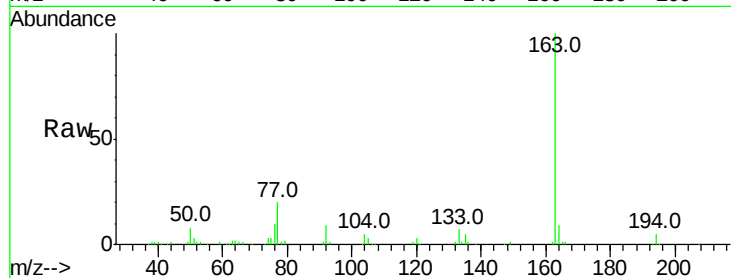

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

