




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026621.D
 Acq On : 21 Jul 2023 10:13
 Operator : MA/JU
 Sample : PB154070BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Quant Time: Jul 22 00:26:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

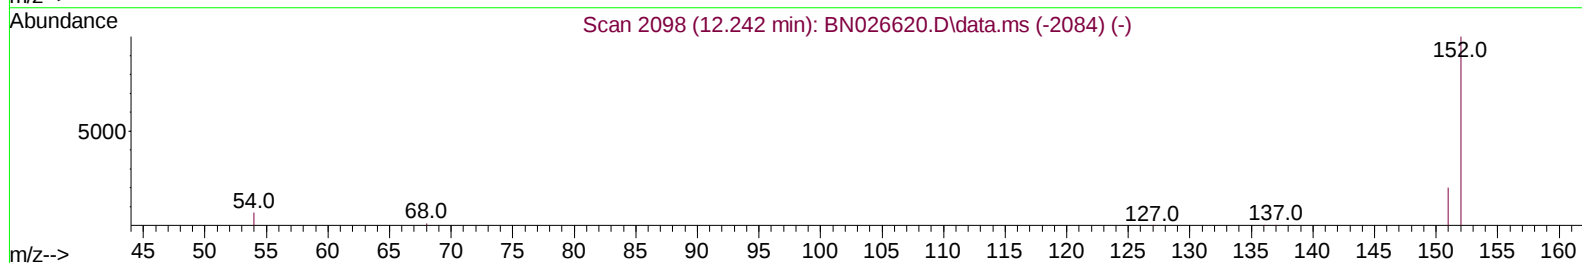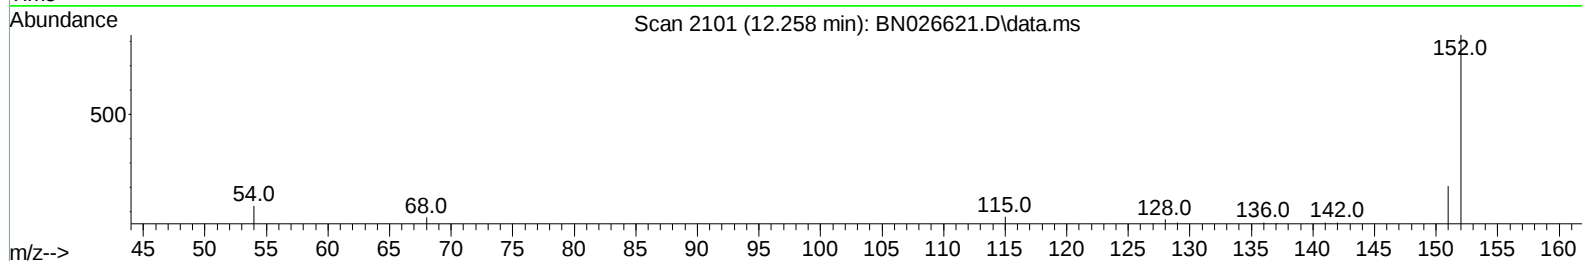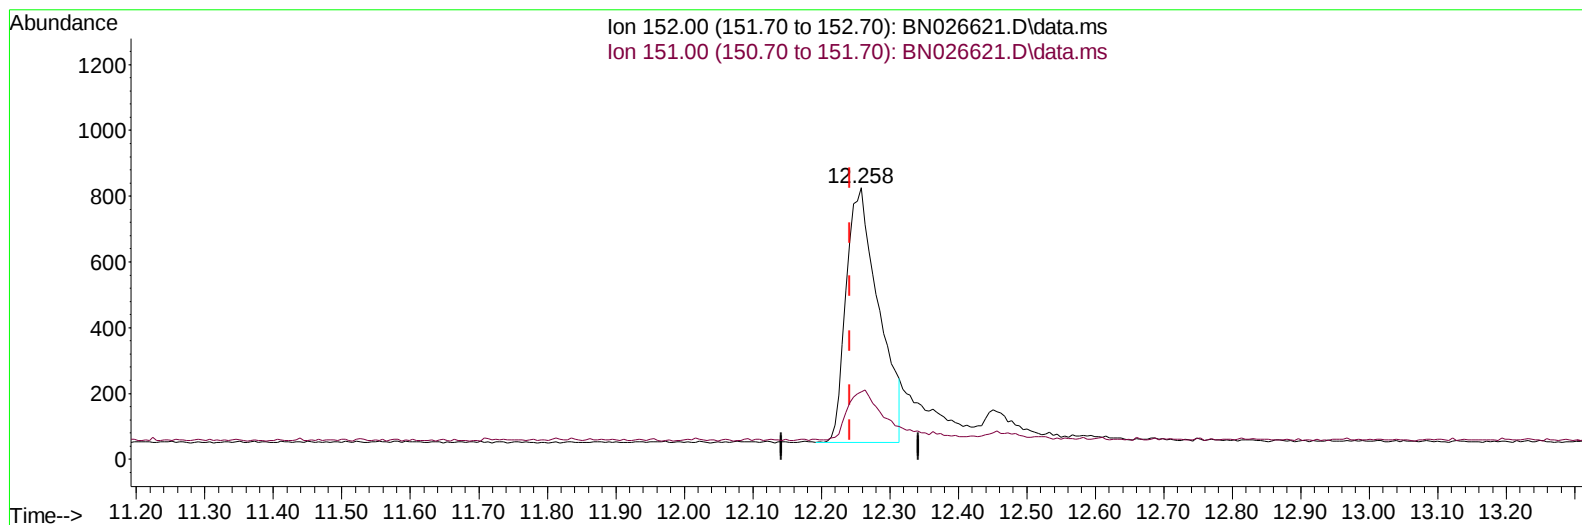

TIC: BN026621.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.258min (+ 0.016) 0.31 ng/ul

response 2544

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	20.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026621.D
 Acq On : 21 Jul 2023 10:13
 Operator : MA/JU
 Sample : PB154070BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Quant Time: Jul 21 14:03:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 20 22:32:26 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

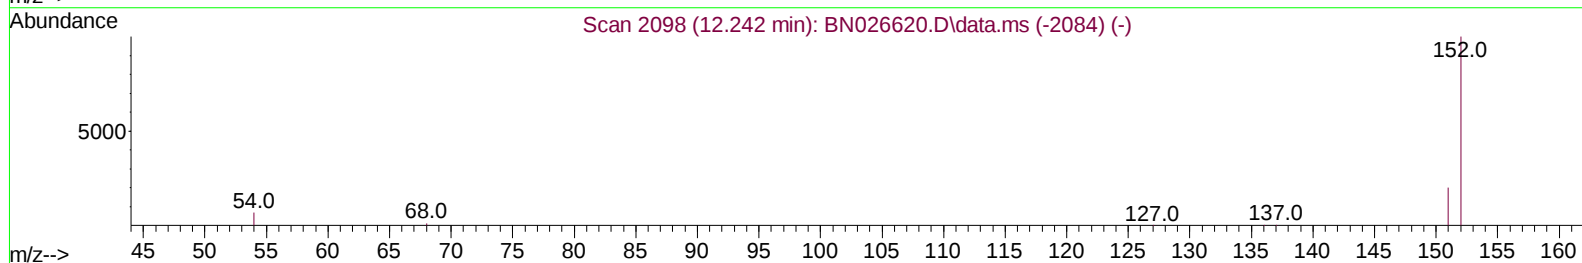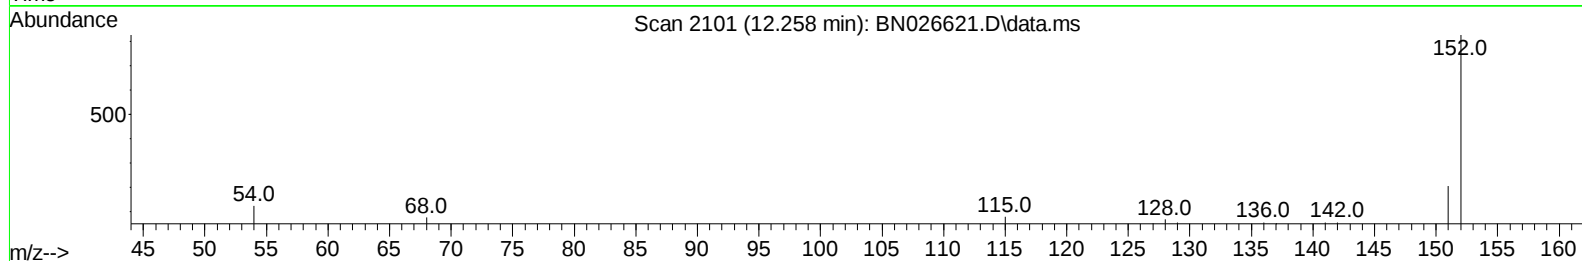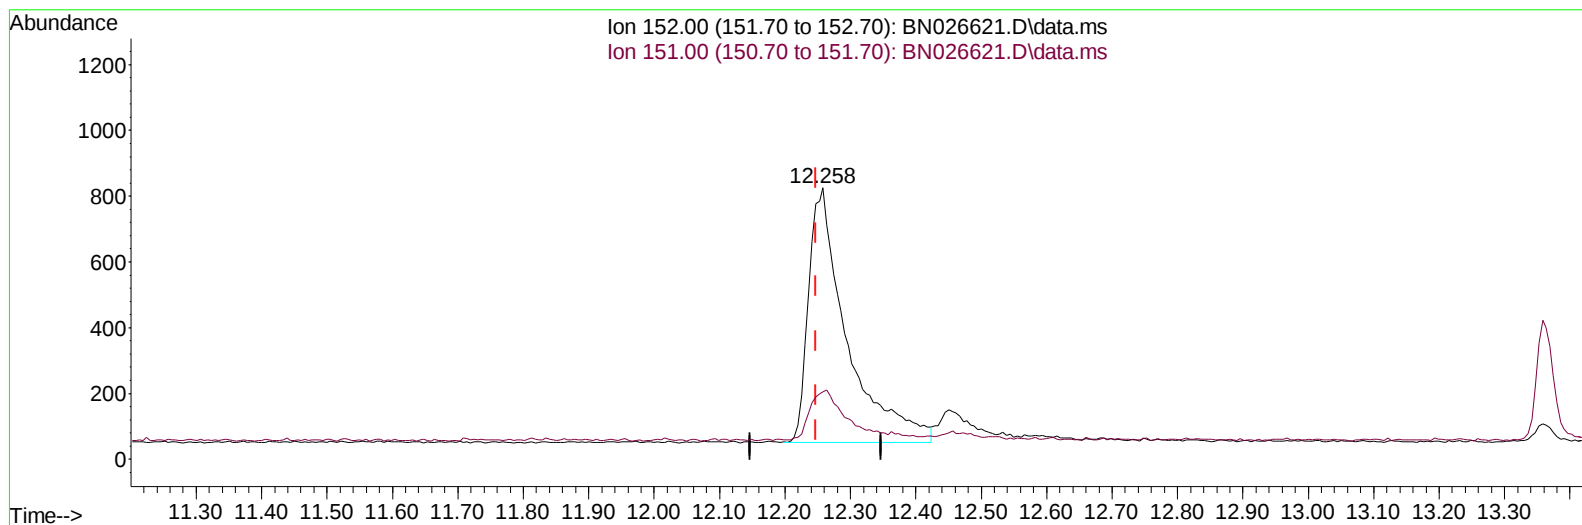

TIC: BN026621.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.258min (+ 0.011) 0.39 ng/ul m

response 3138

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	16.35#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026621.D
 Acq On : 21 Jul 2023 10:13
 Operator : MA/JU
 Sample : PB154070BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

Quant Time: Jul 21 14:03:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 20 22:32:26 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.840	152		1775	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.636	136		5974	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.472	164		3934	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.219	188		9104	0.400	ng/ul	0.00
17) Chrysene-d12	21.431	240		6757	0.400	ng/ul	0.01
23) Perylene-d12	23.796	264		8279	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.199	96		13515	5.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152		3138m	0.386	ng/ul	0.01
18) Fluoranthene-d10	19.255	212		9190	0.392	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026621.D
Acq On : 21 Jul 2023 10:13
Operator : MA/JU
Sample : PB154070BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Quant Time: Jul 21 14:03:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 20 22:32:26 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

