




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026633.D
 Acq On : 21 Jul 2023 18:17
 Operator : MA/JU
 Sample : PB154137BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK137

Manual IntegrationsAPPROVED

Quant Time: Jul 22 00:48:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

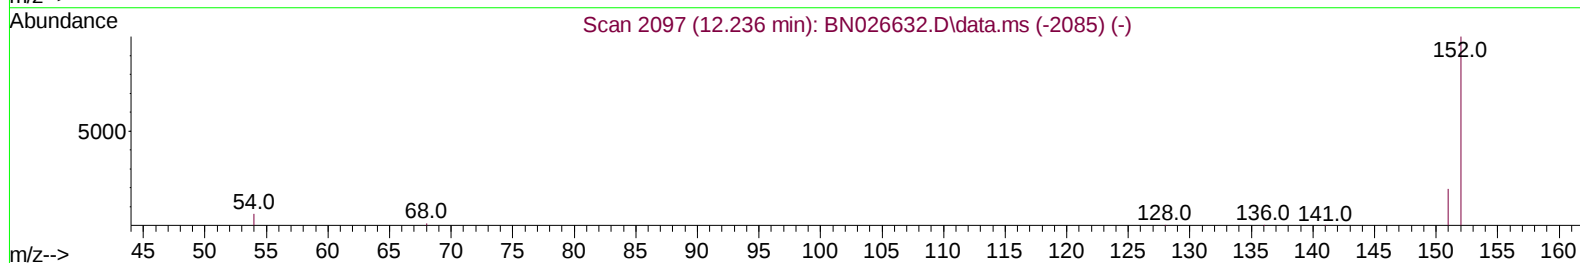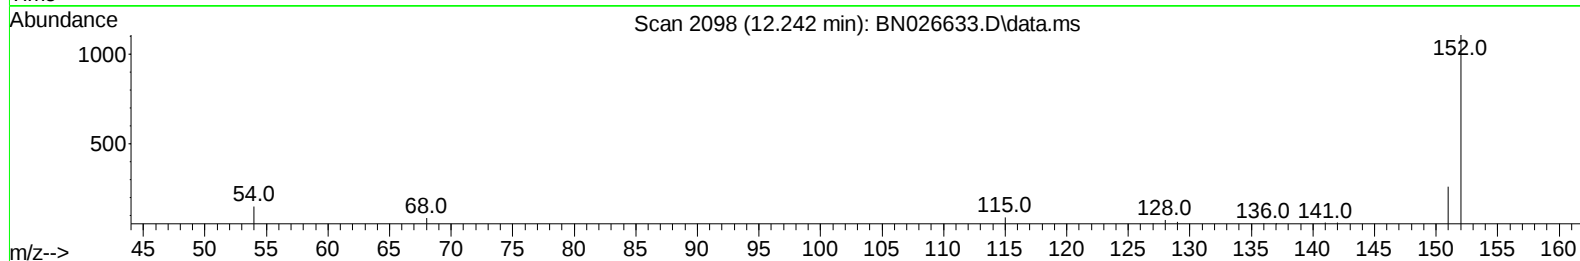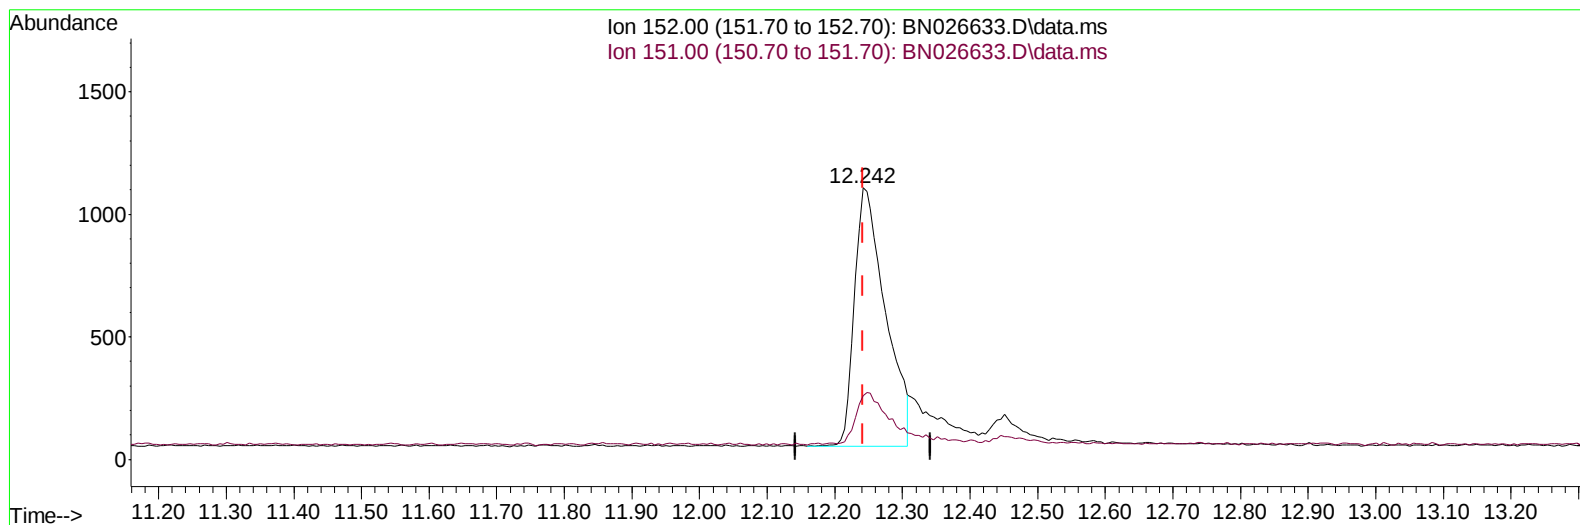

TIC: BN026633.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.242min (-0.000) 0.31 ng/u1

response 3352

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	20.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026633.D
 Acq On : 21 Jul 2023 18:17
 Operator : MA/JU
 Sample : PB154137BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK137

Manual IntegrationsAPPROVED

Quant Time: Jul 22 00:48:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

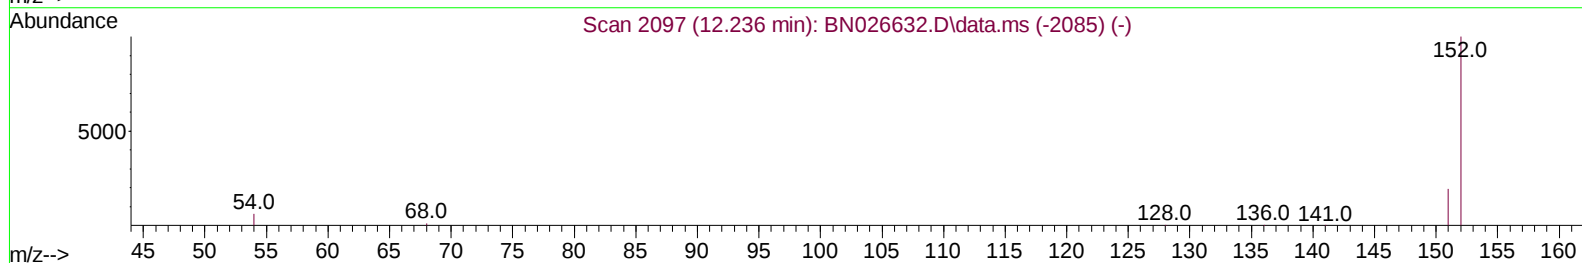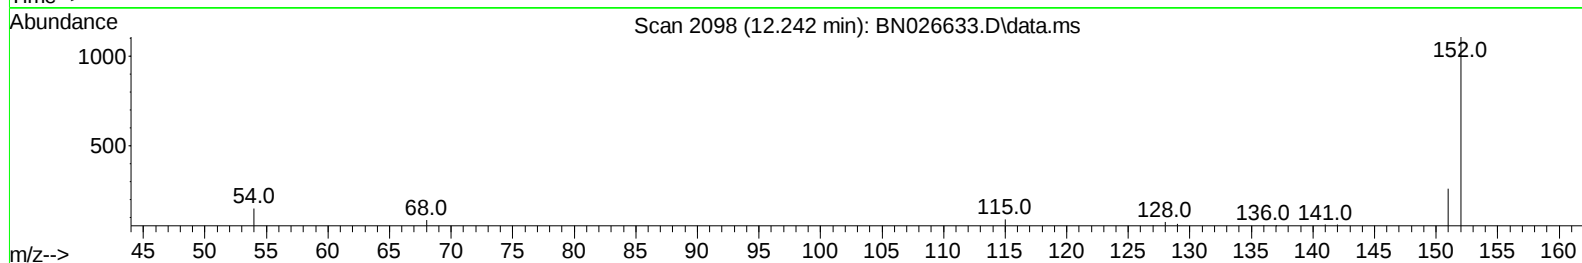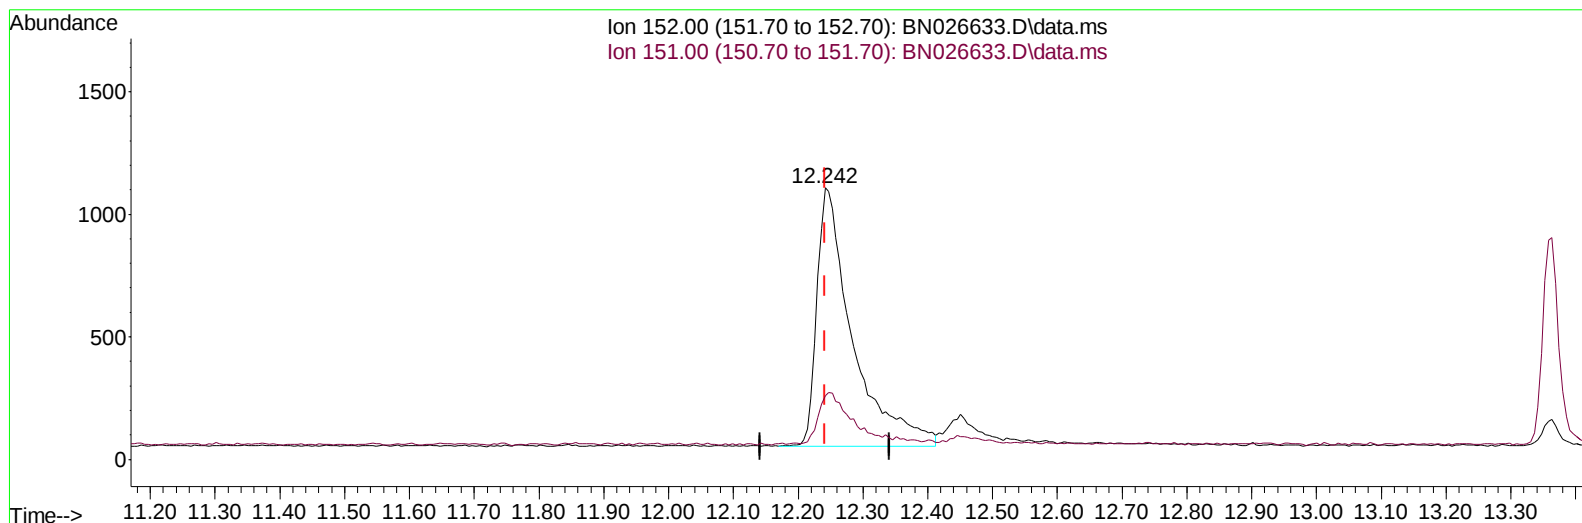

TIC: BN026633.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.242min (-0.000) 0.37 ng/ul m

response 4019

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	16.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026633.D
 Acq On : 21 Jul 2023 18:17
 Operator : MA/JU
 Sample : PB154137BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK137

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

Quant Time: Jul 22 00:48:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.836	152		2281	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.630	136		8000	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.472	164		5094	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188		11286	0.400	ng/ul	0.00
17) Chrysene-d12	21.419	240		7833	0.400	ng/ul	0.00
23) Perylene-d12	23.784	264		9099	0.400	ng/ul	#-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.199	96		15874	5.284	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.242	152		4019m	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.250	212		10825	0.399	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026633.D
Acq On : 21 Jul 2023 18:17
Operator : MA/JU
Sample : PB154137BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK137

Manual IntegrationsAPPROVED

Quant Time: Jul 22 00:48:36 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

