

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026613.D
 Acq On : 21 Jul 2023 04:44
 Operator : MA/JU
 Sample : 03472-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46Q4

Quant Time: Jul 21 05:48:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 20 22:32:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.836	152	1960	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.630	136	6545	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.472	164	4164	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	9977	0.400	ng/ul	0.00
17) Chrysene-d12	21.416	240	10014	0.400	ng/ul	0.00
23) Perylene-d12	23.784	264	10929	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	6914	2.678	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.231	152	3529	0.397	ng/ul	-0.02
18) Fluoranthene-d10	19.250	212	10868	0.313	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.278	202	1374	0.029	ng/ul#	67
21) Benzo(a)anthracene	21.399	228	783	0.021	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026613.D
Acq On : 21 Jul 2023 04:44
Operator : MA/JU
Sample : 03472-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A46Q4


Quant Time: Jul 21 05:48:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 20 22:32:26 2023
Response via : Initial Calibration

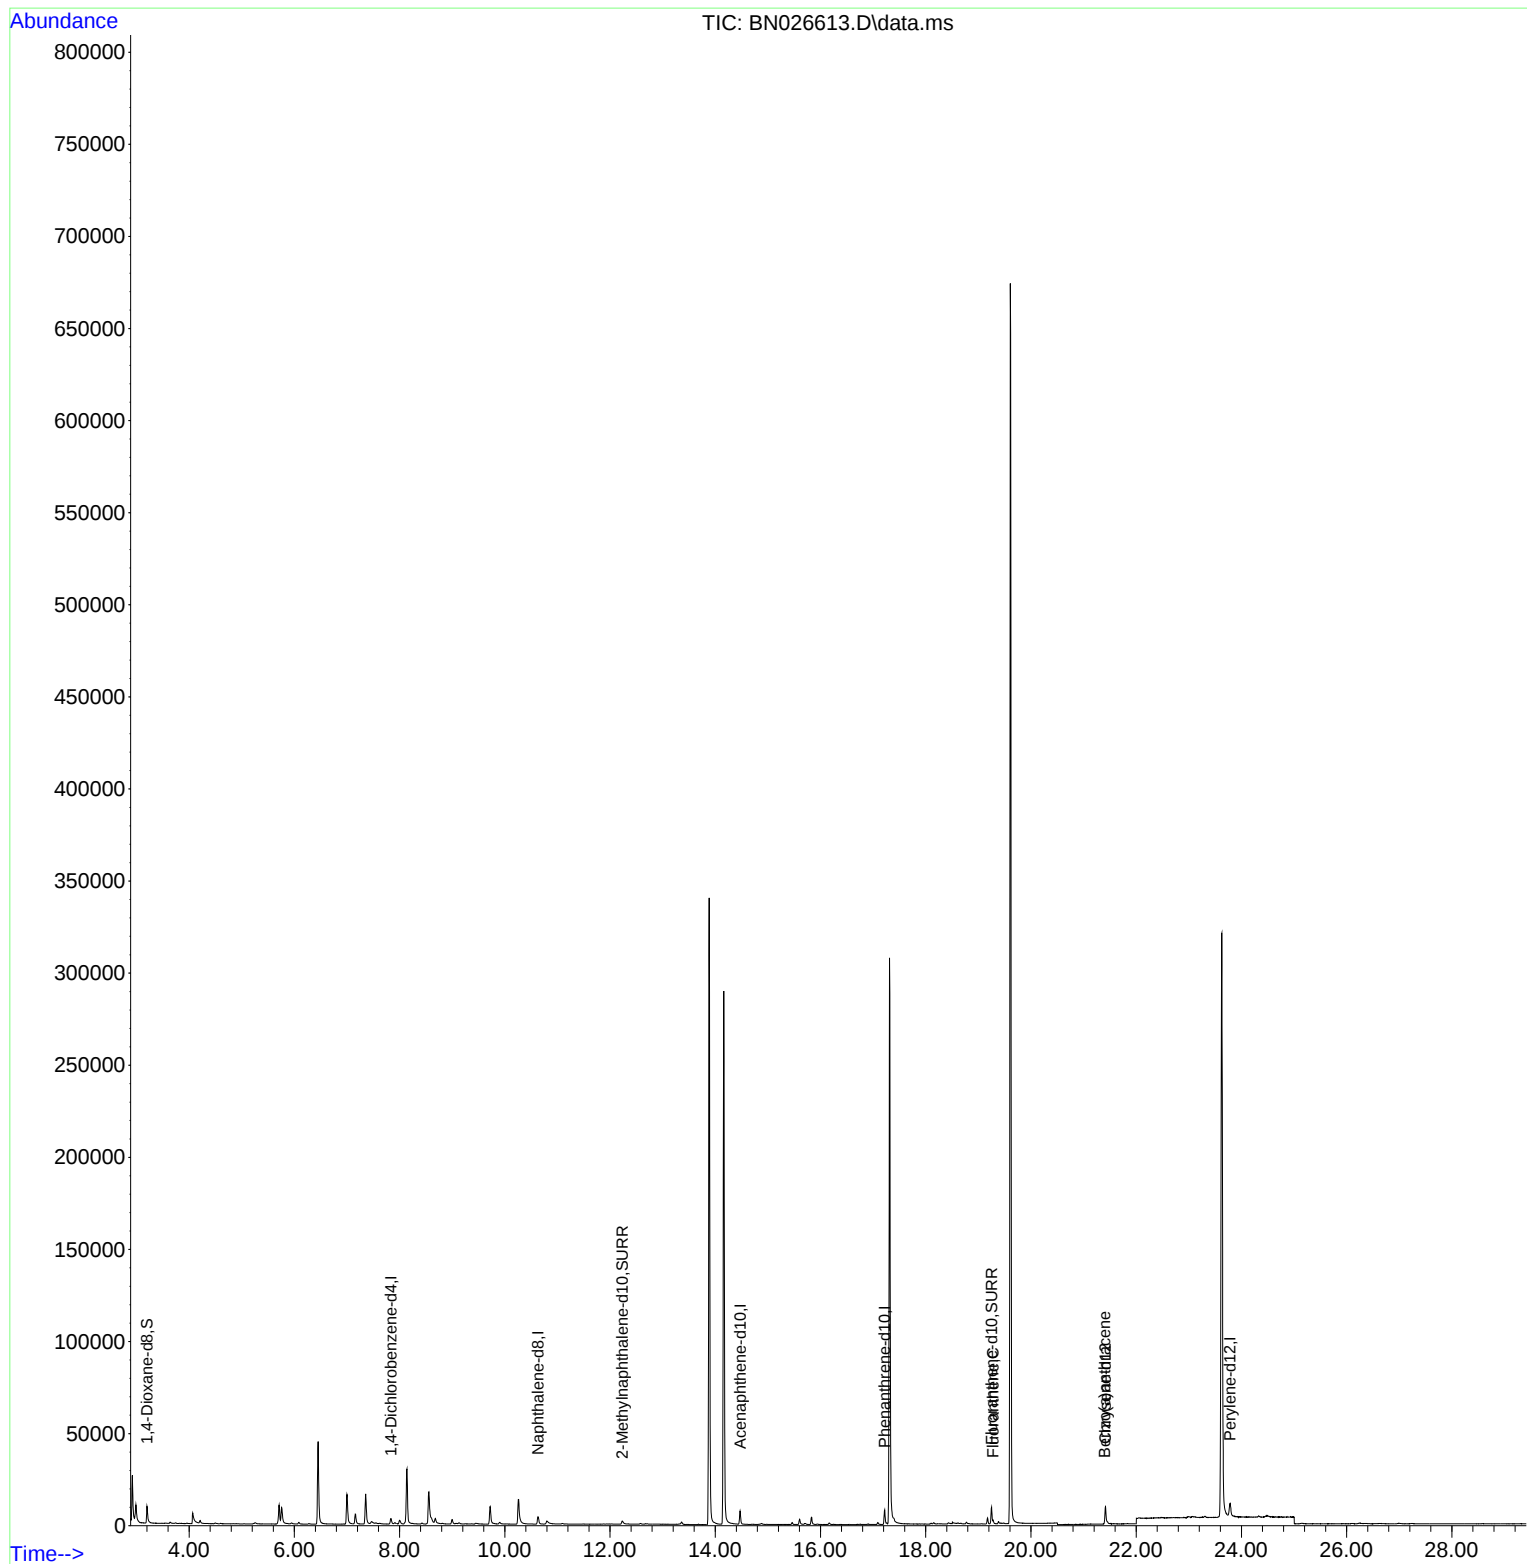



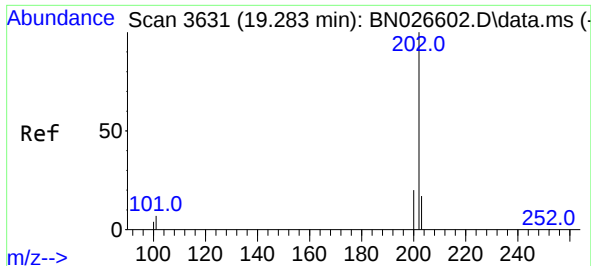


#19
Fluoranthene
Concen: 0.029 ng/ul
RT: 19.278 min Scan# 3630
Delta R.T. -0.005 min
Lab File: BN026613.D
Acq: 21 Jul 2023 04:44

Instrument :
BNA_N
ClientSampleId :
A46Q4

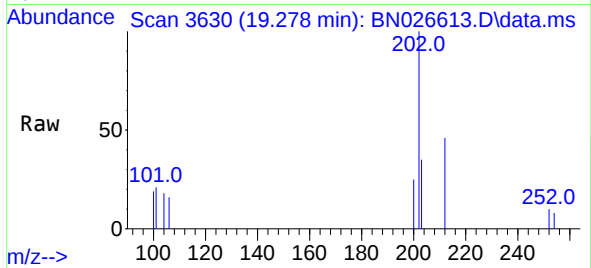

Tgt Ion:202 Resp: 1374
Ion Ratio Lower Upper
202 100
101 20.8 7.0 10.4#
100 18.8 6.0 9.0#

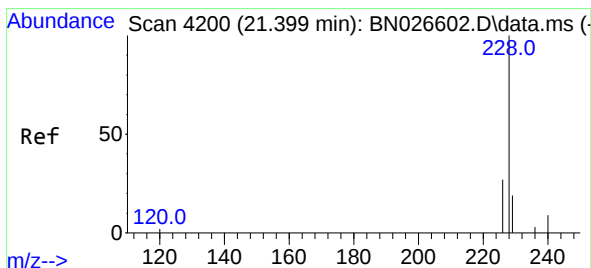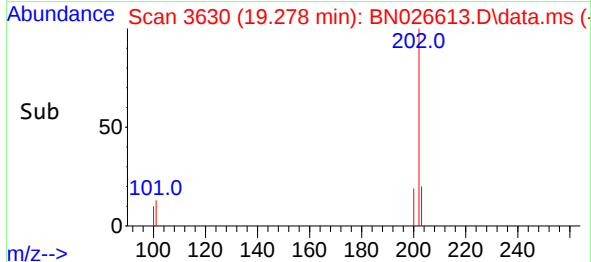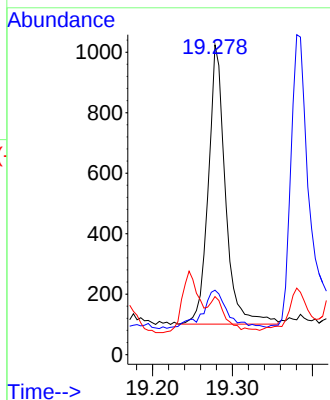

#21
Benzo(a)anthracene
Concen: 0.021 ng/ul
RT: 21.399 min Scan# 4200
Delta R.T. -0.000 min
Lab File: BN026613.D
Acq: 21 Jul 2023 04:44

Tgt Ion:228 Resp: 783
Ion Ratio Lower Upper
228 100
229 42.6 16.7 25.1#
226 45.5 23.5 35.3#

