

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026639.D
 Acq On : 21 Jul 2023 22:00
 Operator : MA/JU
 Sample : 03536-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW63

Quant Time: Jul 22 01:10:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	3762	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.630	136	10893	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.471	164	6446	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	13823	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.410	240	9423	0.400	ng/ul	#-0.01
23) Perylene-d12	23.784	264	8934	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	7521	1.518	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	5156	0.348	ng/ul	-0.02
18) Fluoranthene-d10	19.250	212	11358	0.348	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.224	88	1149	0.245	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026639.D
Acq On : 21 Jul 2023 22:00
Operator : MA/JU
Sample : 03536-09
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW63


Quant Time: Jul 22 01:10:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

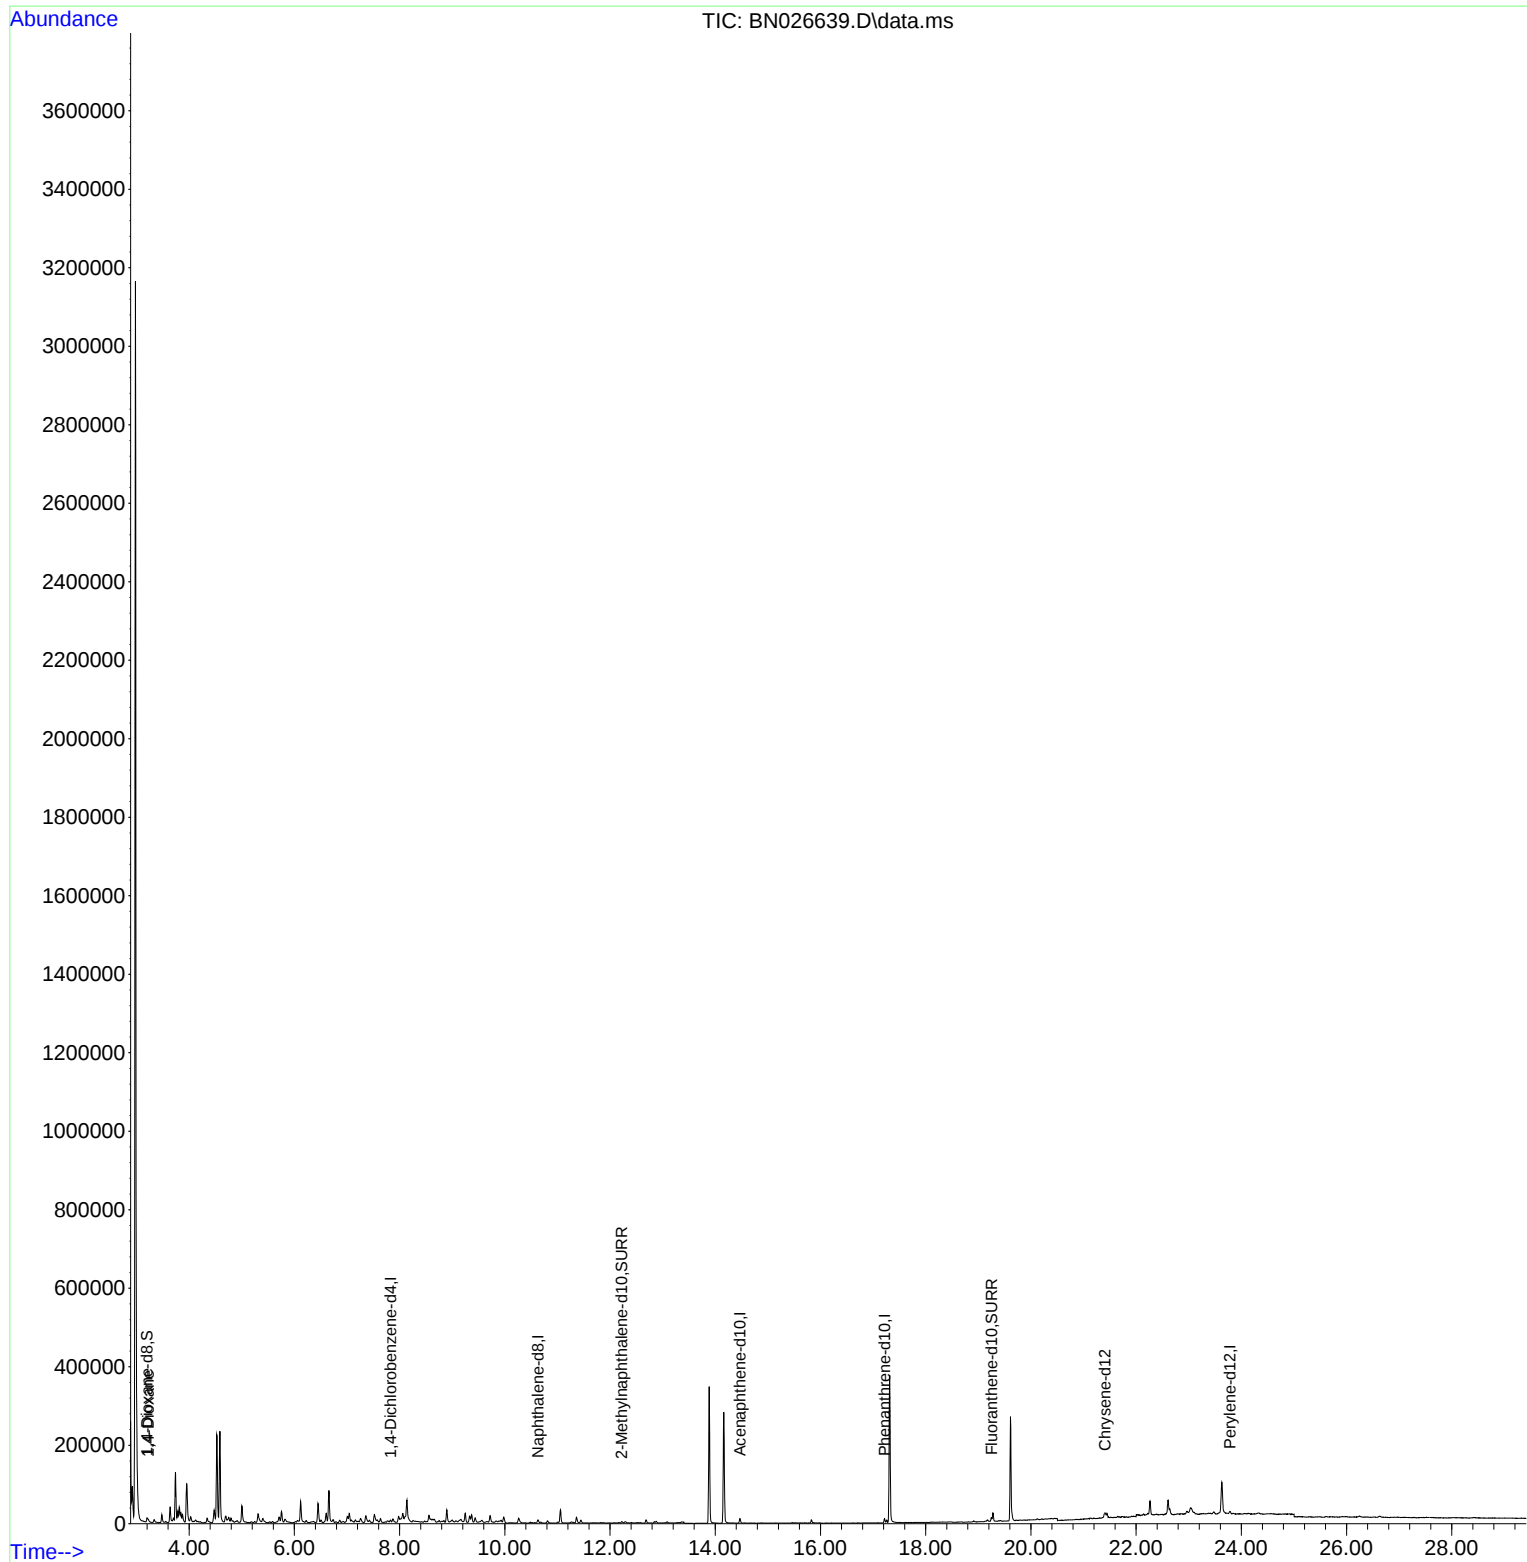

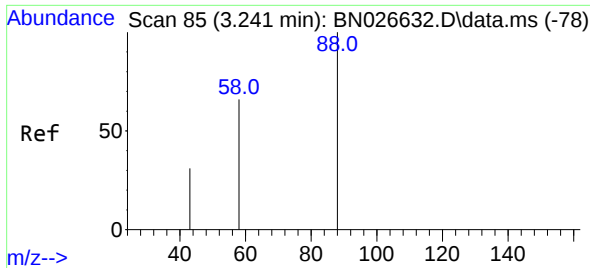

#2
 1,4-Dioxane
 Concen: 0.245 ng/ul
 RT: 3.224 min Scan# 81
 Delta R.T. -0.017 min
 Lab File: BN026639.D
 Acq: 21 Jul 2023 22:00

Instrument :
 BNA_N
 ClientSampleId :
 YBW63

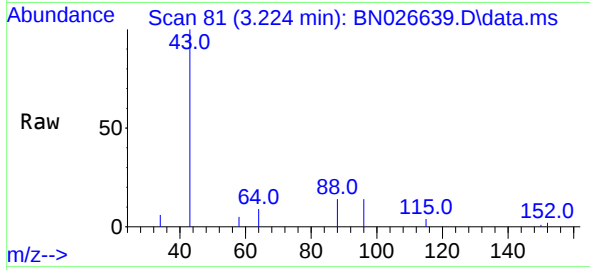

Tgt Ion: 88 Resp: 1149

Ion	Ratio	Lower	Upper
88	100		
43	738.3	33.0	49.6#
58	33.5	41.7	62.5#

