

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026641.D
 Acq On : 21 Jul 2023 23:16
 Operator : MA/JU
 Sample : 03536-05
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW59

Quant Time: Jul 22 01:12:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.832	152	3750	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.636	136	10774	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.472	164	6282	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	12602	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.411	240	8765	0.400	ng/ul	#-0.01
23) Perylene-d12	23.781	264	8945	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.203	96	9218	1.866	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	5564	0.380	ng/ul	-0.02
18) Fluoranthene-d10	19.250	212	12942	0.426	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.224	88	912	0.195	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026641.D
Acq On : 21 Jul 2023 23:16
Operator : MA/JU
Sample : 03536-05
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW59


Quant Time: Jul 22 01:12:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

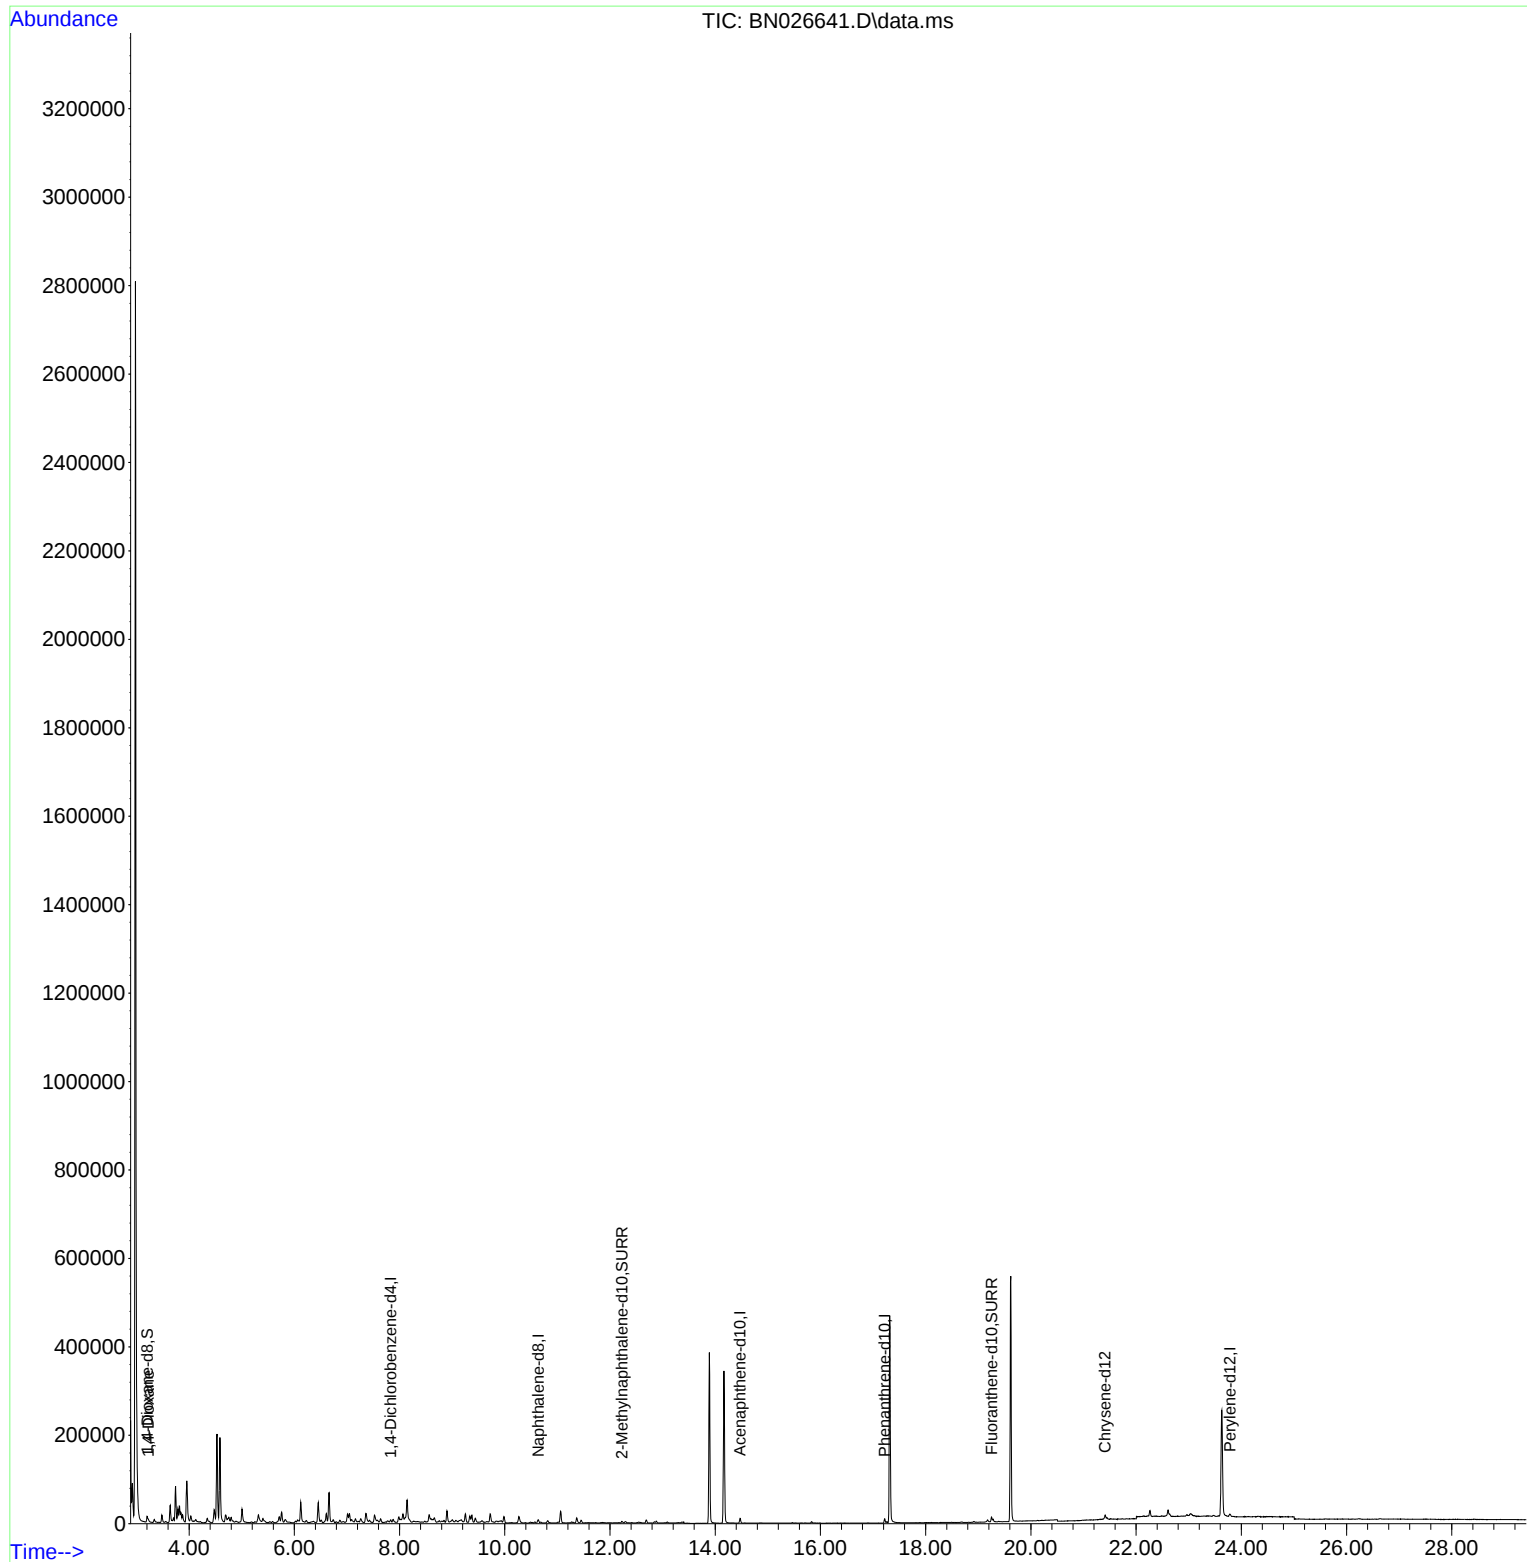

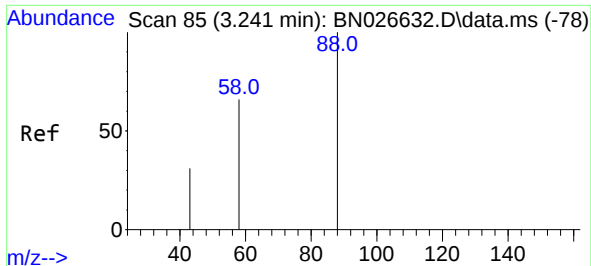

#2
1,4-Dioxane
Concen: 0.195 ng/ul
RT: 3.224 min Scan# 81
Delta R.T. -0.017 min
Lab File: BN026641.D
Acq: 21 Jul 2023 23:16

Instrument :
BNA_N
ClientSampleId :
YBW59

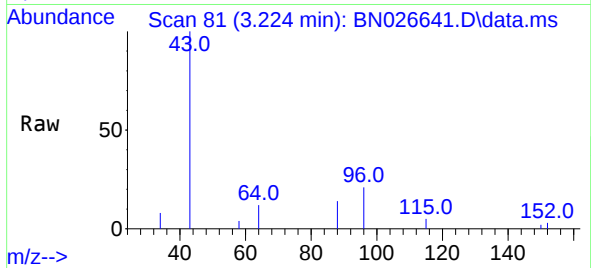

Tgt Ion: 88 Resp: 912
Ion Ratio Lower Upper
88 100
43 725.9 33.0 49.6#
58 30.8 41.7 62.5#

