

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026642.D
 Acq On : 21 Jul 2023 23:54
 Operator : MA/JU
 Sample : 03536-04
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW58

Quant Time: Jul 22 01:13:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.832	152	3625	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.636	136	11461	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.476	164	6459	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.223	188	13318	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.413	240	8100	0.400	ng/ul	#-0.01
23) Perylene-d12	23.784	264	8551	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.203	96	3225	0.676	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	3443	0.221	ng/ul	-0.02
18) Fluoranthene-d10	19.255	212	6943	0.247	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.224	88	968	0.214	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026642.D
Acq On : 21 Jul 2023 23:54
Operator : MA/JU
Sample : 03536-04
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW58


Quant Time: Jul 22 01:13:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

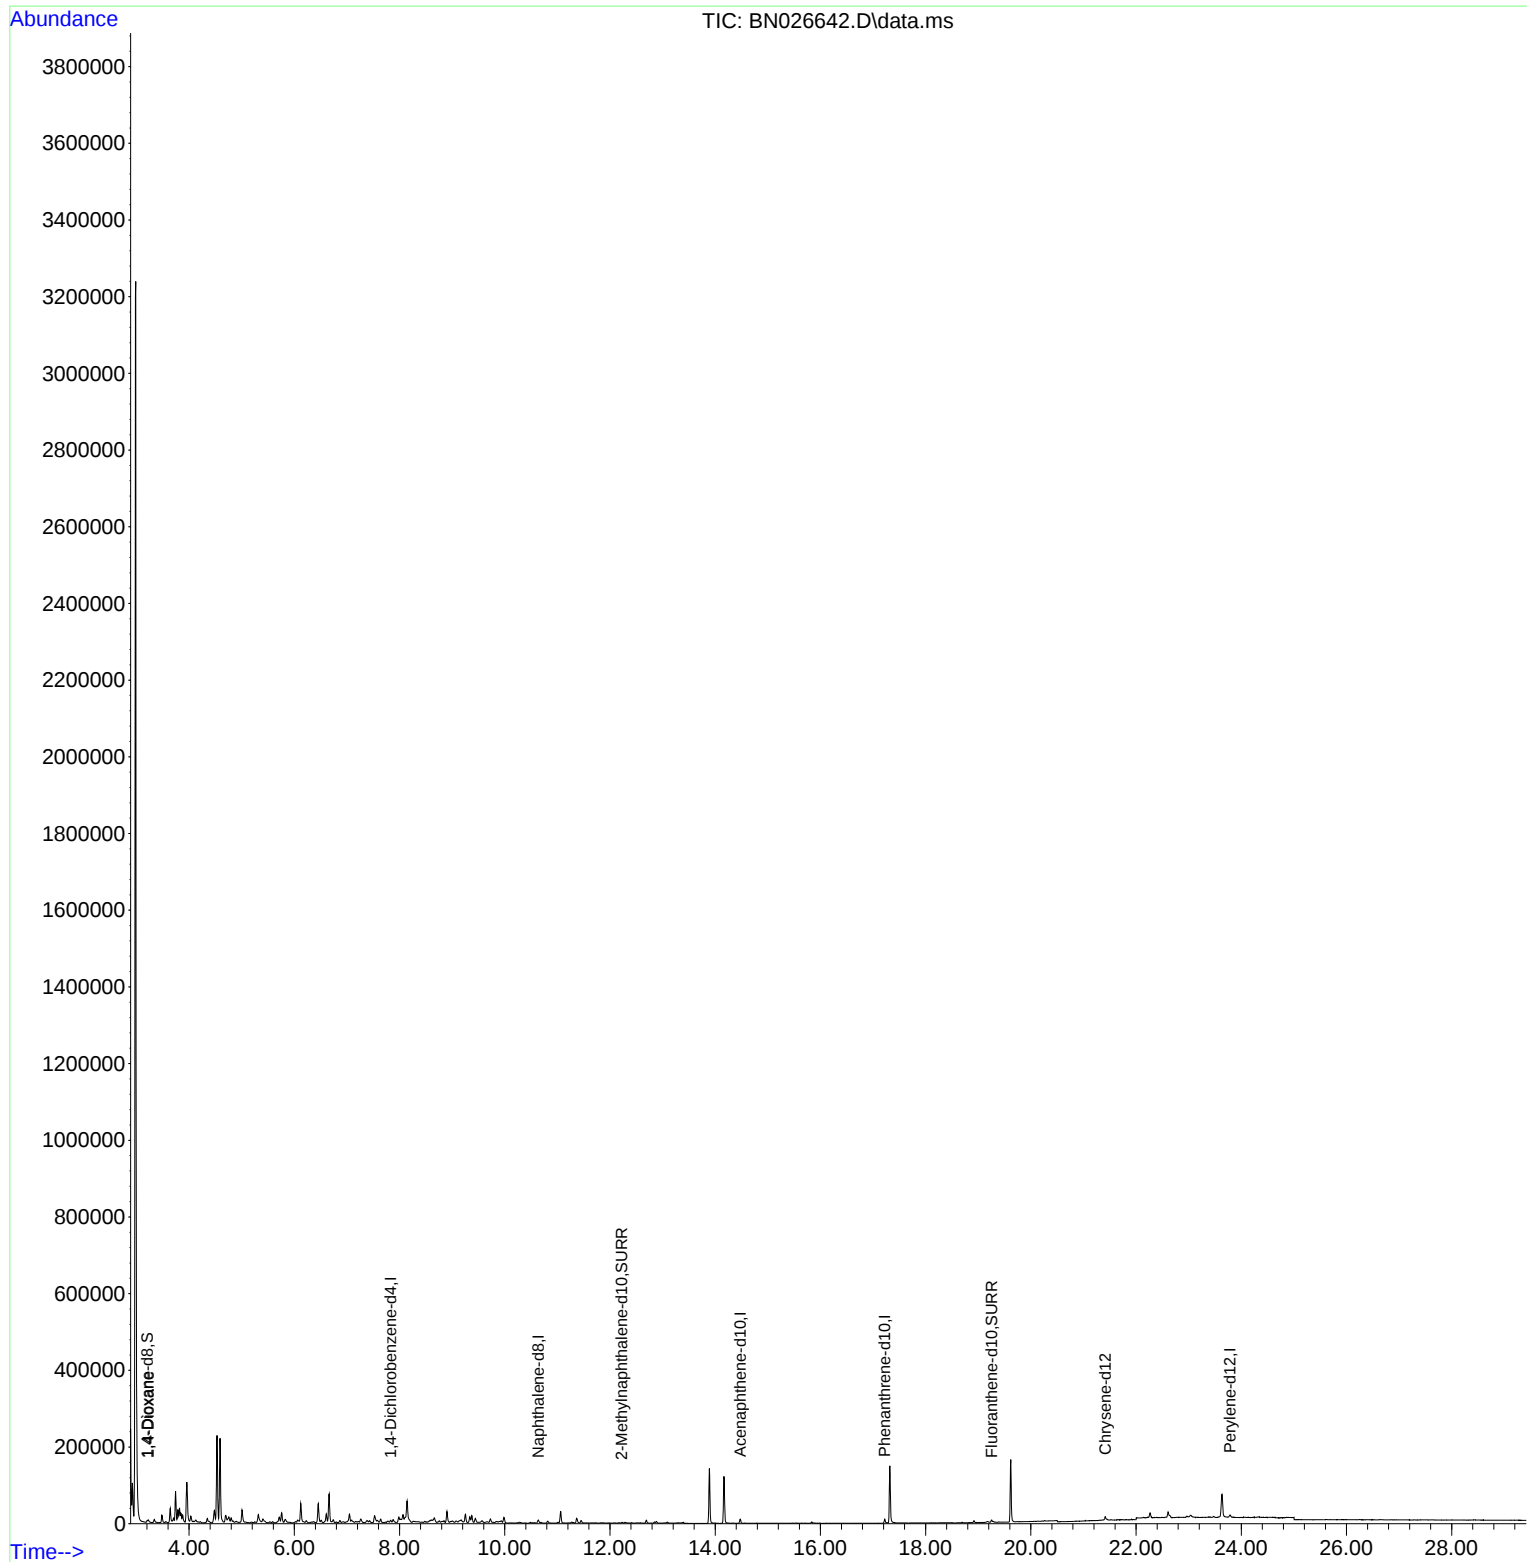


Abundance Scan 85 (3.241 min): BN026632.D\data.ms (-78)

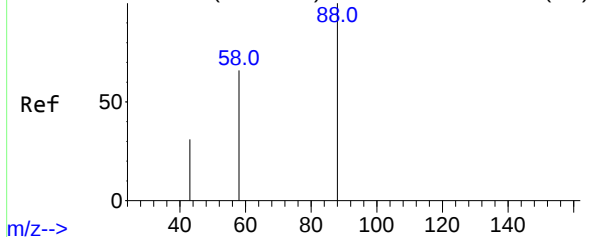

Abundance Scan 81 (3.224 min): BN026642.D\data.ms

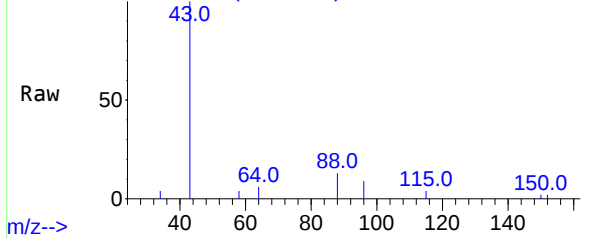

Abundance Scan 81 (3.224 min): BN026642.D\data.ms (-73)

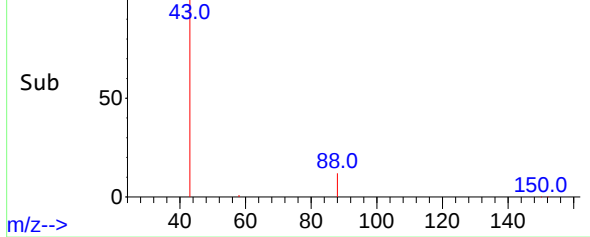

#2
1,4-Dioxane
Concen: 0.214 ng/ul
RT: 3.224 min Scan# 81
Delta R.T. -0.017 min
Lab File: BN026642.D
Acq: 21 Jul 2023 23:54

Instrument :
BNA_N
ClientSampleId :
YBW58

Tgt Ion: 88 Resp: 968
Ion Ratio Lower Upper
88 100
43 755.4 33.0 49.6#
58 29.6 41.7 62.5#

