

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026643.D
 Acq On : 22 Jul 2023 00:32
 Operator : MA/JU
 Sample : 03536-07
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW61

Quant Time: Jul 22 01:15:21 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.832	152	3922	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.636	136	11705	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.476	164	5708	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.223	188	13779	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.419	240	8630	0.400	ng/ul	# 0.00
23) Perylene-d12	23.796	264	8620	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.203	96	6966	1.349	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	3968	0.249	ng/ul	-0.02
18) Fluoranthene-d10	19.255	212	9854	0.329	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.224	88	1215	0.249	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026643.D
Acq On : 22 Jul 2023 00:32
Operator : MA/JU
Sample : 03536-07
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW61

Quant Time: Jul 22 01:15:21 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

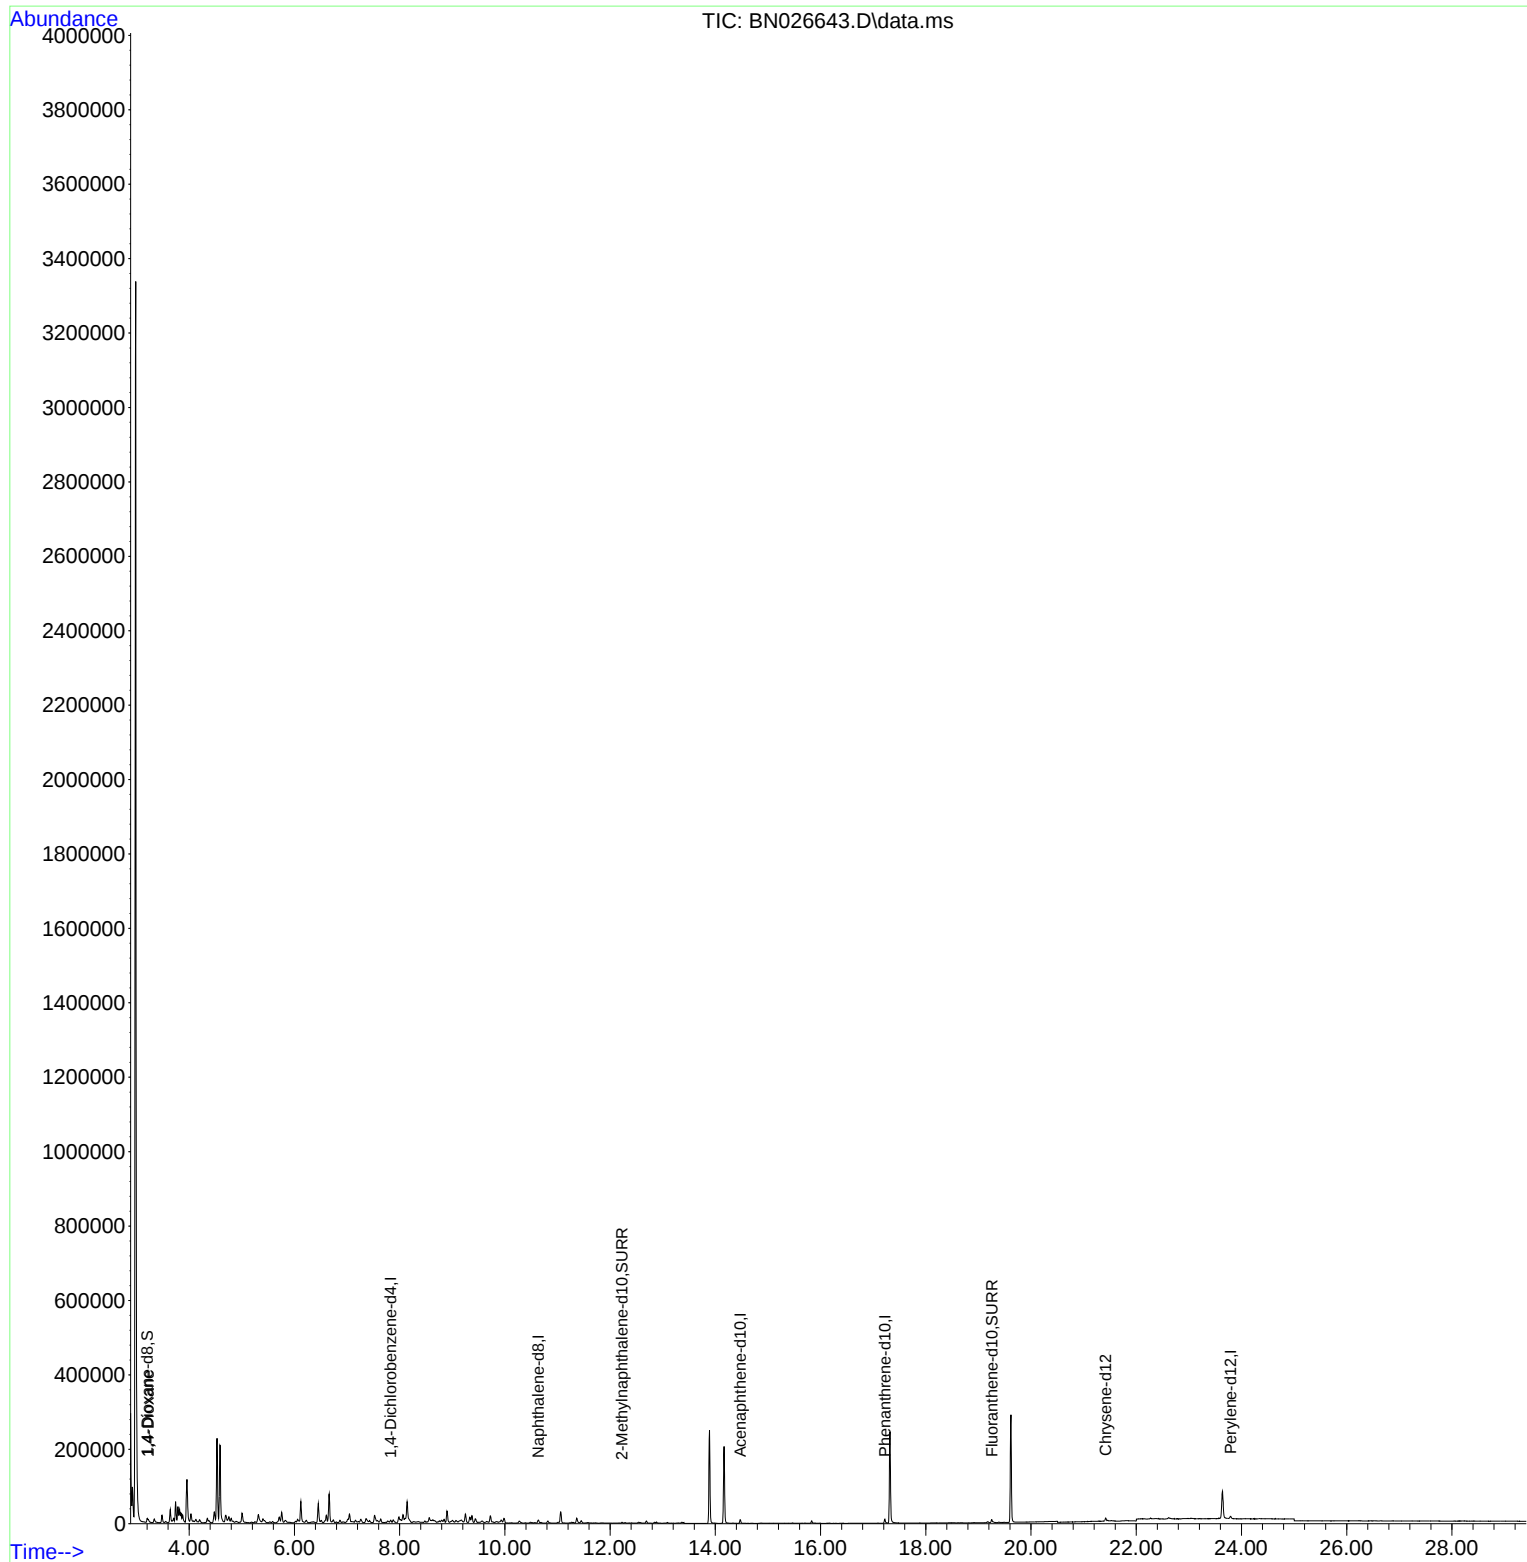

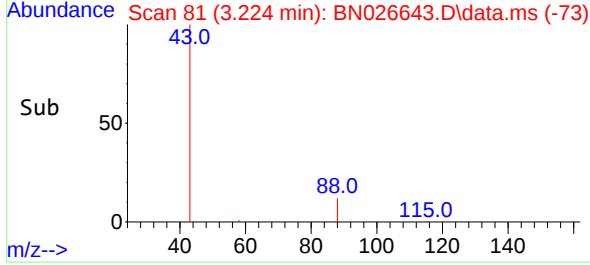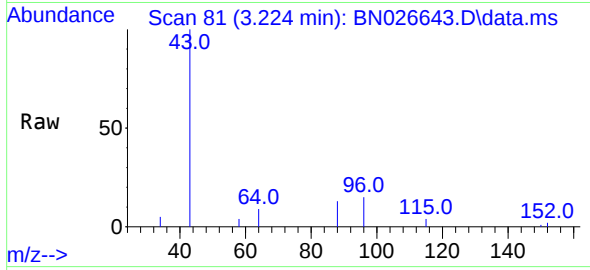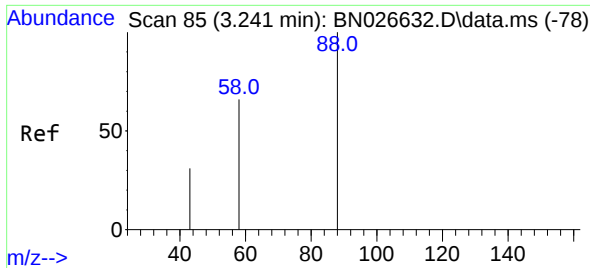

#2
1,4-Dioxane
Concen: 0.249 ng/ul
RT: 3.224 min Scan# 81
Delta R.T. -0.017 min
Lab File: BN026643.D
Acq: 22 Jul 2023 00:32

Instrument :
BNA_N
ClientSampleId :
YBW61

Tgt Ion: 88 Resp: 1215
Ion Ratio Lower Upper
88 100
43 748.0 33.0 49.6#
58 29.2 41.7 62.5#

