

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
 Data File : BN026646.D
 Acq On : 22 Jul 2023 02:23
 Operator : MA/JU
 Sample : 03536-12
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW66

Quant Time: Jul 22 04:11:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.831	152	3400	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.630	136	10705	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.471	164	6300	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	13356	0.400	ng/ul	0.00
17) Chrysene-d12	21.419	240	8037	0.400	ng/ul	# 0.00
23) Perylene-d12	23.790	264	9587	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	20666	4.615	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	9409	0.647	ng/ul	-0.02
18) Fluoranthene-d10	19.250	212	19610	0.704	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	290	0.068	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072023\
Data File : BN026646.D
Acq On : 22 Jul 2023 02:23
Operator : MA/JU
Sample : 03536-12
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW66


Quant Time: Jul 22 04:11:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

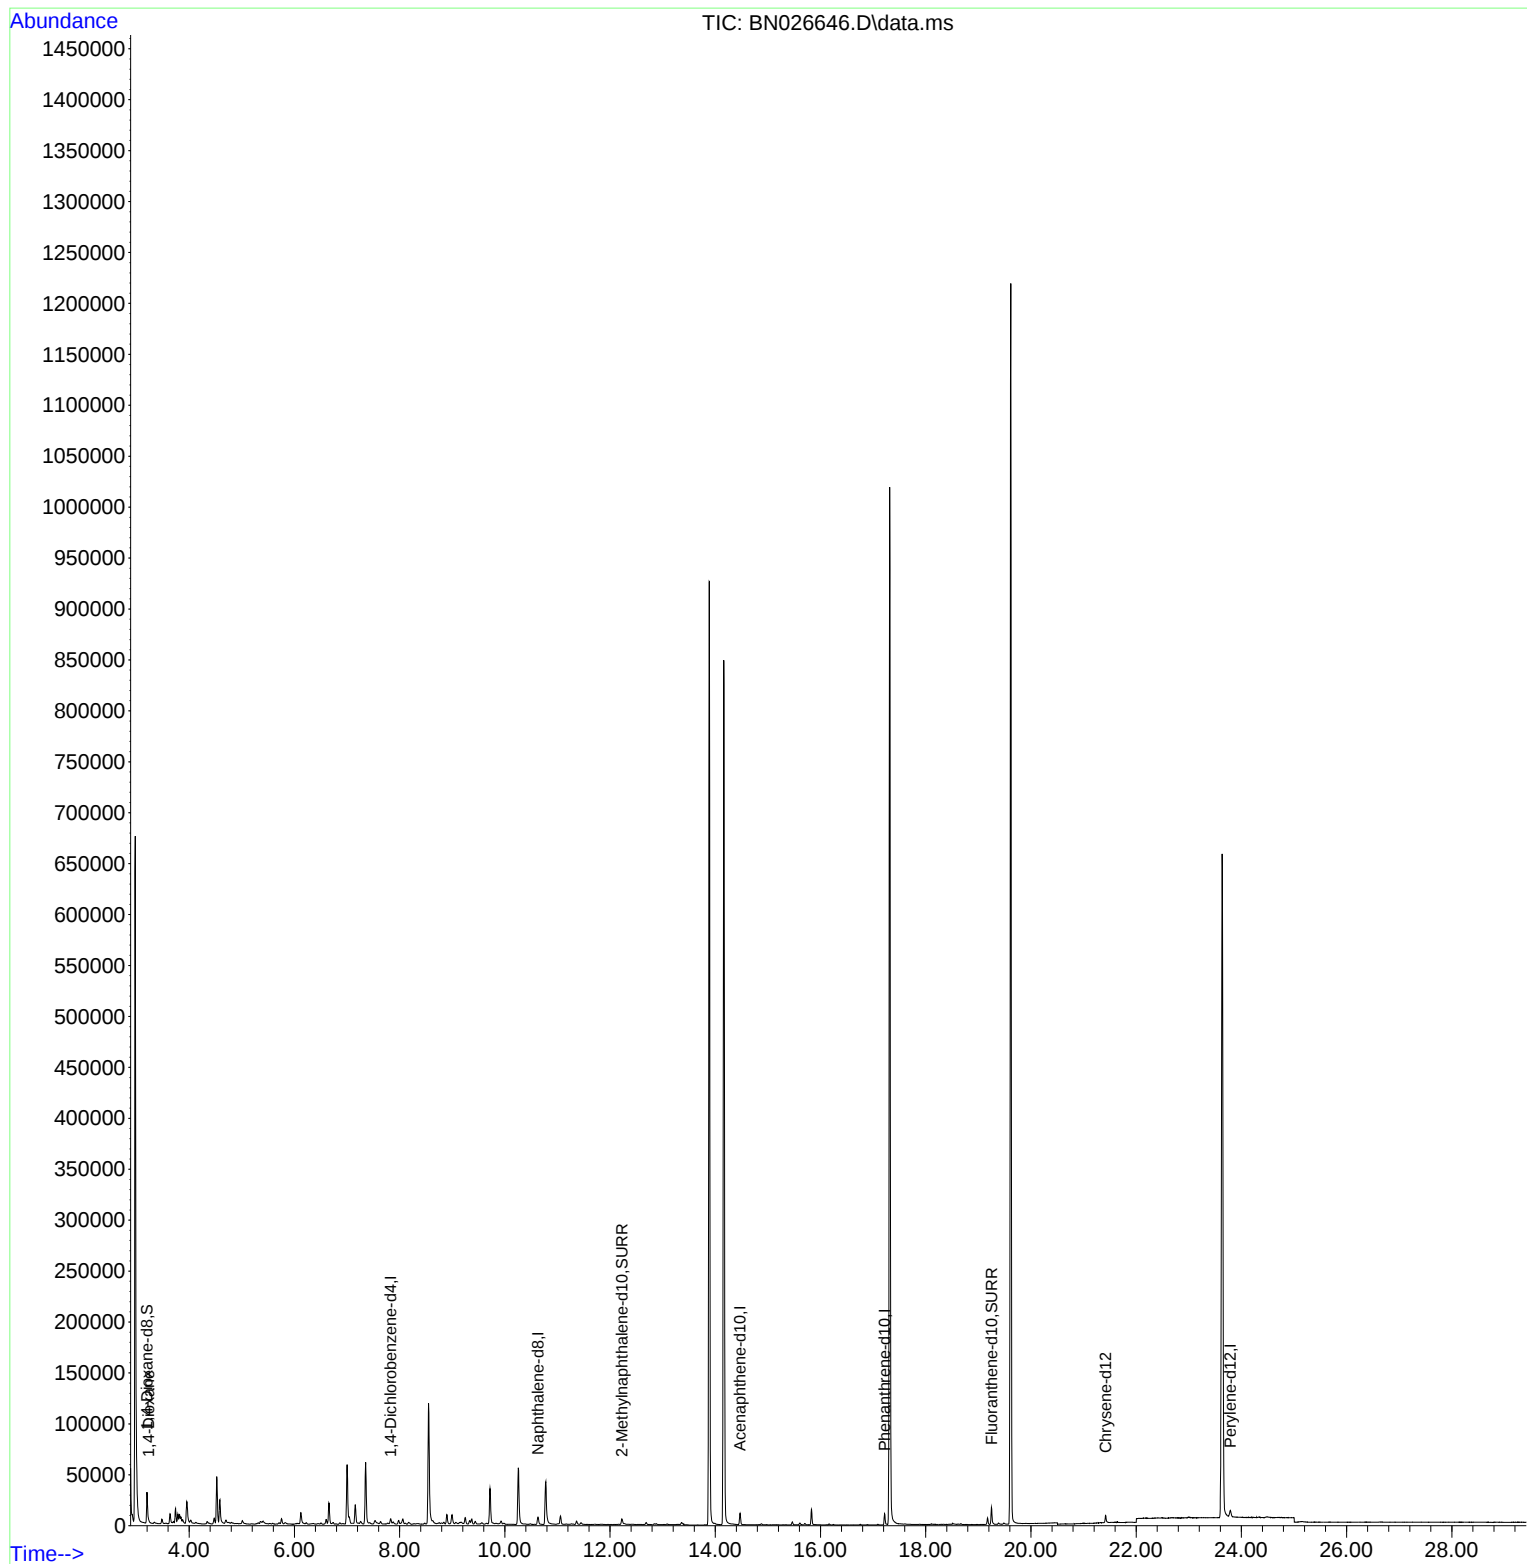


Abundance Scan 85 (3.241 min): BN026632.D\data.ms (-78)

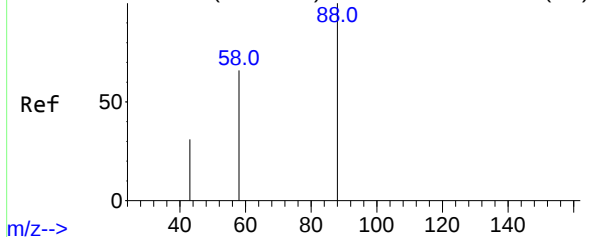

Abundance Scan 82 (3.228 min): BN026646.D\data.ms

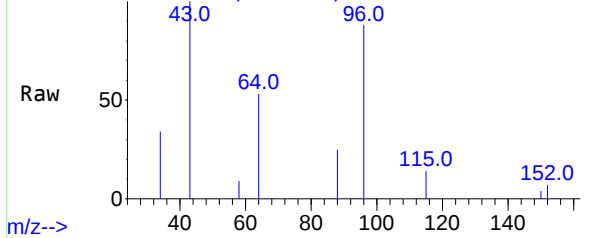

Abundance Scan 82 (3.228 min): BN026646.D\data.ms (-73)

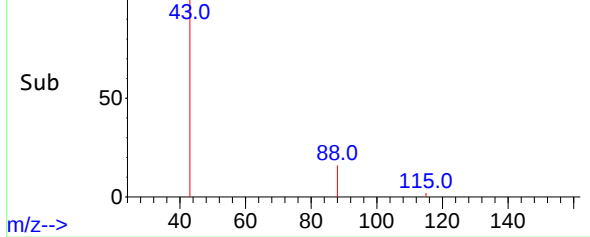

#2
1,4-Dioxane
Concen: 0.068 ng/ul
RT: 3.228 min Scan# 81
Delta R.T. -0.013 min
Lab File: BN026646.D
Acq: 22 Jul 2023 02:23

Instrument :
BNA_N
ClientSampleId :
YBW66

Tgt Ion: 88 Resp: 290
Ion Ratio Lower Upper
88 100
43 406.9 33.0 49.6#
58 35.6 41.7 62.5#

