


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072220\
 Data File : BN011217.D
 Acq On : 21 Jul 2020 13:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 21 14:35:20 2020

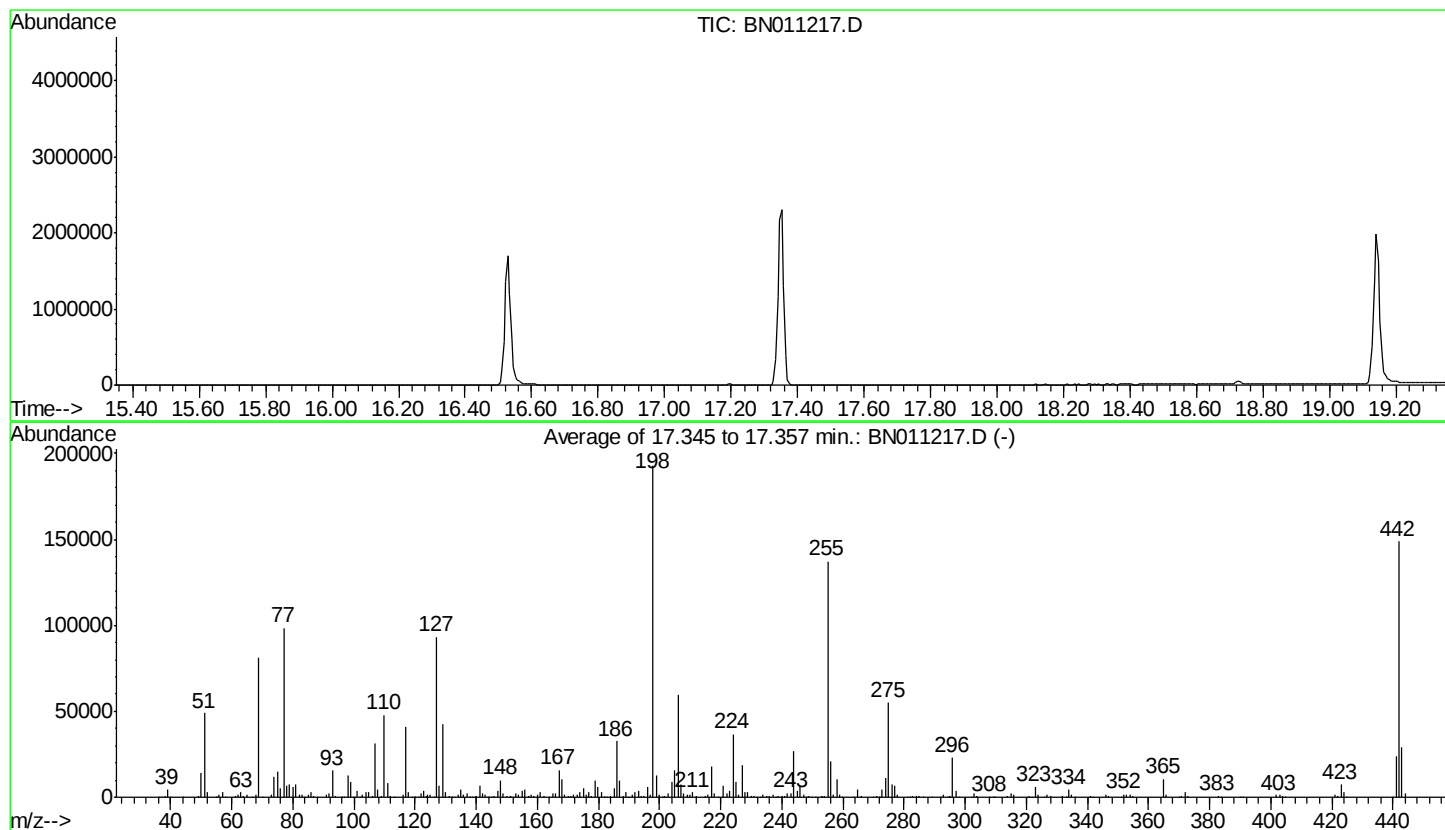

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	49096	PASS
68	69	0.00	2	1.9	1582	PASS
69	198	0.00	100	42.1	81229	PASS
70	69	0.00	2	0.5	367	PASS
127	198	10	80	48.4	93336	PASS
197	198	0.00	2	0.6	1249	PASS
198	198	100	100	100.0	192853	PASS
199	198	5	9	6.7	12996	PASS
275	198	10	60	28.4	54749	PASS
365	198	1	100	5.5	10566	PASS
441	198	0.01	100	12.5	24194	PASS
442	198	50	100	77.1	148698	PASS
443	442	15	24	19.7	29344	PASS