

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072223\
 Data File : BN026659.D
 Acq On : 22 Jul 2023 17:56
 Operator : MA/JU
 Sample : 03536-04RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW58RE

Quant Time: Jul 22 23:15:01 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 19:02:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	3872	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.630	136	12929	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.467	164	7410	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	14893	0.400	ng/ul	0.00
17) Chrysene-d12	21.411	240	9005	0.400	ng/ul	#-0.01
23) Perylene-d12	23.784	264	9699	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	3389	0.665	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.220	152	3965	0.226	ng/ul	-0.02
18) Fluoranthene-d10	19.250	212	7614	0.244	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.225	88	1097	0.227	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072223\
Data File : BN026659.D
Acq On : 22 Jul 2023 17:56
Operator : MA/JU
Sample : 03536-04RE
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW58RE


Quant Time: Jul 22 23:15:01 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 19:02:16 2023
Response via : Initial Calibration

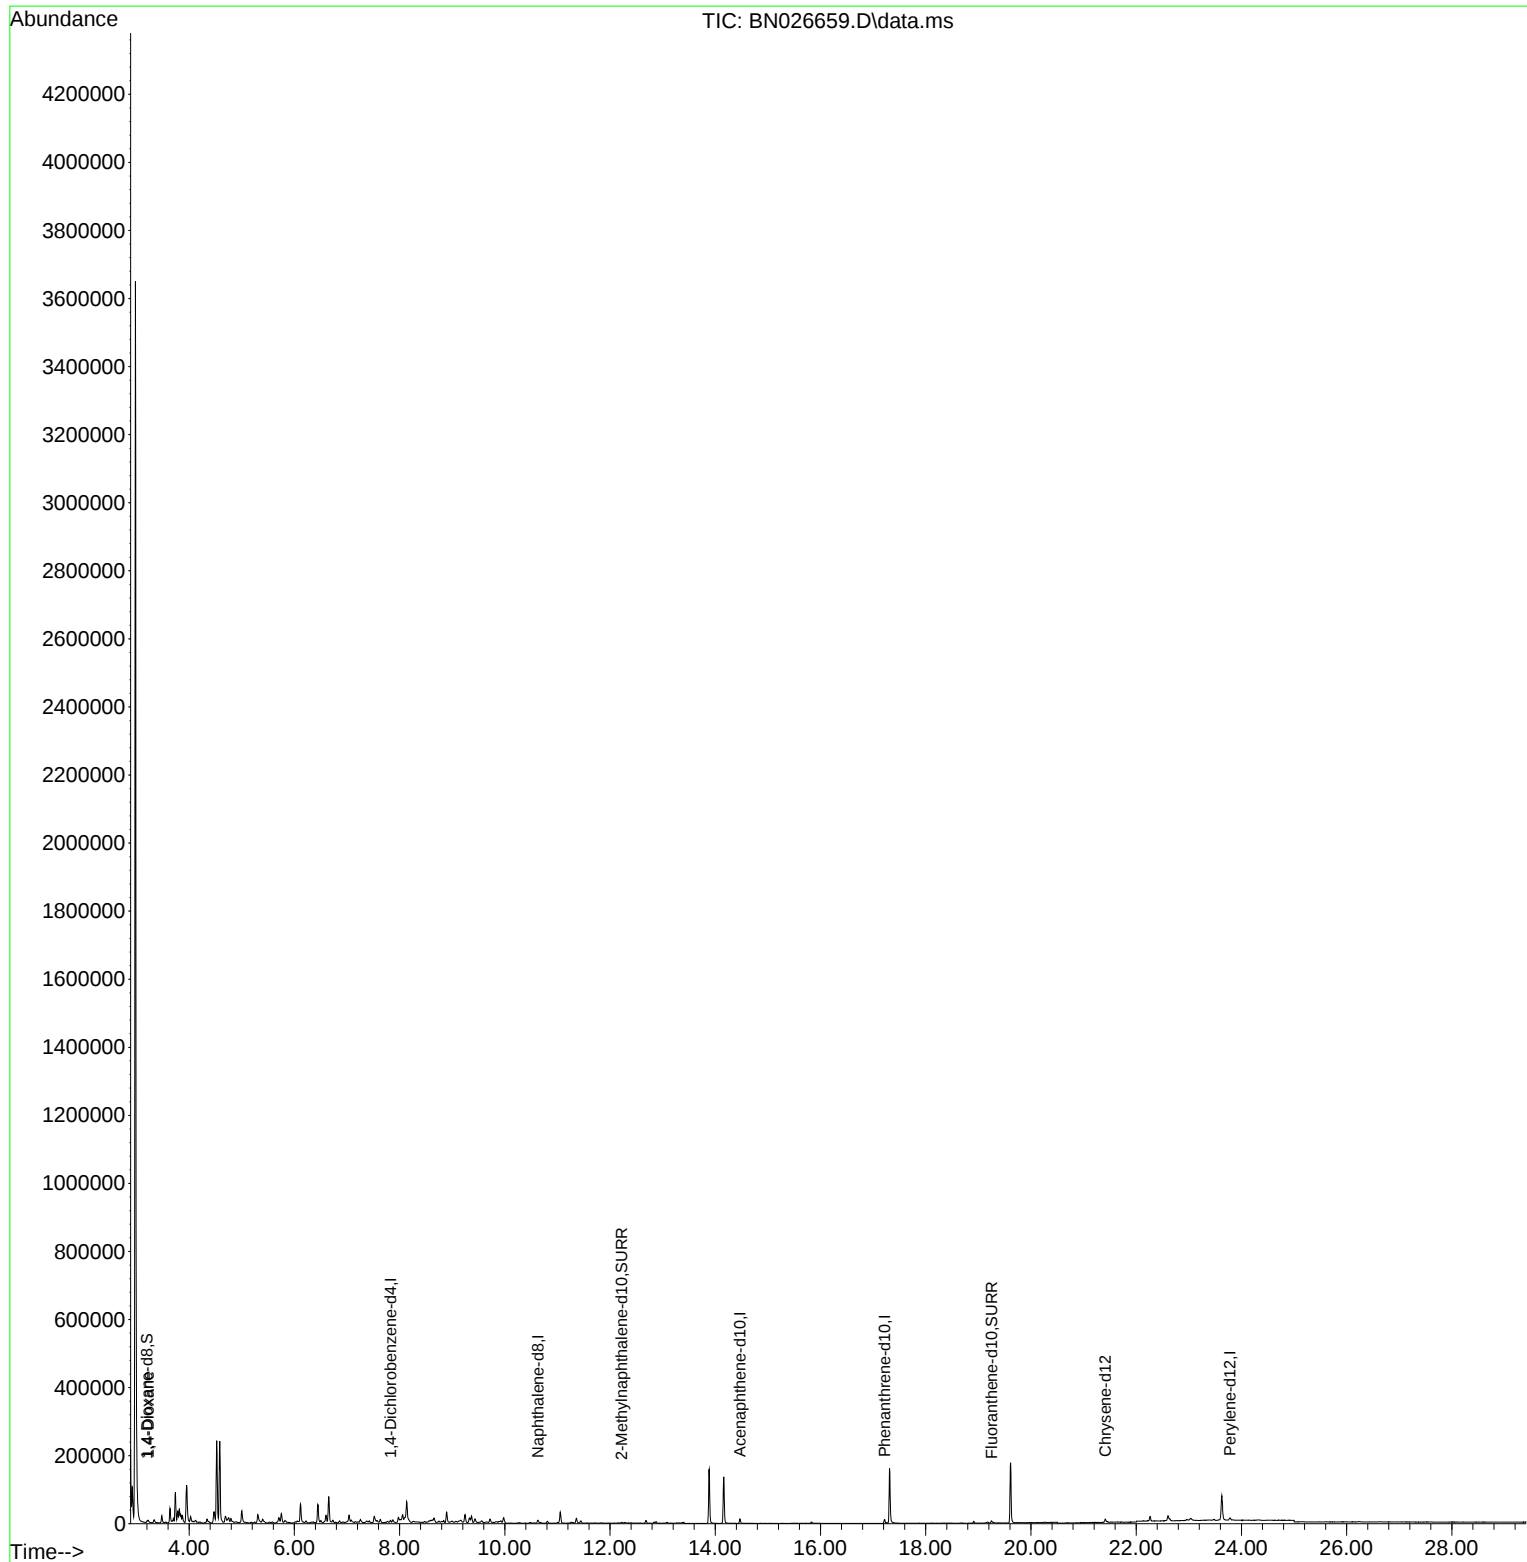

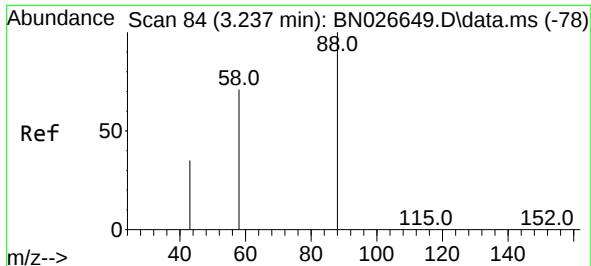

#2
 1,4-Dioxane
 Concen: 0.227 ng/ul
 RT: 3.225 min Scan# 81
 Delta R.T. -0.017 min
 Lab File: BN026659.D
 Acq: 22 Jul 2023 17:56

Instrument :
 BNA_N
 ClientSampleId :
 YBW58RE

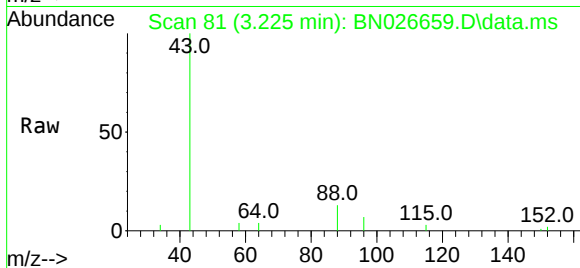

Tgt Ion: 88 Resp: 1097

Ion	Ratio	Lower	Upper
88	100		
43	757.9	33.0	49.6#
58	29.7	41.7	62.5#

