
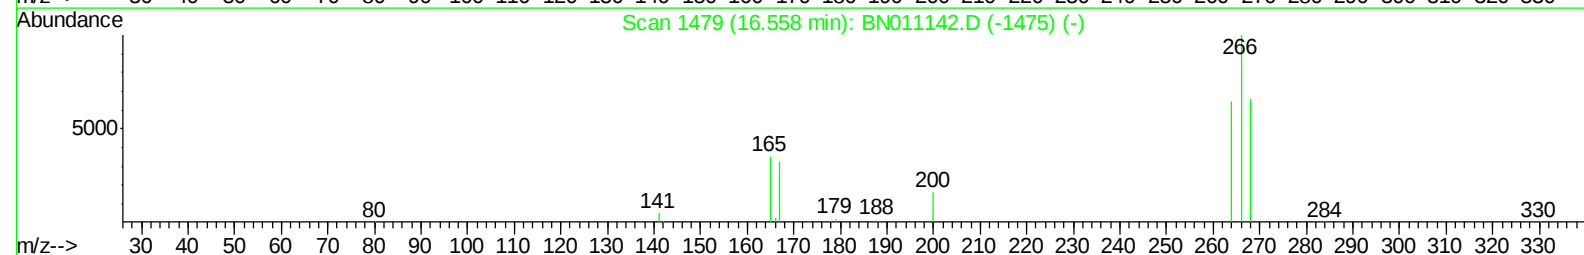
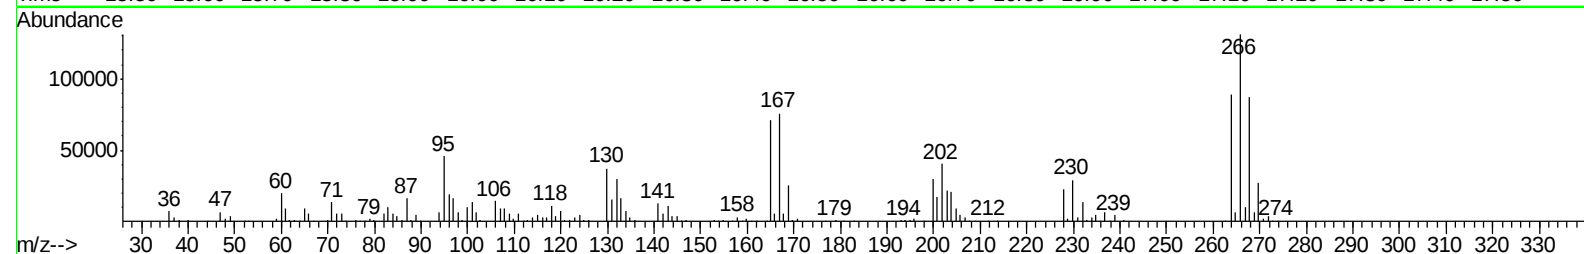


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072320\
 Data File : BN011223.D
 Acq On : 22 Jul 2020 17:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 04:46:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN071120.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 22 19:29:31 2020
 Response via : Initial Calibration

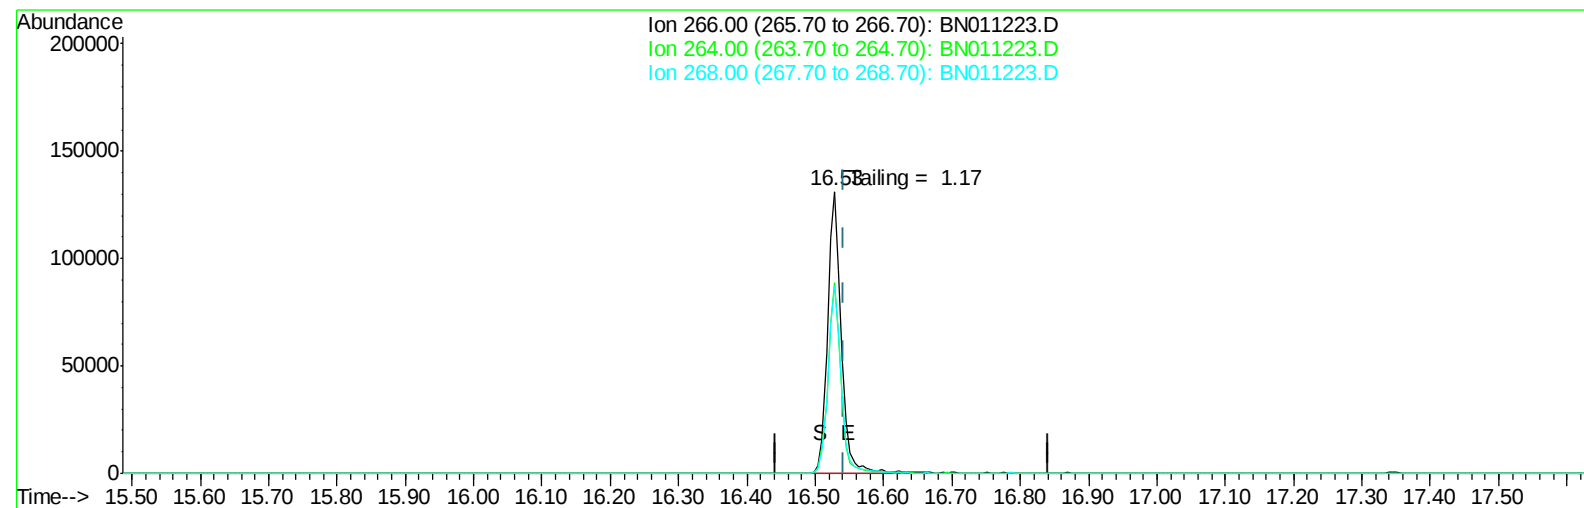

TIC: BN011223.D

(24) Pentachlorophenol

16.528min (-0.014) 0.00ng

response 184324

Ion	Exp%	Act%
266.00	100	100
264.00	65.60	65.06
268.00	61.10	64.99
0.00	0.00	0.00