


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072320\
 Data File : BN011223.D
 Acq On : 22 Jul 2020 17:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 22 19:29:31 2020

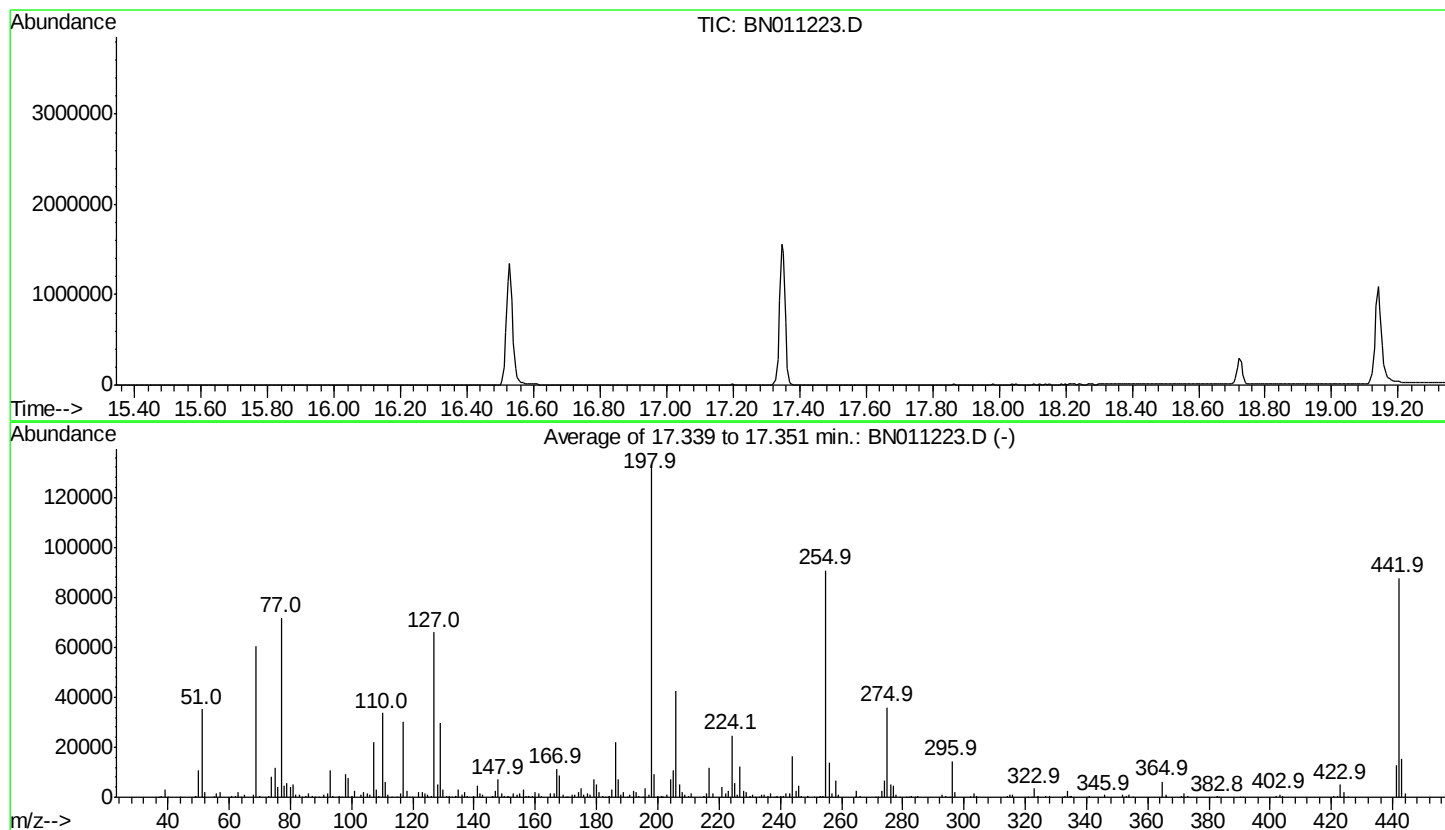

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	35312	PASS
68	69	0.00	2	1.9	1150	PASS
69	198	0.00	100	45.4	60269	PASS
70	69	0.00	2	0.7	393	PASS
127	198	10	80	49.7	65930	PASS
197	198	0.00	2	0.8	1071	PASS
198	198	100	100	100.0	132706	PASS
199	198	5	9	7.0	9266	PASS
275	198	10	60	27.1	35941	PASS
365	198	1	100	4.8	6351	PASS
441	198	0.01	100	9.5	12571	PASS
442	198	50	100	66.1	87714	PASS
443	442	15	24	17.6	15445	PASS