
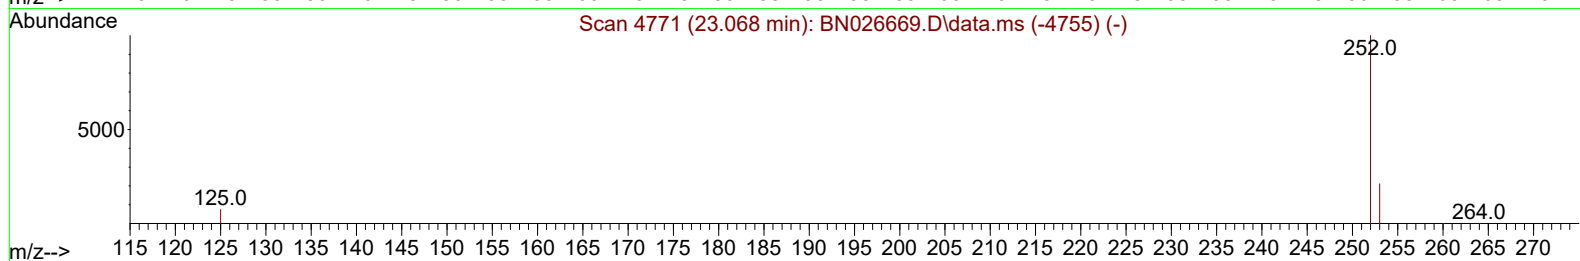
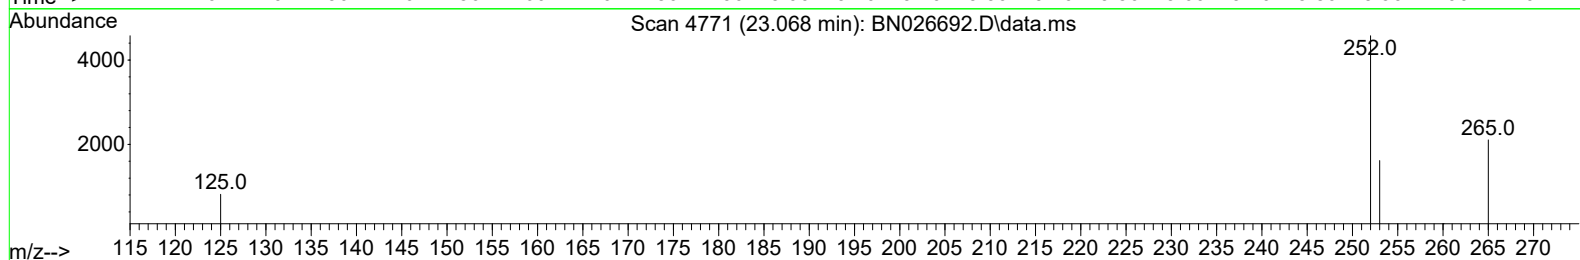


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026692.D
Acq On : 24 Jul 2023 01:01
Operator : MA/JU
Sample : 03472-34DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Jul 24 01:30:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

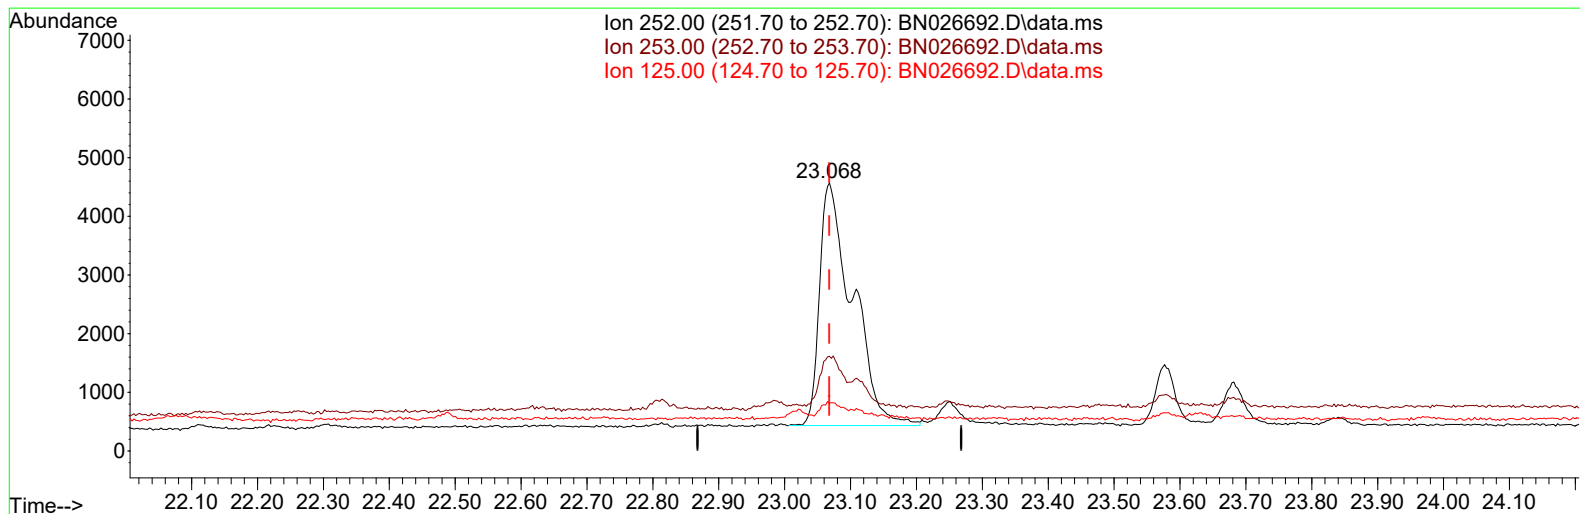

TIC: BN026692.D\data.ms

(24) Benzo(b)fluoranthene

23.068min (+ 0.000) 0.47 ng/u1

response 14357

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.30	35.30
125.00	17.00	17.84
0.00	0.00	0.00