

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058424.D
 Acq On : 23 Jul 2023 7:19
 Operator : CG/JU
 Sample : 03553-20
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 24 01:28:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.891	152	85754	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	374377	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.536	164	234575	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188	483892	20.000	ng/ul	0.00
79) Chrysene-d12	21.534	240	406395	20.000	ng/ul	0.00
88) Perylene-d12	24.671	264	492116	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.337	96	3172	1.361	ng/uL	0.00
4) Pyridine-d5	3.749	84	68547	9.912	ng/ul	0.00
7) Phenol-d5	7.062	99	34965	4.298	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.221	67	104519	20.556	ng/ul	0.00
11) 2-Chlorophenol-d4	7.427	132	94528	16.600	ng/ul	0.00
15) 4-Methylphenol-d8	8.602	113	62462	10.066	ng/ul	0.00
21) Nitrobenzene-d5	9.054	128	63658	22.685	ng/ul	0.00
24) 2-Nitrophenol-d4	9.777	143	46718	15.250	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.323	165	102016	17.371	ng/ul	0.00
31) 4-Chloroaniline-d4	10.834	131	134368	15.783	ng/ul	0.00
46) Dimethylphthalate-d6	13.937	166	405758	22.432	ng/ul	0.00
49) Acenaphthylene-d8	14.225	160	450880	23.785	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	0.00
60) Fluorene-d10	15.523	176	357563	23.876	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	0.00
73) Anthracene-d10	17.380	188	572840	27.398	ng/ul	0.00
81) Pyrene-d10	19.671	212	644387	26.846	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.454	264	652012	27.412	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.410	149	17833	1.143	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
Data File : BG058424.D
Acq On : 23 Jul 2023 7:19
Operator : CG/JU
Sample : 03553-20
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 24 01:28:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

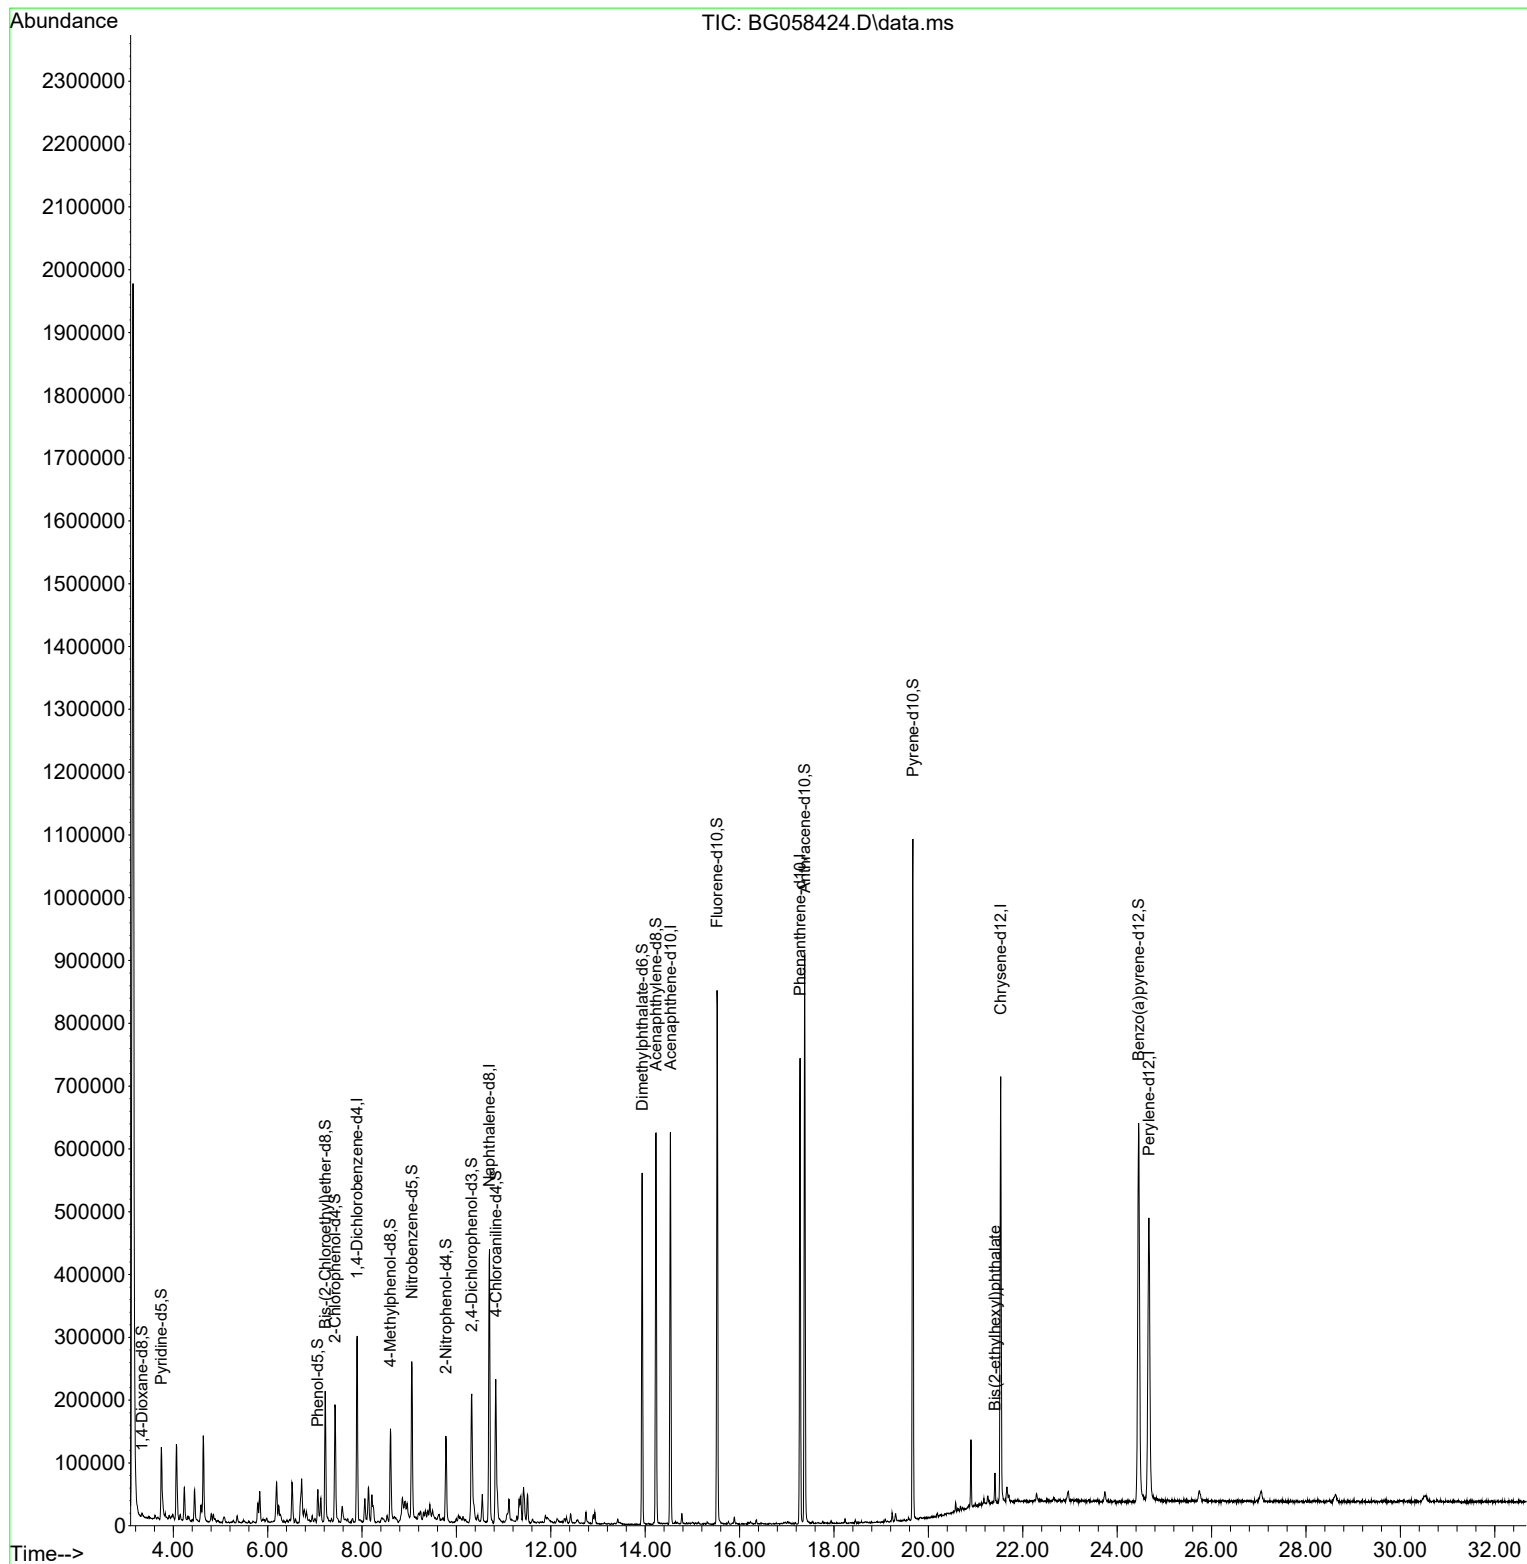

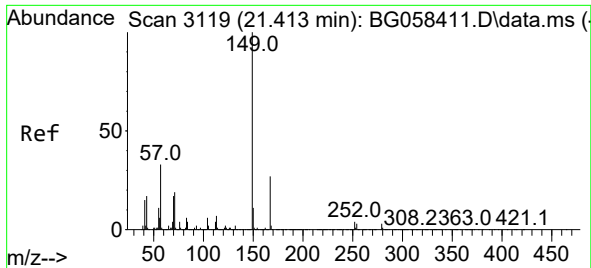

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.143 ng/ul
 RT: 21.410 min Scan# 3118
 Delta R.T. -0.002 min
 Lab File: BG058424.D
 Acq: 23 Jul 2023 7:19

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:149 Resp: 17833
 Ion Ratio Lower Upper
 149 100
 167 33.1 21.6 32.4#
 279 3.3 3.0 4.4

