

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026671.D
 Acq On : 23 Jul 2023 11:40
 Operator : MA/JU
 Sample : PB154124BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 24 00:40:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	5477	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	19065	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	11819	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	25244	0.400	ng/ul	0.00
17) Chrysene-d12	21.422	240	14917	0.400	ng/ul	0.00
23) Perylene-d12	23.796	264	18424	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	28542	3.957	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	8196	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.246	212	18477	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.613	202	3053	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.641	252	5846	0.091	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026671.D
Acq On : 23 Jul 2023 11:40
Operator : MA/JU
Sample : PB154124BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 24 00:40:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

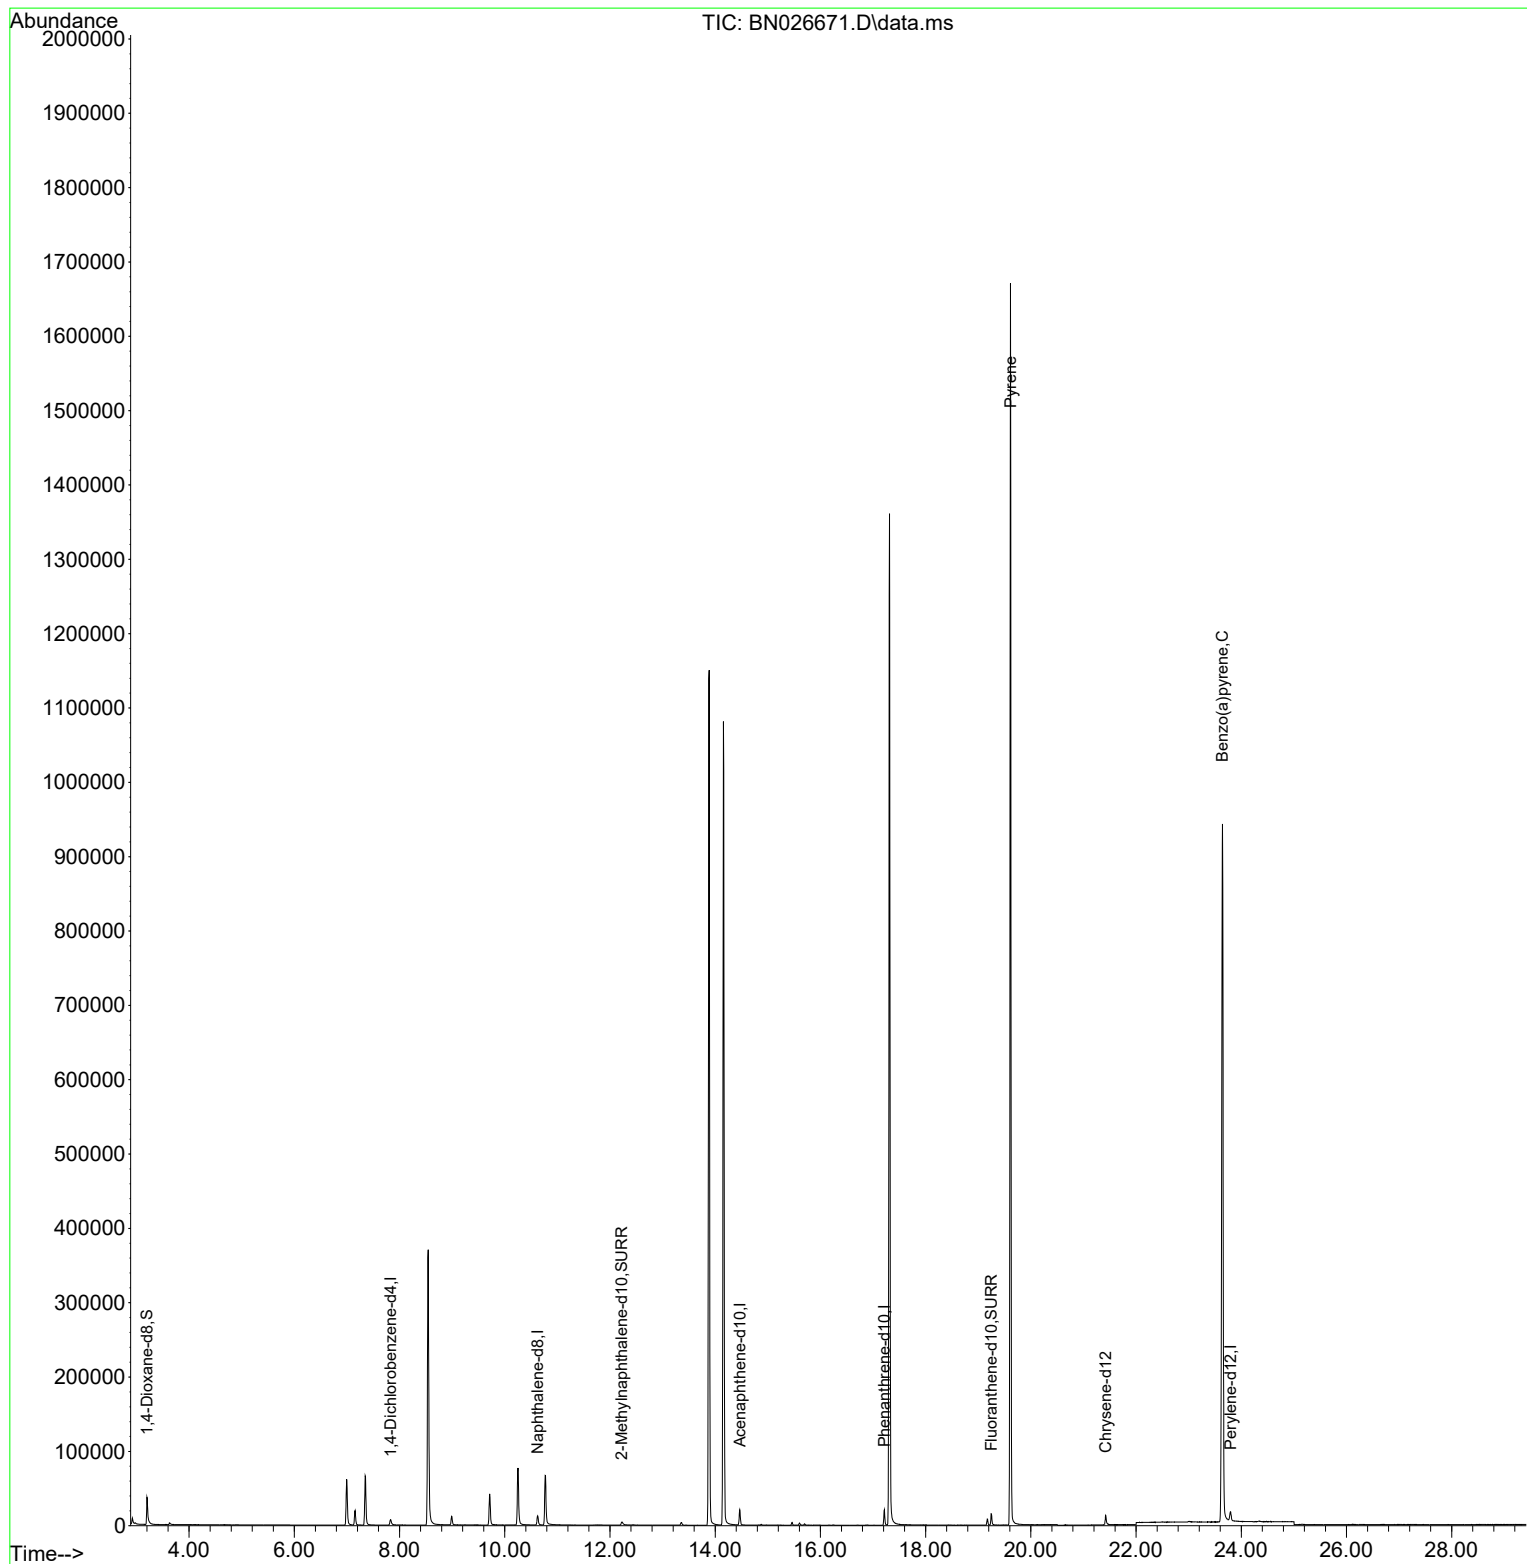

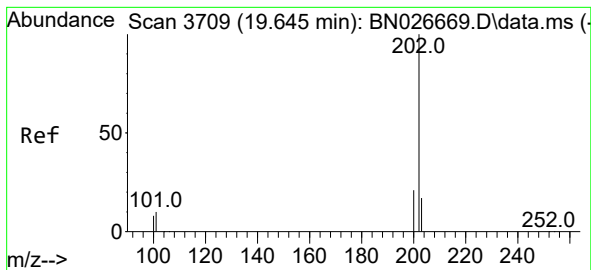

#20

Pyrene

Concen: 0.040 ng/ul

RT: 19.613 min Scan# 31

Delta R.T. -0.033 min


Lab File: BN026671.D

Acq: 23 Jul 2023 11:40

Instrument :

BNA_N

ClientSampleId :

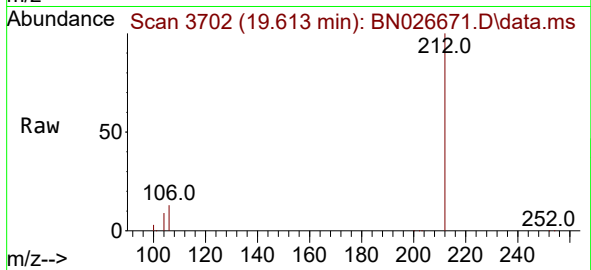




Tgt Ion:202 Resp: 3053

Ion Ratio Lower Upper

202 100

101 201.5 8.0 12.0#

100 1593.9 6.2 9.2#

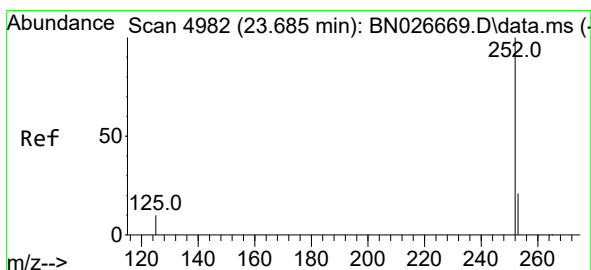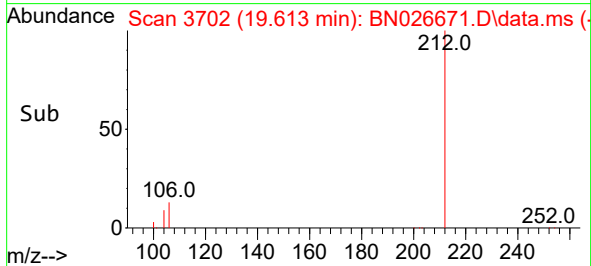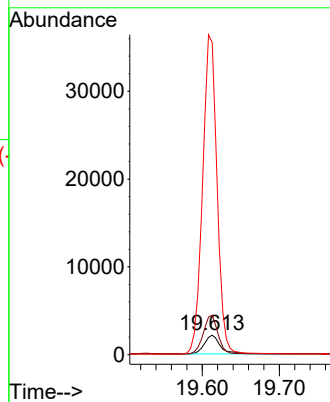

#26

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 23.641 min Scan# 4967

Delta R.T. -0.044 min

Lab File: BN026671.D

Acq: 23 Jul 2023 11:40

Tgt Ion:252 Resp: 5846

Ion Ratio Lower Upper

252 100

253 53.1 32.6 49.0#

125 64.5 19.3 28.9#

