

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026676.D
 Acq On : 23 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03504-21MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 24 00:41:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.823	152	4255	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	13654	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.467	164	8309	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	18274	0.400	ng/ul	0.00
17) Chrysene-d12	21.419	240	13123	0.400	ng/ul #	0.00
23) Perylene-d12	23.793	264	11142	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	1005	0.179	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.220	152	3157	0.170	ng/ul	0.00
18) Fluoranthene-d10	19.246	212	5646	0.124	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.233	88	4025	0.759	ng/ul#	1
5) Naphthalene	10.674	128	8406	0.224	ng/ul	98
7) 2-Methylnaphthalene	12.291	142	4924	0.231	ng/ul	98
8) 1-Methylnaphthalene	12.511	142	5222	0.229	ng/ul	95
10) Acenaphthylene	14.189	152	7163	0.176	ng/ul	97
11) Acenaphthene	14.527	153	7874	0.254	ng/ul	100
12) Fluorene	15.517	166	9467	0.291	ng/ul	98
14) Pentachlorophenol	16.886	266	160	0.035	ng/ul	84
15) Phenanthrene	17.257	178	60345	1.037	ng/ul	97
16) Anthracene	17.350	178	6068	0.120	ng/ul	96
19) Fluoranthene	19.278	202	94210	1.532	ng/ul#	94
20) Pyrene	19.641	202	17229	0.258	ng/ul	99
21) Benzo(a)anthracene	21.402	228	30809	0.639	ng/ul	98
22) Chrysene	21.454	228	33244	0.606	ng/ul	99
24) Benzo(b)fluoranthene	23.074	252	37562	0.865	ng/ul	90
25) Benzo(k)fluoranthene	23.117	252	22147	0.487	ng/ul#	88
27) Indeno(1,2,3-cd)pyrene	26.254	276	6883	0.136	ng/ul#	90
28) Dibenzo(a,h)anthracene	26.257	278	12400	0.319	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026676.D
 Acq On : 23 Jul 2023 14:42
 Operator : MA/JU
 Sample : 03504-21MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :


Quant Time: Jul 24 00:41:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

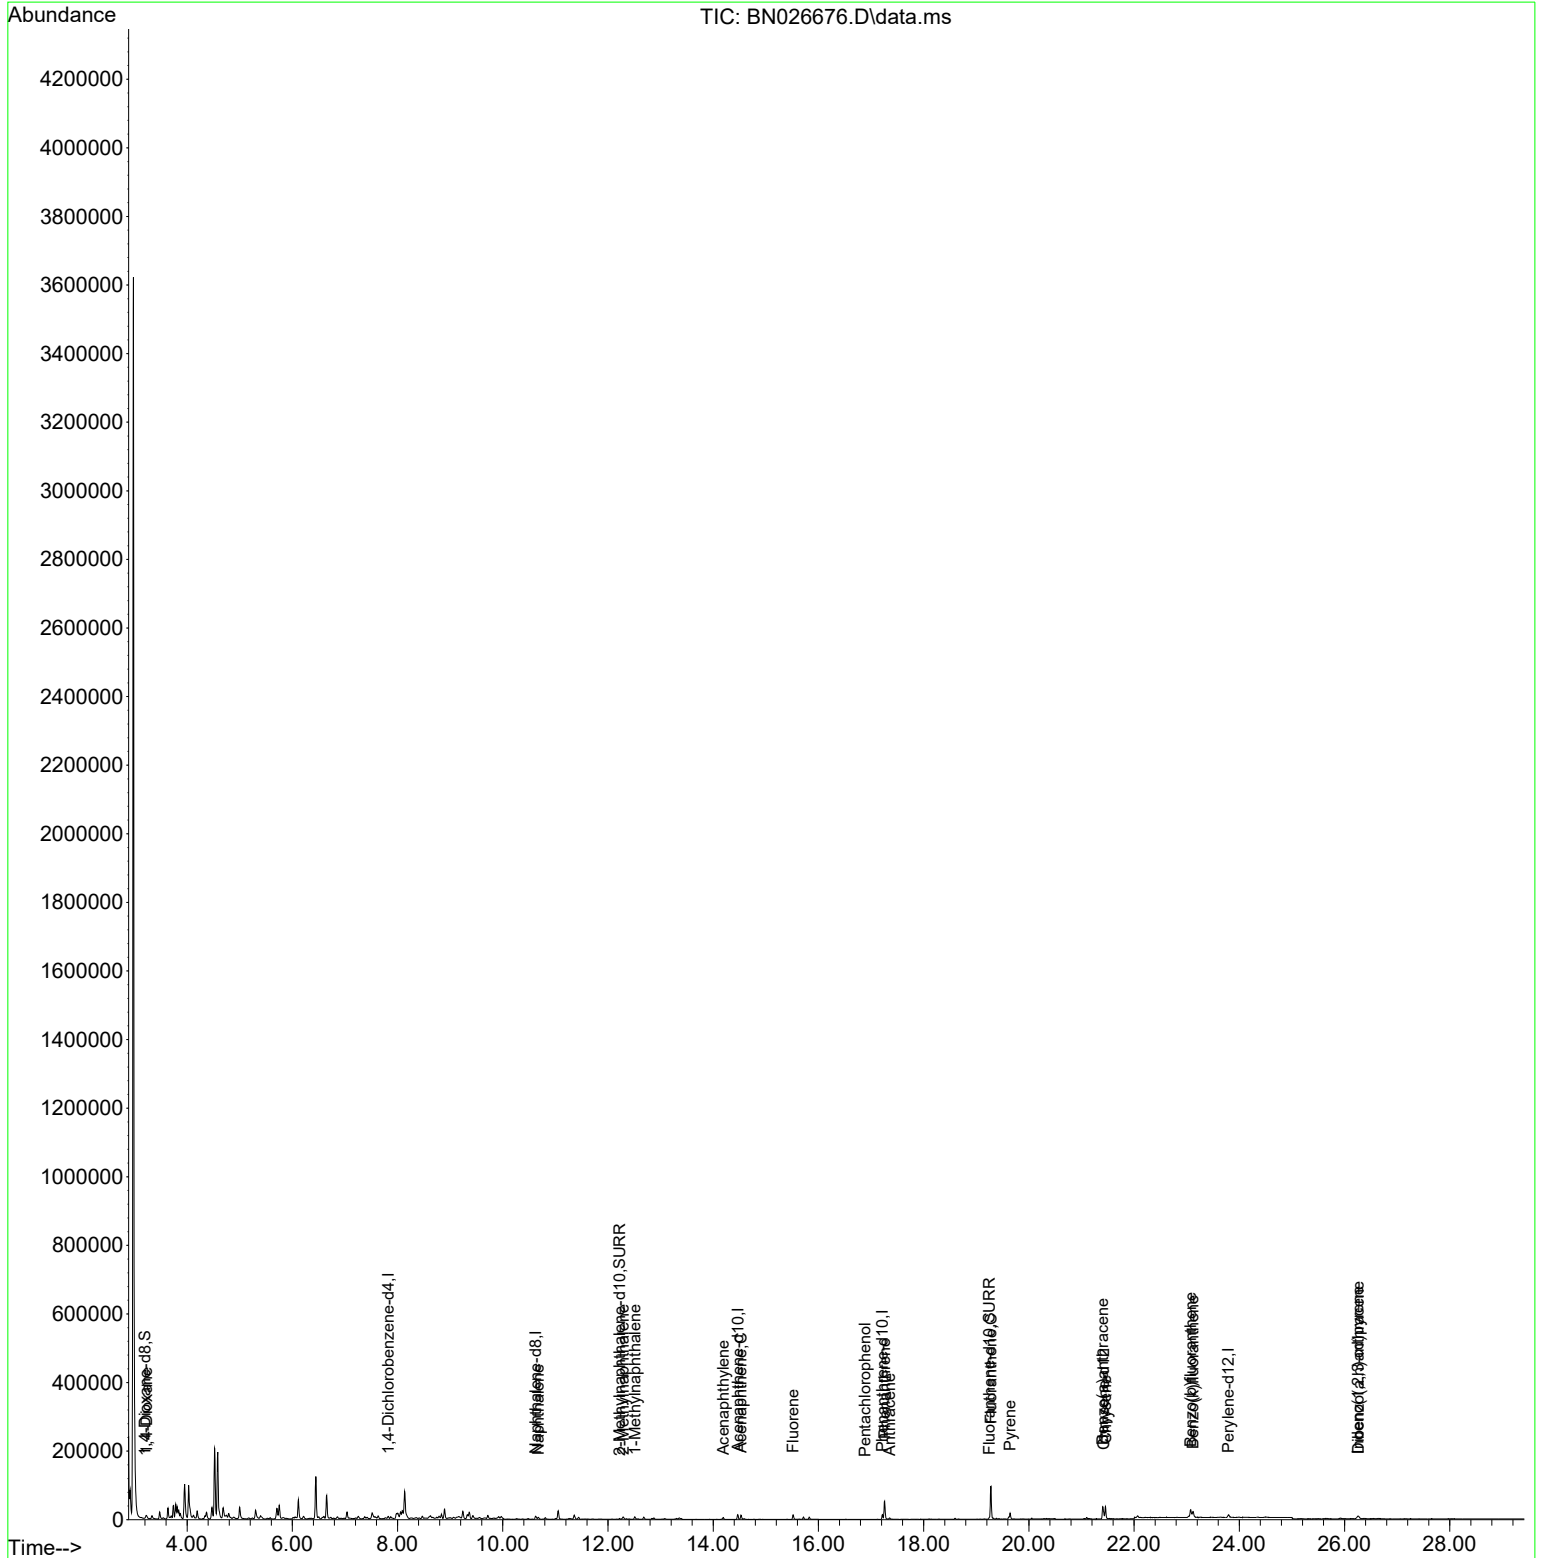



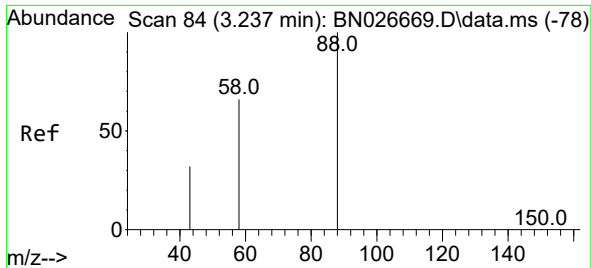


#2
 1,4-Dioxane
 Concen: 0.759 ng/ul
 RT: 3.233 min Scan# 81
 Delta R.T. -0.004 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument :
 BNA_N
 ClientSampleId :



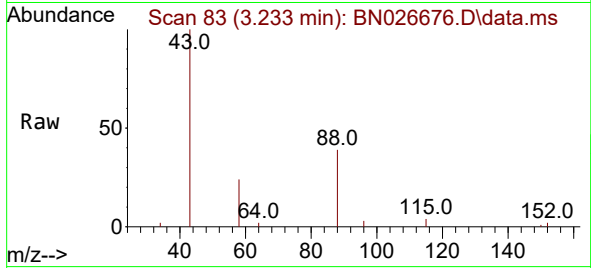



Tgt Ion: 88 Resp: 4025
 Ion Ratio Lower Upper
 88 100
 43 254.0 33.0 49.6#
 58 60.3 41.7 62.5

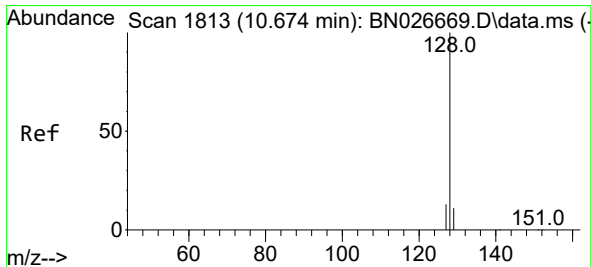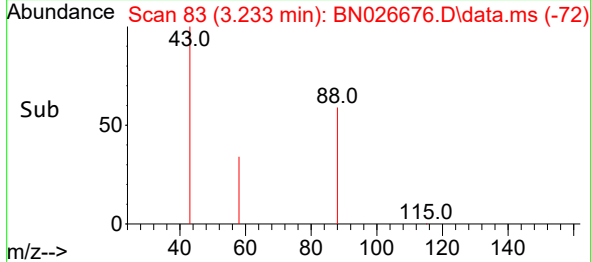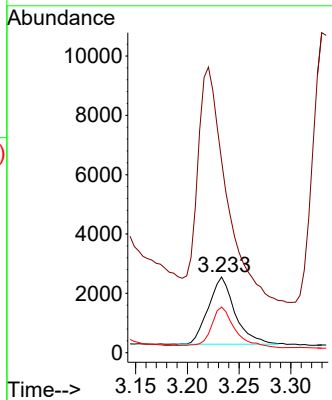

#5
 Naphthalene
 Concen: 0.224 ng/ul
 RT: 10.674 min Scan# 1813
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42


Tgt Ion:128 Resp: 8406
 Ion Ratio Lower Upper
 128 100
 129 13.2 10.2 15.2
 127 15.6 11.4 17.0

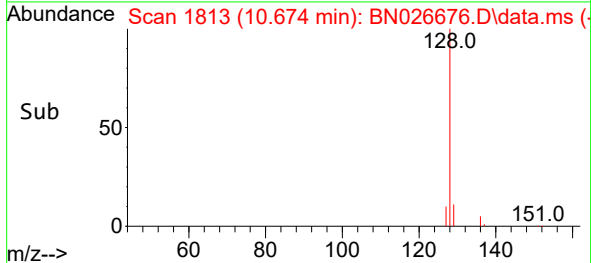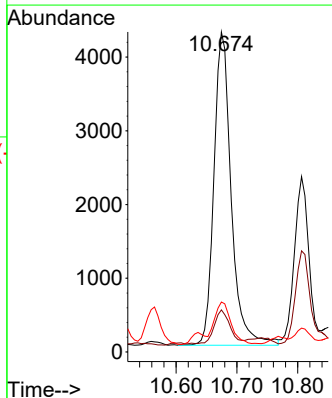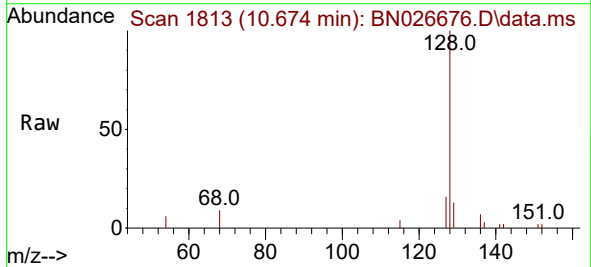



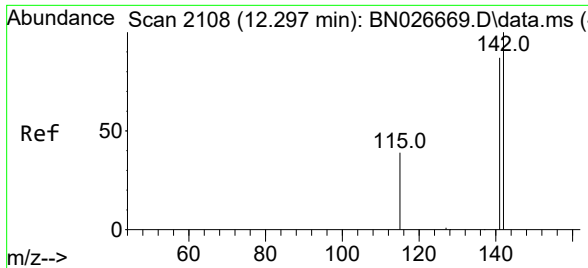


#7
 2-Methylnaphthalene
 Concen: 0.231 ng/ul
 RT: 12.291 min Scan# 2107
 Delta R.T. -0.006 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument :
 BNA_N
 ClientSampleId :



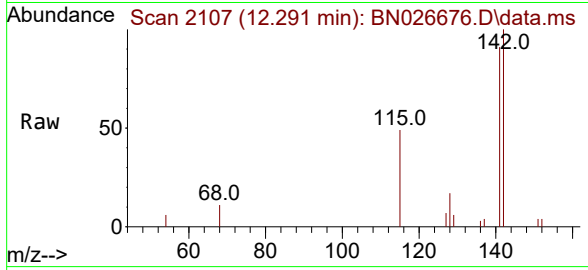



Tgt Ion:142 Resp: 4924
 Ion Ratio Lower Upper
 142 100
 141 92.0 72.3 108.5

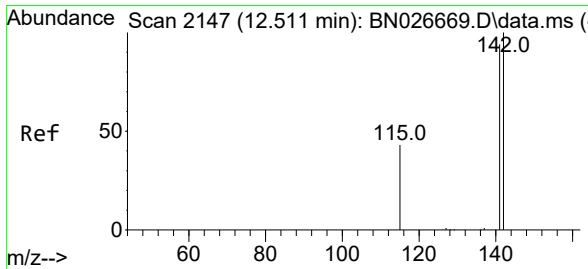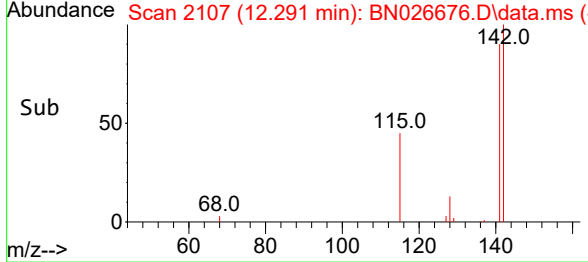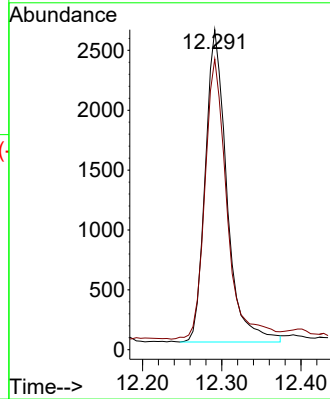

#8
 1-Methylnaphthalene
 Concen: 0.229 ng/ul
 RT: 12.511 min Scan# 2147
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42


Tgt Ion:142 Resp: 5222
 Ion Ratio Lower Upper
 142 100
 141 88.8 74.5 111.7

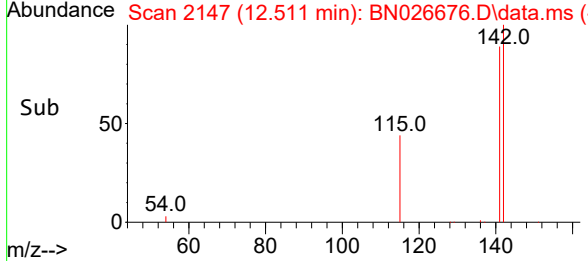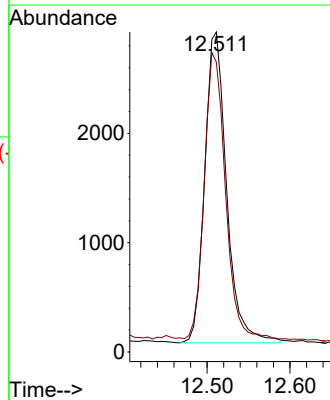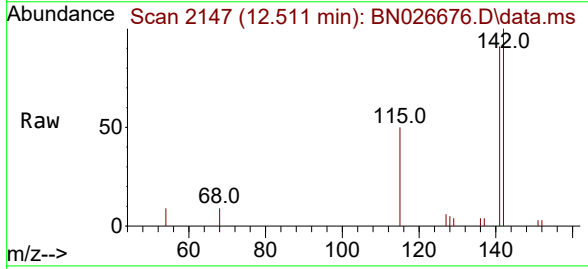

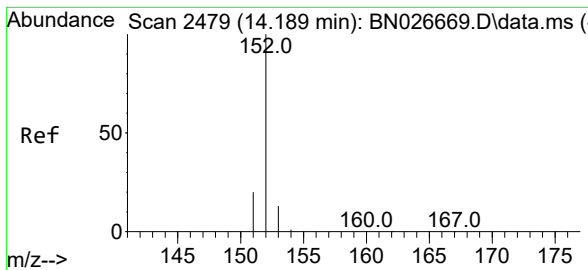




#10
 Acenaphthylene
 Concen: 0.176 ng/u1
 RT: 14.189 min Scan# 2479
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument :
 BNA_N
 ClientSampleId :

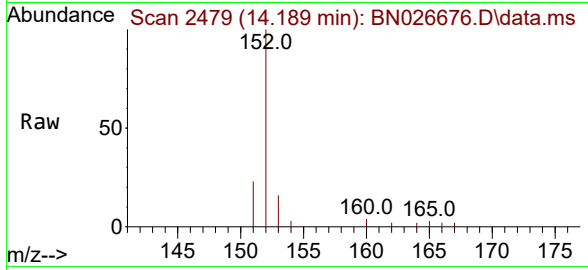

Tgt Ion:152 Resp: 7163




Ion	Ratio	Lower	Upper
152	100		
151	22.7	17.0	25.6
153	15.7	11.4	17.2

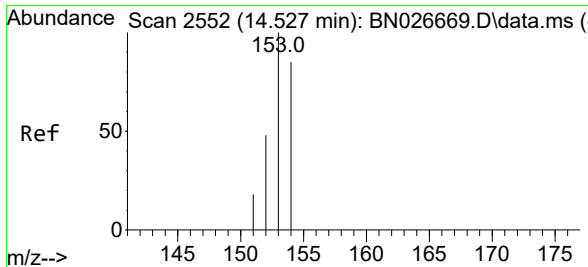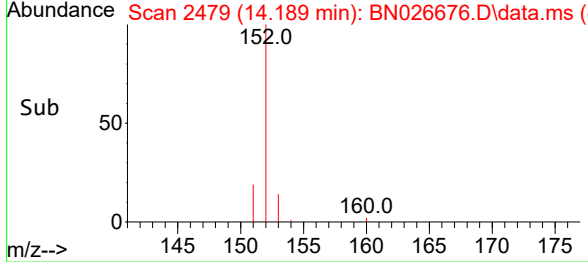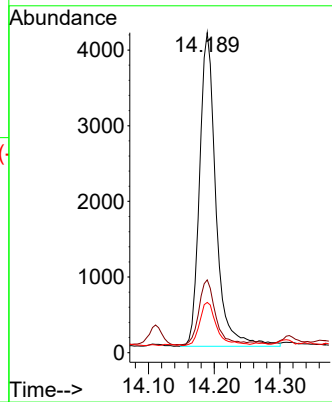


#11
 Acenaphthene
 Concen: 0.254 ng/u1
 RT: 14.527 min Scan# 2552
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Tgt Ion:153 Resp: 7874


Ion	Ratio	Lower	Upper
153	100		
152	50.3	40.2	60.4
154	86.1	69.3	103.9

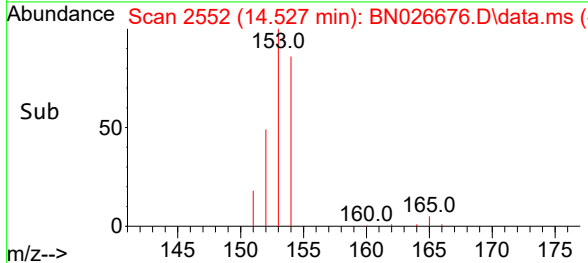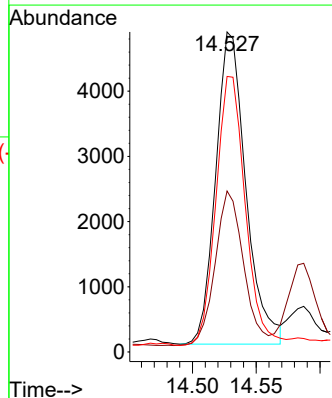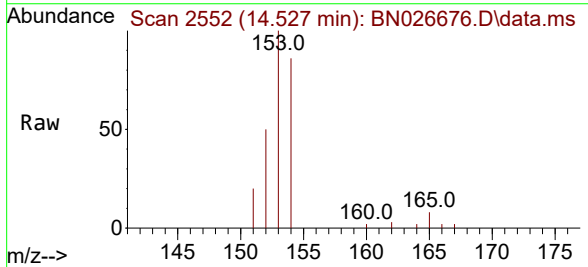

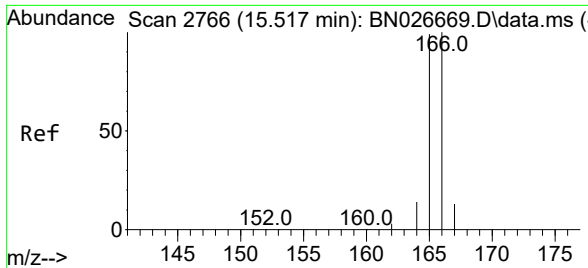




#12
 Fluorene
 Concen: 0.291 ng/ul
 RT: 15.517 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument :
 BNA_N
 ClientSampleId :

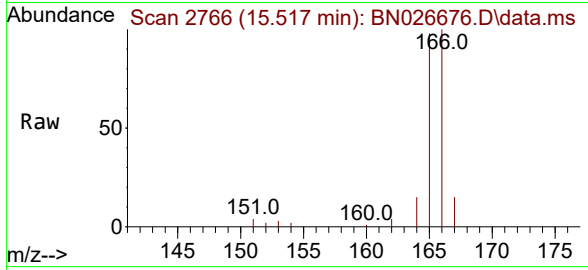

Tgt Ion:166 Resp: 9467




Ion	Ratio	Lower	Upper
166	100		
165	98.2	80.6	120.8
167	15.2	12.0	18.0

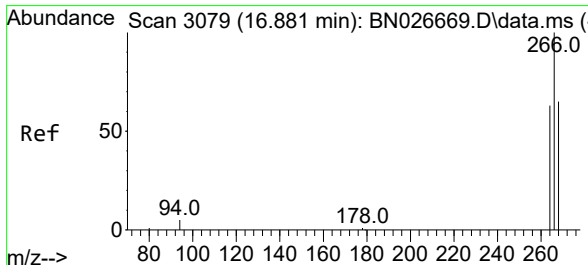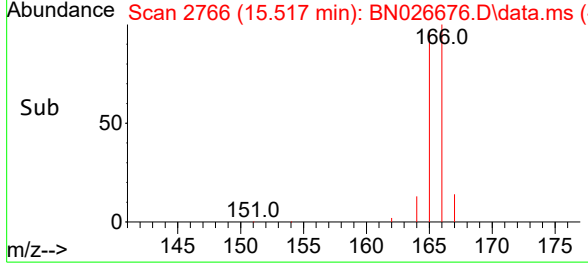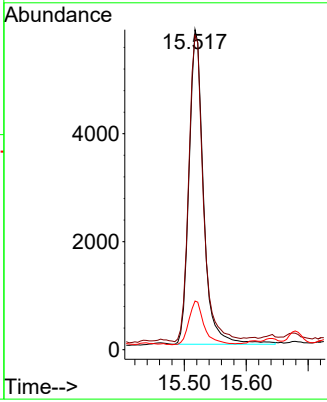


#14
 Pentachlorophenol
 Concen: 0.035 ng/ul
 RT: 16.886 min Scan# 3080
 Delta R.T. 0.004 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Tgt Ion:266 Resp: 160


Ion	Ratio	Lower	Upper
266	100		
264	52.5	52.0	78.0
268	79.4	53.0	79.6

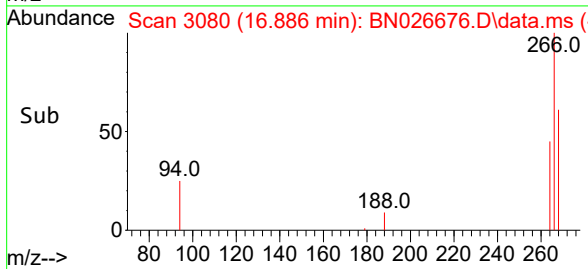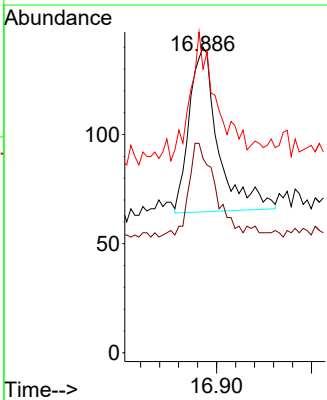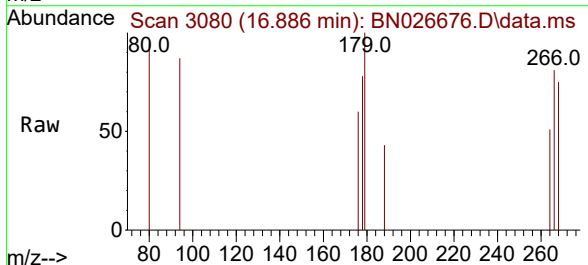

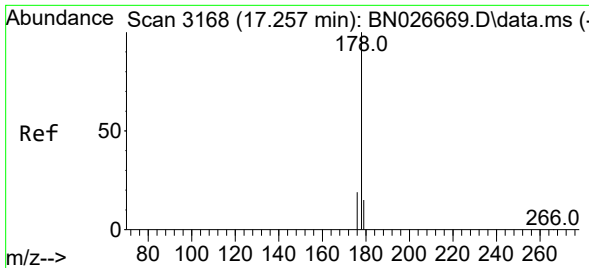




#15
 Phenanthrene
 Concen: 1.037 ng/u1
 RT: 17.257 min Scan# 3168
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument : BNA_N
 ClientSampleId :

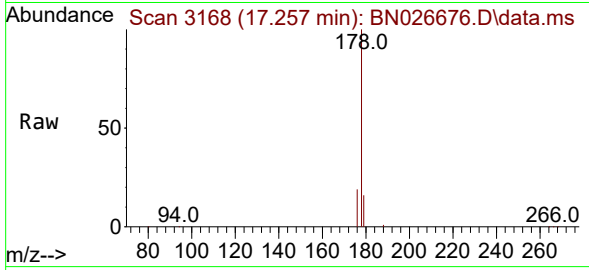

Tgt Ion:178 Resp: 60345




Ion	Ratio	Lower	Upper
178	100		
179	15.8	13.7	20.5
176	19.5	16.5	24.7

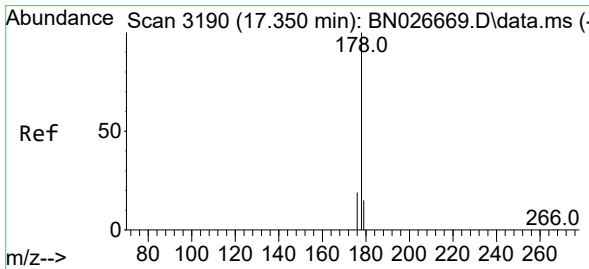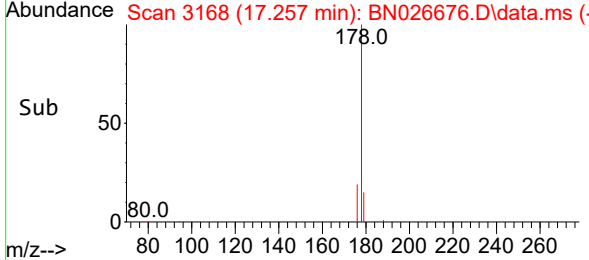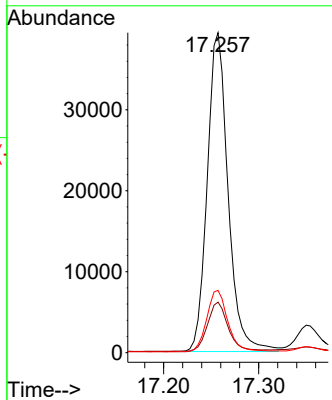


#16
 Anthracene
 Concen: 0.120 ng/u1
 RT: 17.350 min Scan# 3190
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Tgt Ion:178 Resp: 6068


Ion	Ratio	Lower	Upper
178	100		
179	20.8	14.8	22.2
176	21.9	16.6	25.0

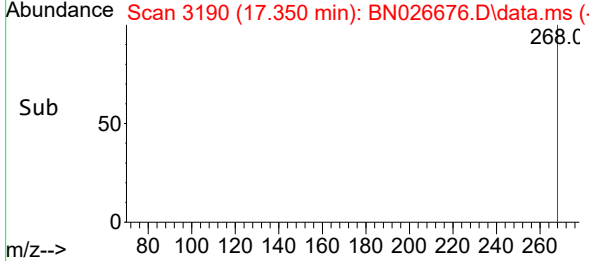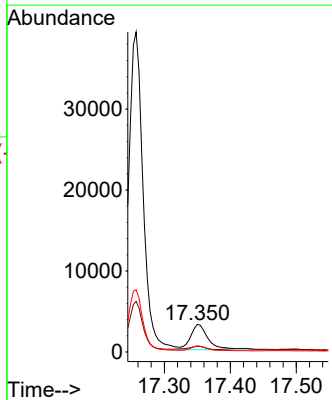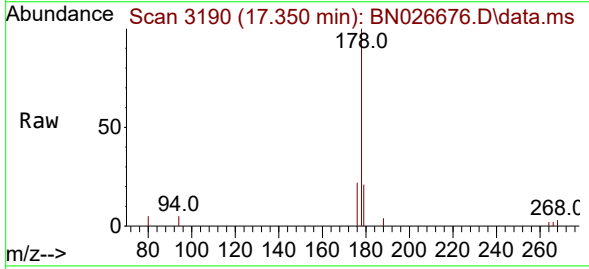



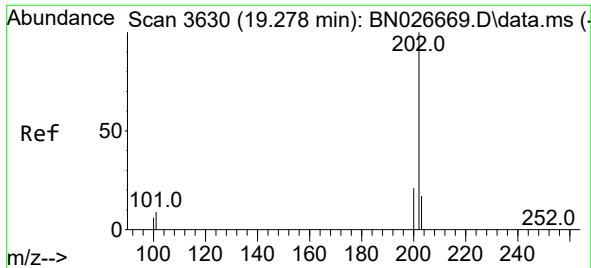


#19
 Fluoranthene
 Concen: 1.532 ng/uI
 RT: 19.278 min Scan# 3630
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument :
 BNA_N
 ClientSampleId :



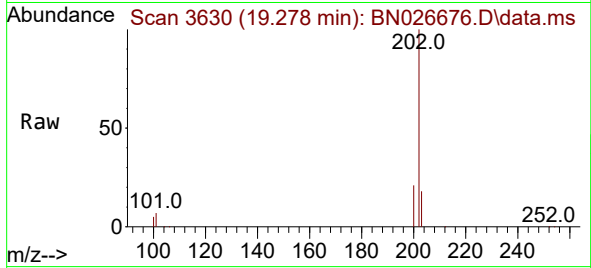



Tgt Ion:202 Resp: 94210
 Ion Ratio Lower Upper
 202 100
 101 6.9 7.0 10.4#
 100 5.3 6.0 9.0#

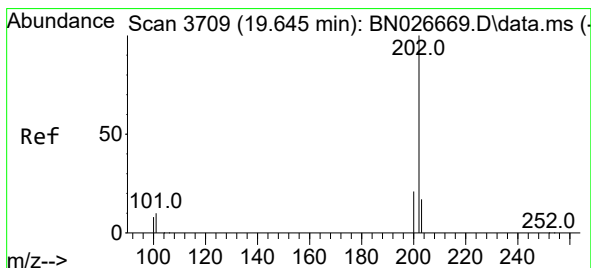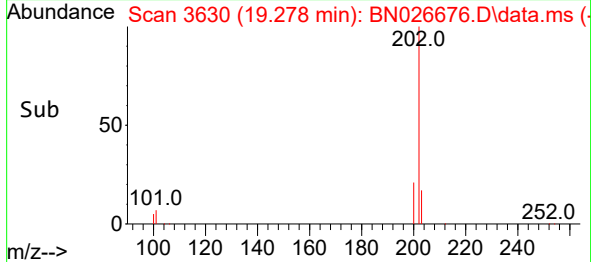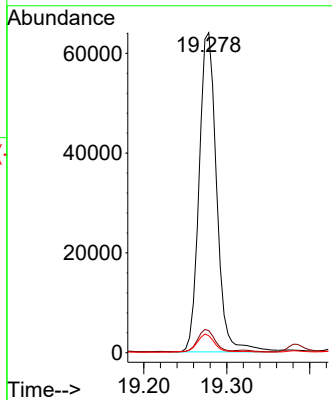

#20
 Pyrene
 Concen: 0.258 ng/uI
 RT: 19.641 min Scan# 3708
 Delta R.T. -0.005 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42


Tgt Ion:202 Resp: 17229
 Ion Ratio Lower Upper
 202 100
 101 9.4 8.0 12.0
 100 7.7 6.2 9.2

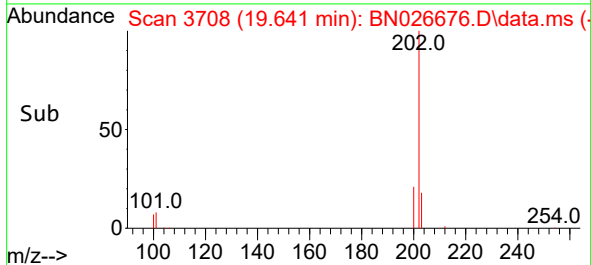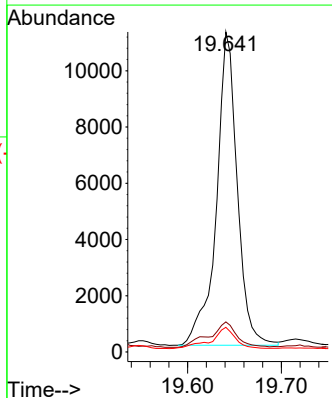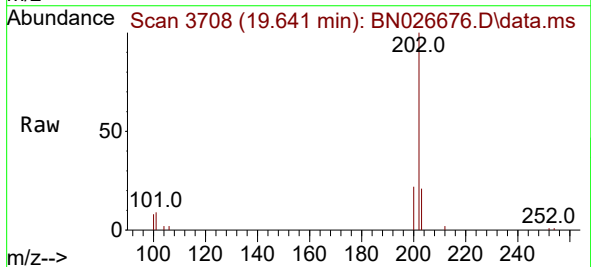

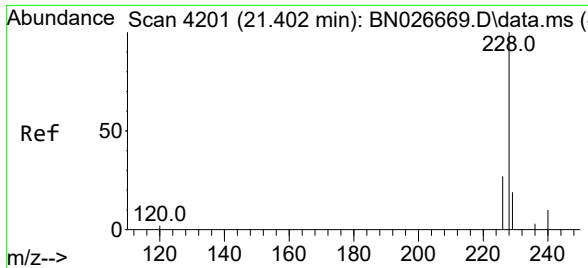




#21
 Benzo(a)anthracene
 Concen: 0.639 ng/u1
 RT: 21.402 min Scan# 419
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument : BNA_N
 ClientSampleId :

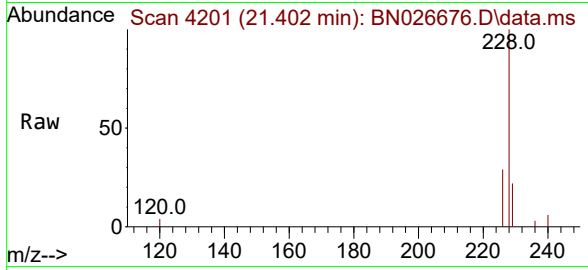


Tgt Ion:228 Resp: 30809

Ion	Ratio	Lower	Upper
228	100		
229	22.1	16.7	25.1
226	28.5	23.5	35.3

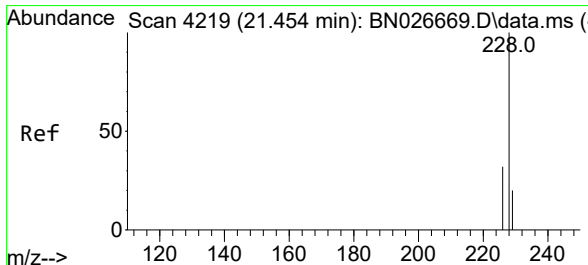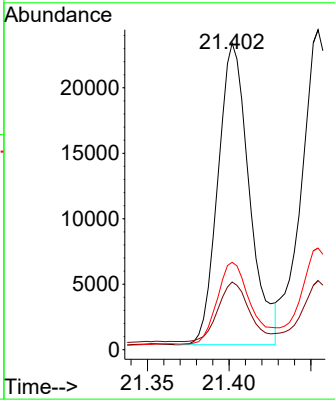
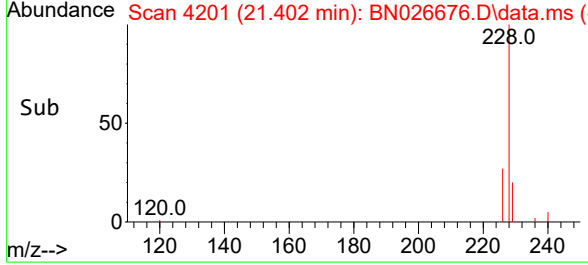



#22
 Chrysene
 Concen: 0.606 ng/u1
 RT: 21.454 min Scan# 4219
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

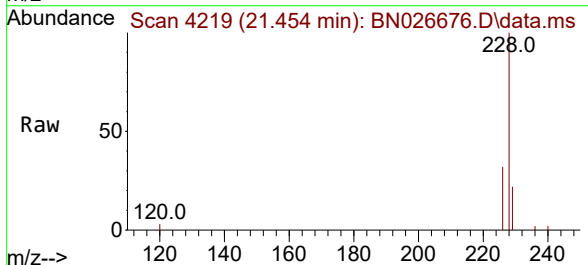

Tgt Ion:228 Resp: 33244


Ion	Ratio	Lower	Upper
228	100		
226	31.8	25.2	37.8
229	21.6	16.4	24.6

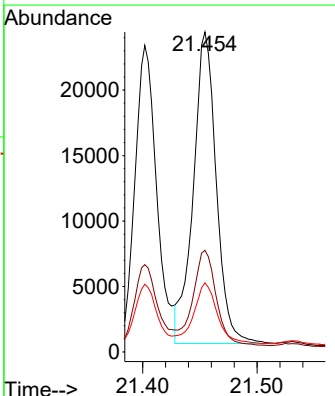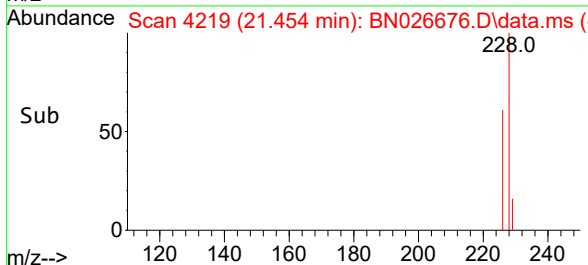



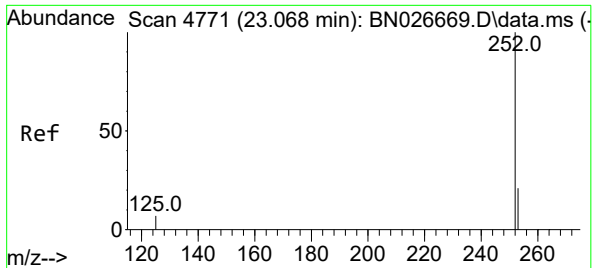


#24
 Benzo(b)fluoranthene
 Concen: 0.865 ng/u1
 RT: 23.074 min Scan# 4773
 Delta R.T. 0.006 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument : BNA_N
 ClientSampleId :



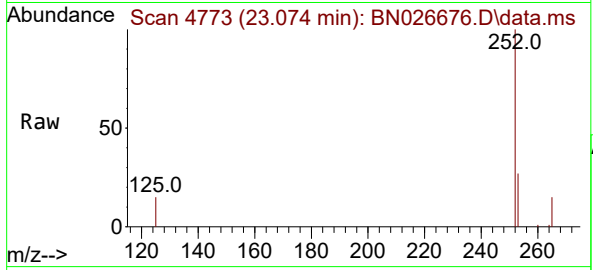



Tgt Ion:252 Resp: 37562
 Ion Ratio Lower Upper
 252 100
 253 27.4 0.0 68.6
 125 14.8 0.0 34.0

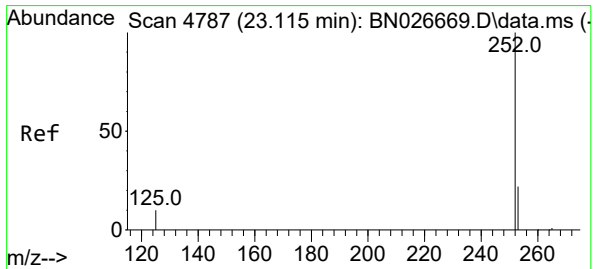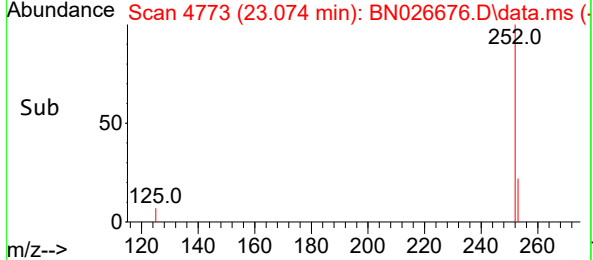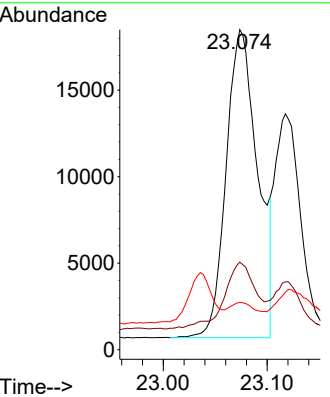

#25
 Benzo(k)fluoranthene
 Concen: 0.487 ng/u1
 RT: 23.117 min Scan# 4788
 Delta R.T. 0.003 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Tgt Ion:252 Resp: 22147
 Ion Ratio Lower Upper
 252 100
 253 28.8 27.2 40.8
 125 24.4 13.4 20.2#

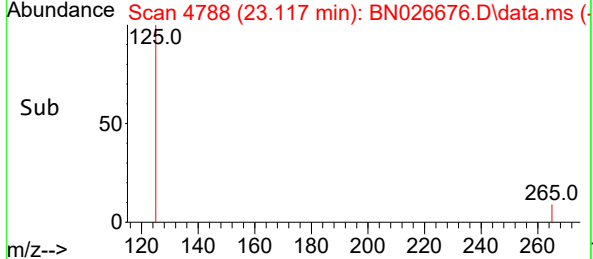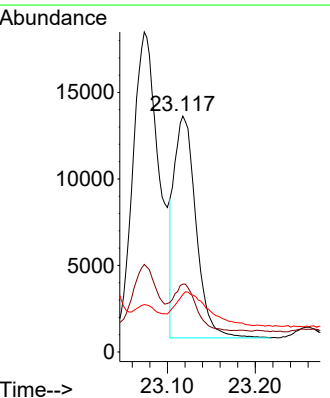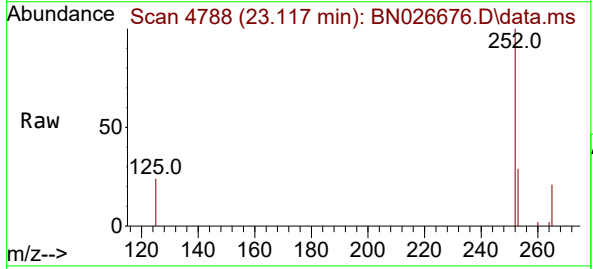




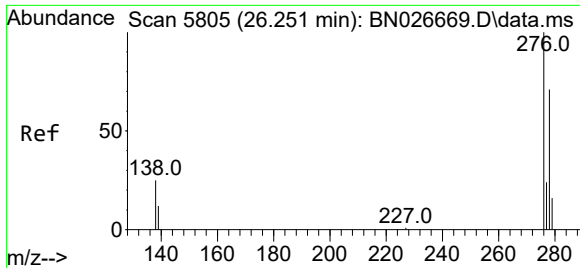


#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.136 ng/uI
 RT: 26.254 min Scan# 5806
 Delta R.T. 0.003 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Instrument : BNA_N
 ClientSampleId :

Tgt Ion:276 Resp: 6883

Ion	Ratio	Lower	Upper
276	100		
138	22.6	22.2	33.4
227	1.9	0.1	0.1#

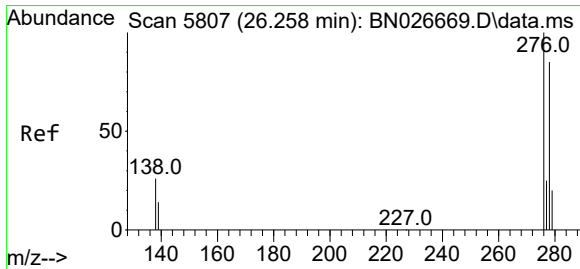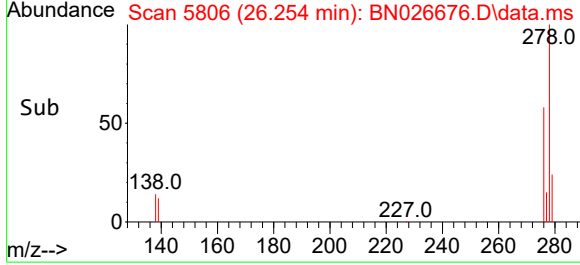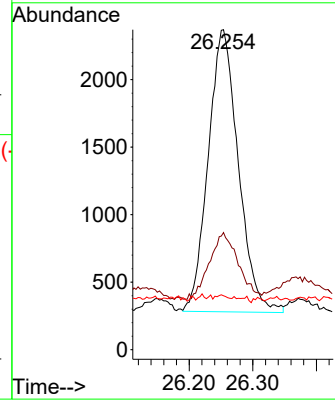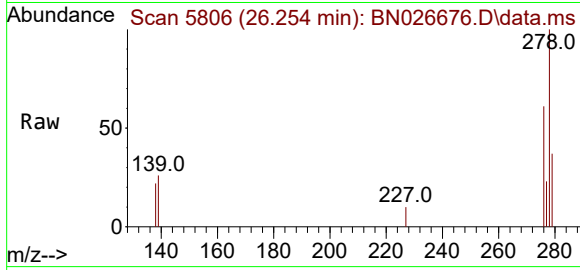

#28
 Dibenzo(a,h)anthracene
 Concen: 0.319 ng/uI
 RT: 26.257 min Scan# 5807
 Delta R.T. -0.000 min
 Lab File: BN026676.D
 Acq: 23 Jul 2023 14:42

Tgt Ion:278 Resp: 12400

Ion	Ratio	Lower	Upper
278	100		
139	25.5	18.9	28.3
279	36.8	31.3	46.9

