

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026685.D
 Acq On : 23 Jul 2023 20:47
 Operator : MA/JU
 Sample : PB154169BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 24 00:42:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	2743	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	9429	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	6038	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	12310	0.400	ng/ul	0.00
17) Chrysene-d12	21.416	240	7271	0.400	ng/ul	0.00
23) Perylene-d12	23.781	264	9896	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.195	96	18809	5.207	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.231	152	4368	0.341	ng/ul	0.01
18) Fluoranthene-d10	19.246	212	9534	0.378	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.608	202	1588	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.623	252	3192	0.093	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026685.D
Acq On : 23 Jul 2023 20:47
Operator : MA/JU
Sample : PB154169BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 24 00:42:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

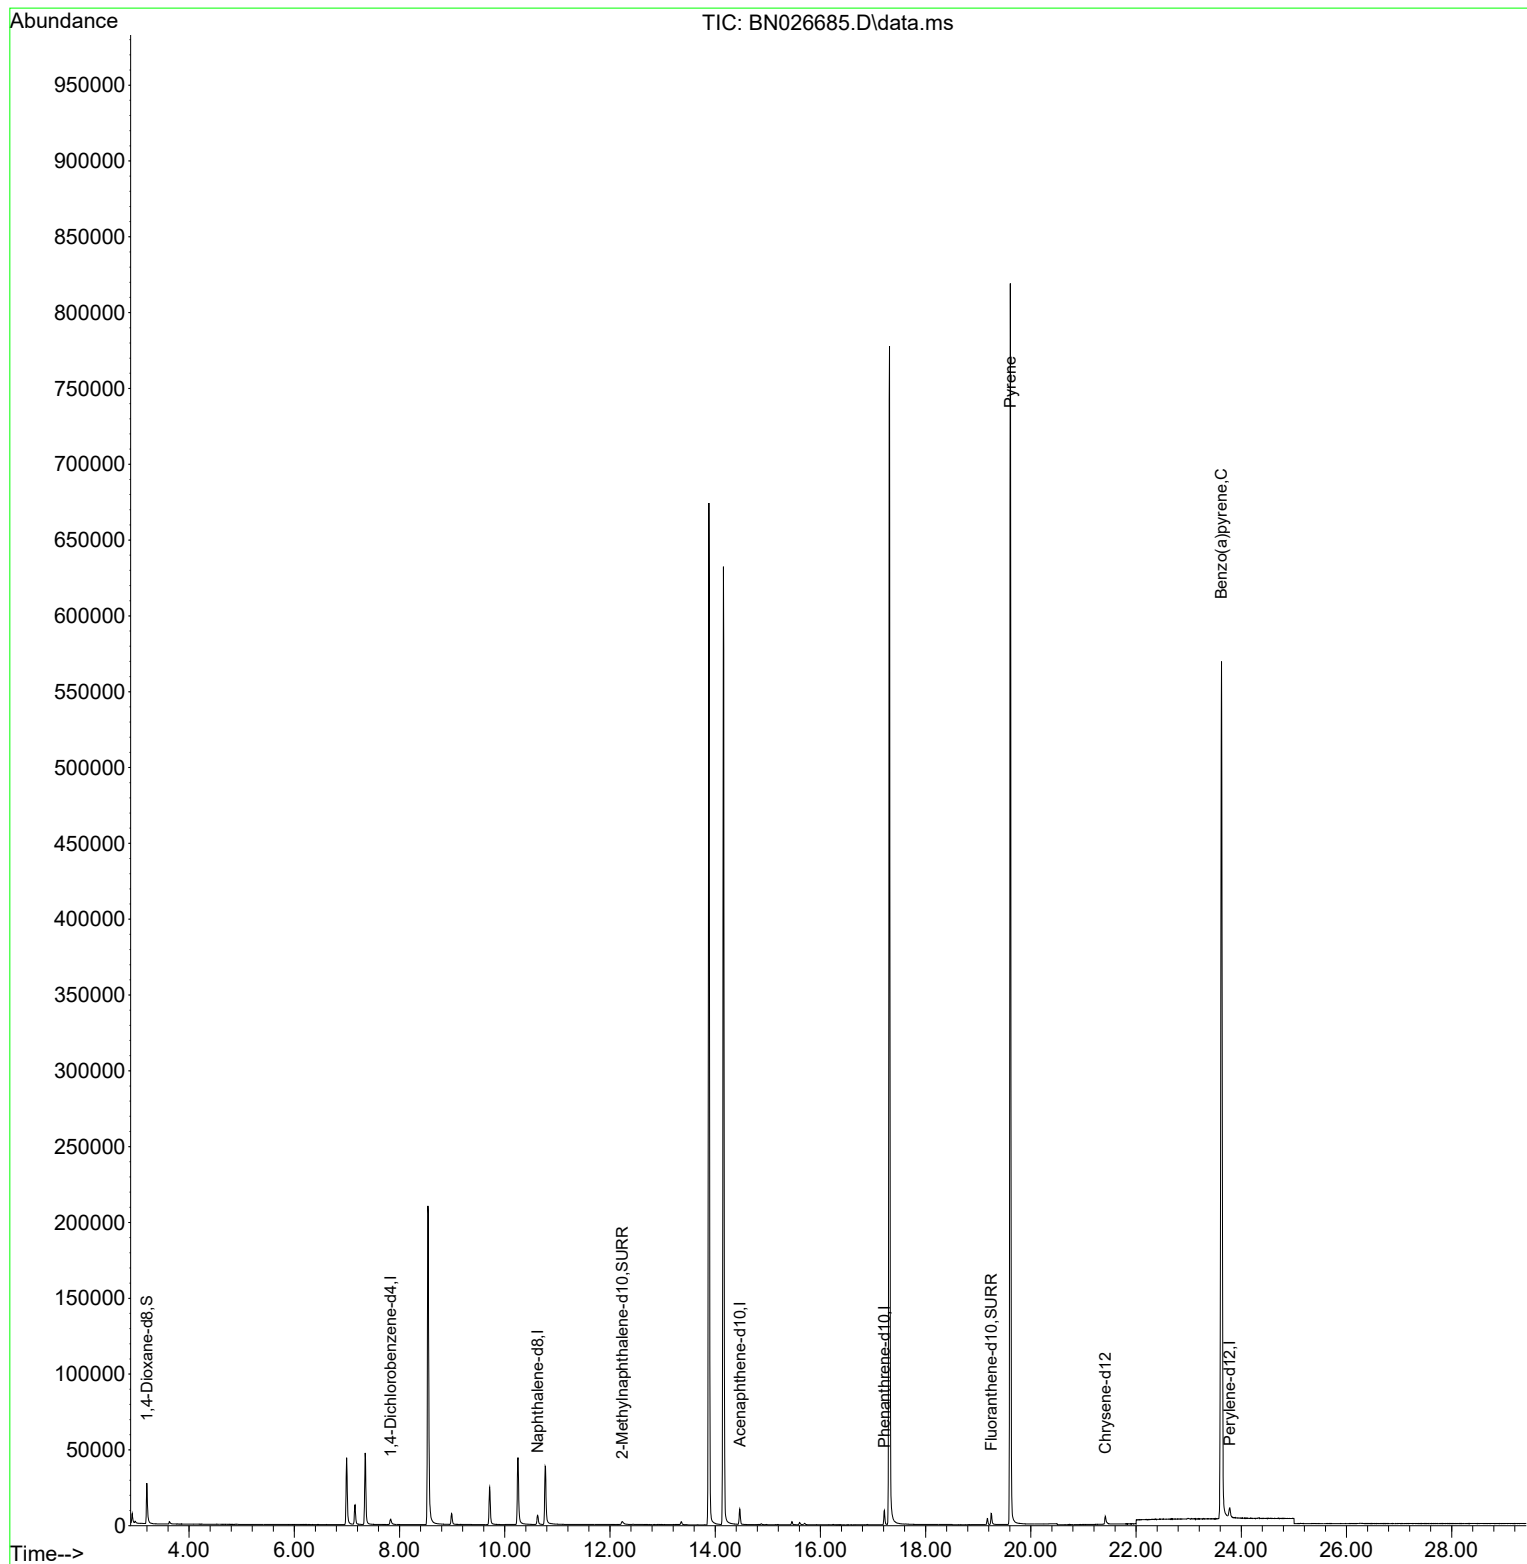

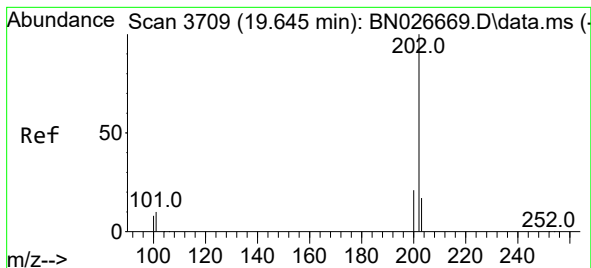

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.608 min Scan# 31

Delta R.T. -0.037 min


Lab File: BN026685.D

Acq: 23 Jul 2023 20:47

Instrument :

BNA_N

ClientSampleId :

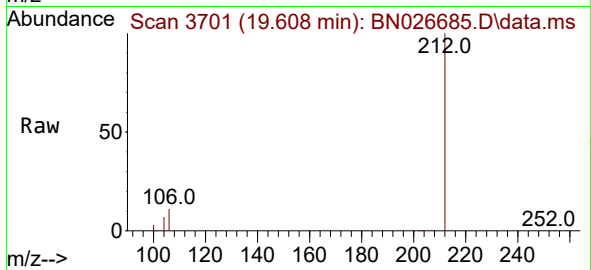




Tgt Ion:202 Resp: 1588

Ion Ratio Lower Upper

202 100

101 208.4 8.0 12.0#

100 1693.2 6.2 9.2#

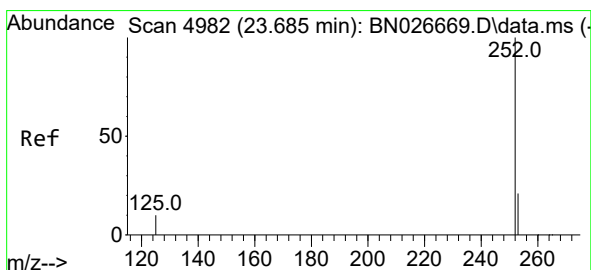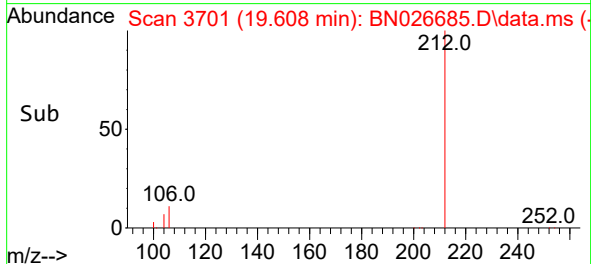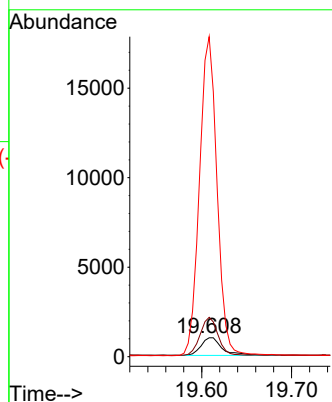

#26

Benzo(a)pyrene

Concen: 0.093 ng/ul

RT: 23.623 min Scan# 4961

Delta R.T. -0.061 min

Lab File: BN026685.D

Acq: 23 Jul 2023 20:47

Tgt Ion:252 Resp: 3192

Ion Ratio Lower Upper

252 100

253 62.6 32.6 49.0#

125 57.1 19.3 28.9#

