

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026690.D
 Acq On : 23 Jul 2023 23:49
 Operator : MA/JU
 Sample : 03472-25RE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 24 00:43:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.823	152	2541	0.400	ng/ul	0.00
4) Naphthalene-d8	10.619	136	8204	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.462	164	5319	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	11378	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.411	240	7624	0.400	ng/ul	# 0.00
23) Perylene-d12	23.778	264	8679	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.195	96	13258	3.962	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.220	152	6290	0.564	ng/ul	0.00
18) Fluoranthene-d10	19.246	212	14686	0.556	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.457	166	1946	0.093	ng/ul#	14
20) Pyrene	19.608	202	1941	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.617	252	2045	0.068	ng/ul#	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026690.D
Acq On : 23 Jul 2023 23:49
Operator : MA/JU
Sample : 03472-25RE
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 24 00:43:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

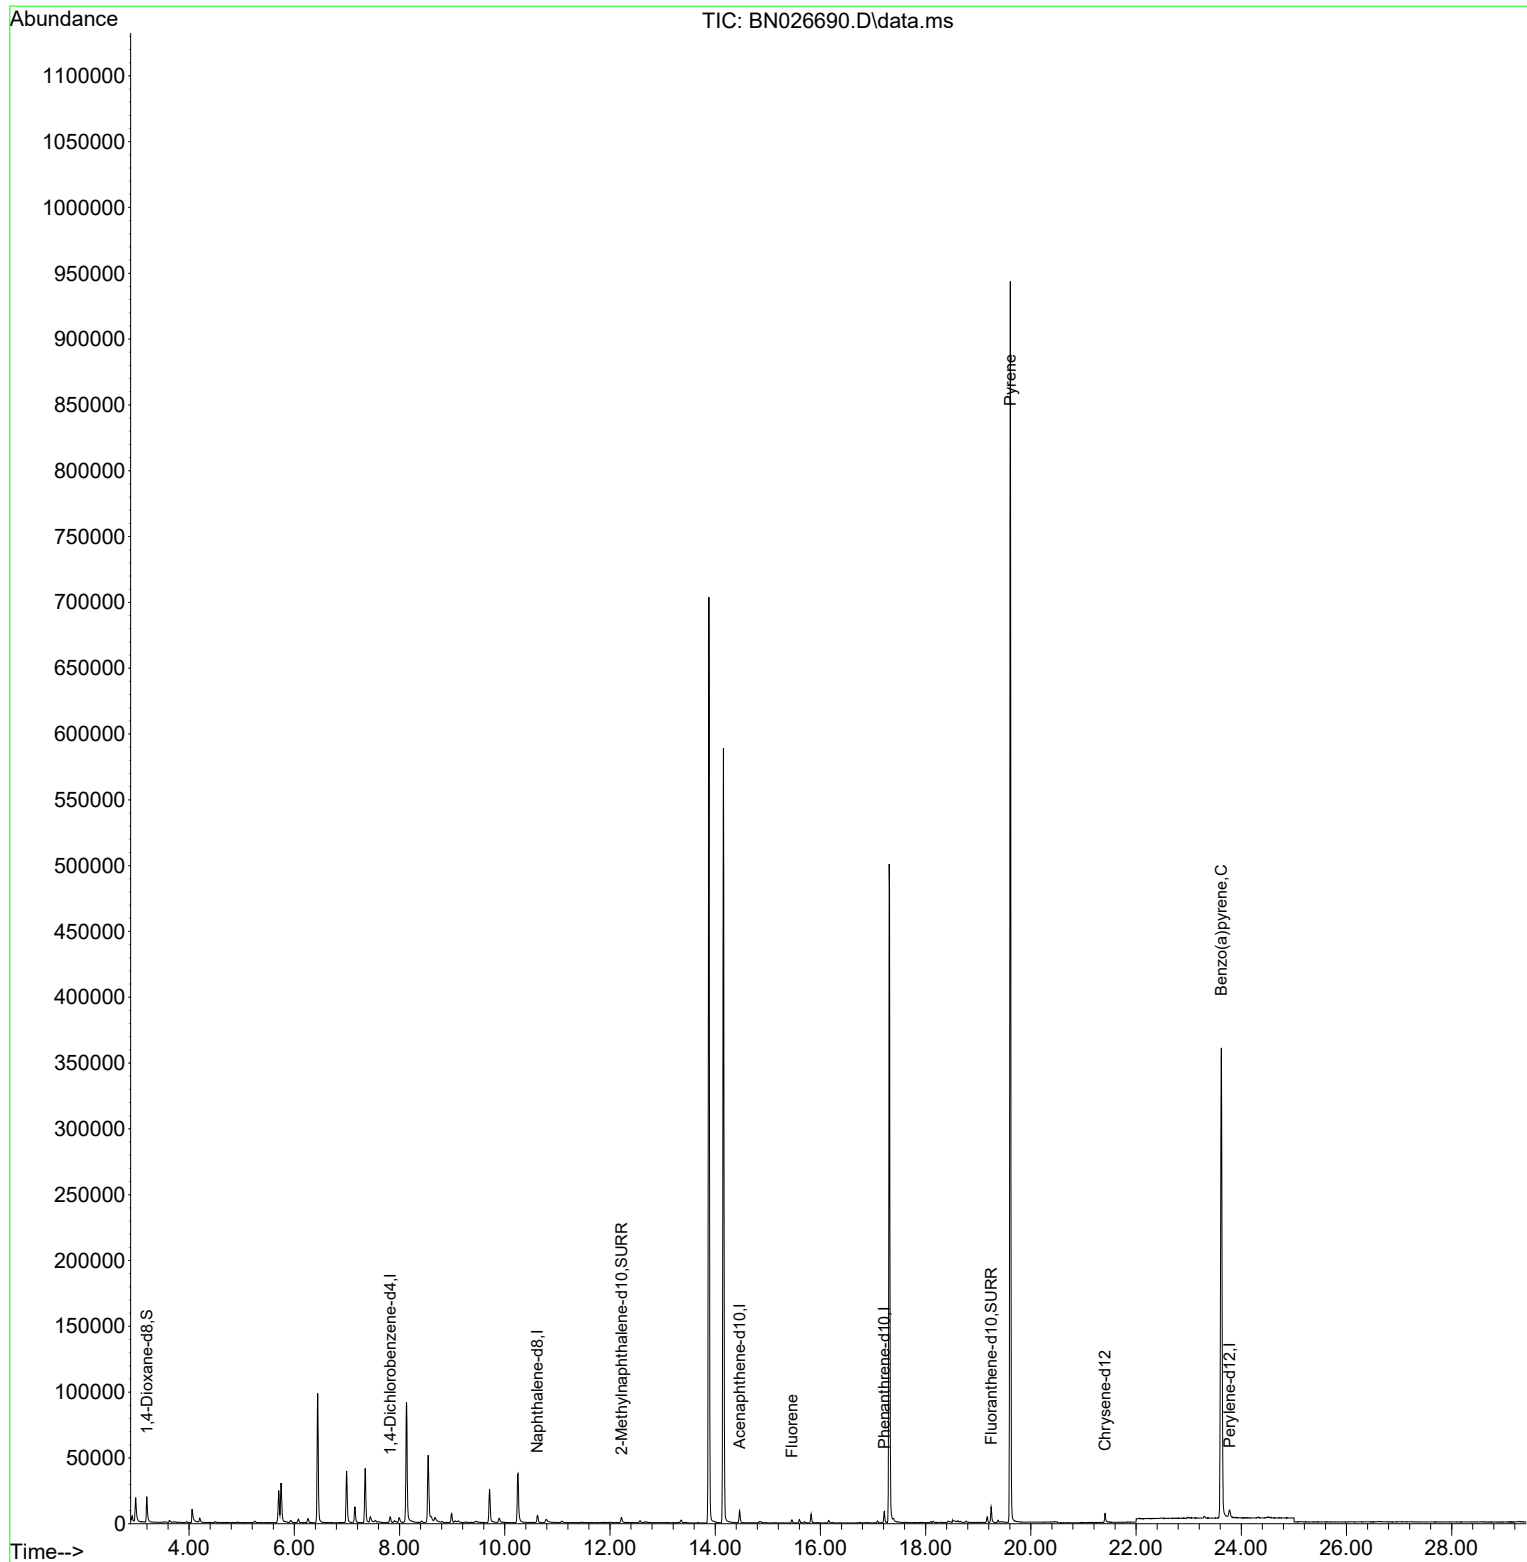



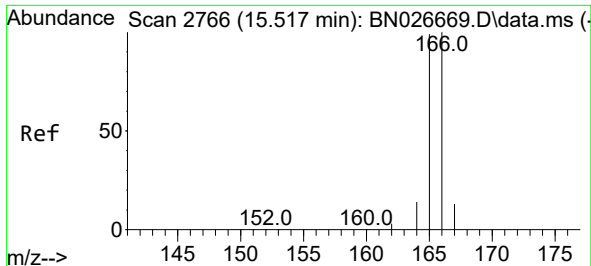


#12
Fluorene
Concen: 0.093 ng/ul
RT: 15.457 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN026690.D
Acq: 23 Jul 2023 23:49

Instrument :
BNA_N
ClientSampleId :



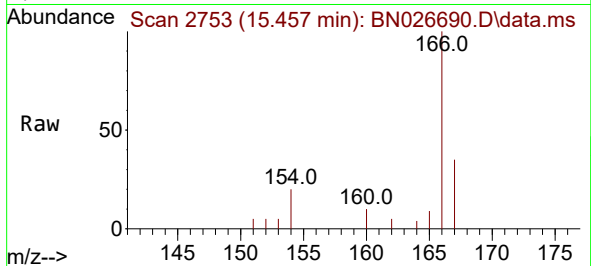



Tgt Ion:166 Resp: 1946
Ion Ratio Lower Upper
166 100
165 9.0 80.6 120.8#
167 35.0 12.0 18.0#

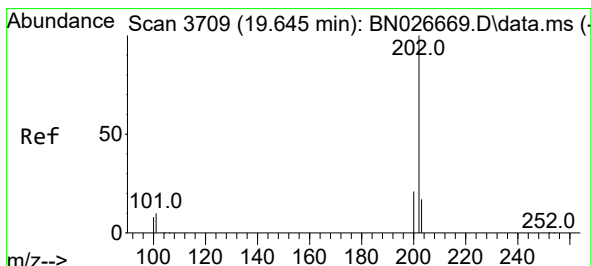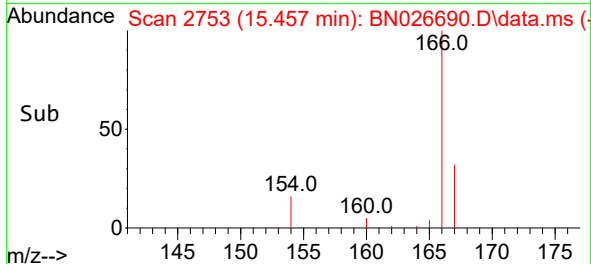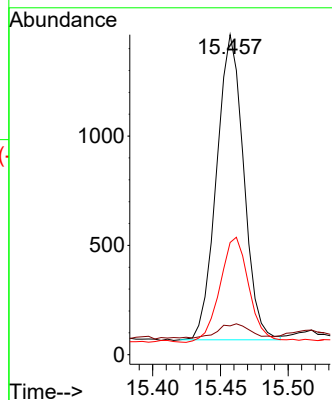

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.608 min Scan# 3701
Delta R.T. -0.037 min
Lab File: BN026690.D
Acq: 23 Jul 2023 23:49


Tgt Ion:202 Resp: 1941
Ion Ratio Lower Upper
202 100
101 204.1 8.0 12.0#
100 1671.8 6.2 9.2#

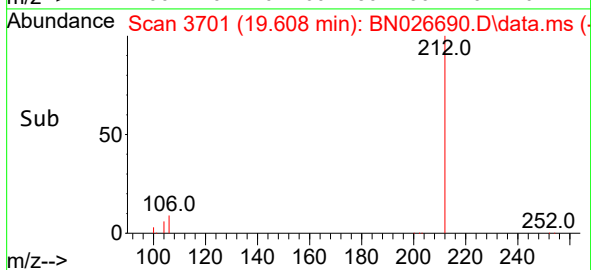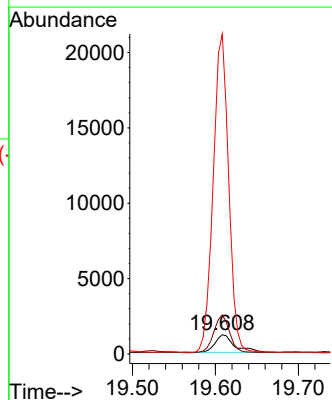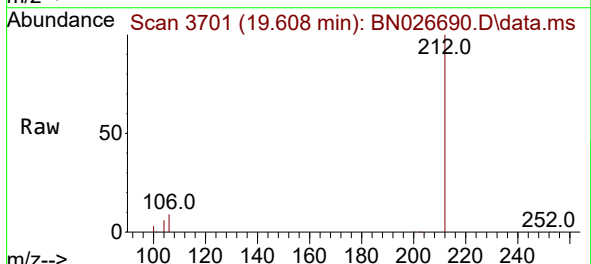

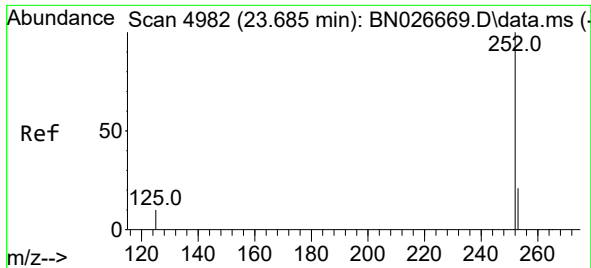

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.617 min Scan# 49
Delta R.T. -0.067 min
Lab File: BN026690.D
Acq: 23 Jul 2023 23:49

Instrument :
BNA_N
ClientSampleId :

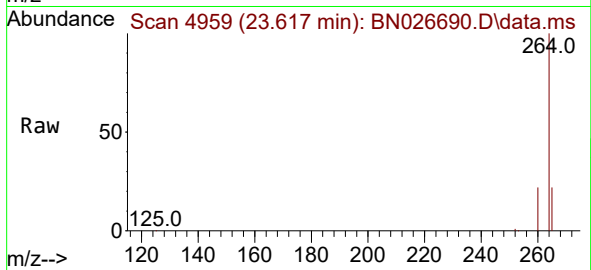

Tgt Ion:252 Resp: 2045
Ion Ratio Lower Upper
252 100
253 77.6 32.6 49.0#
125 82.3 19.3 28.9#

