




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

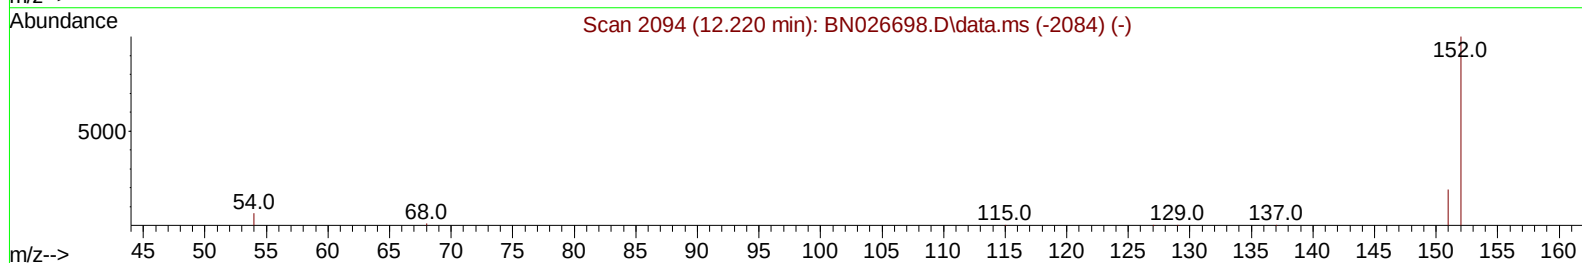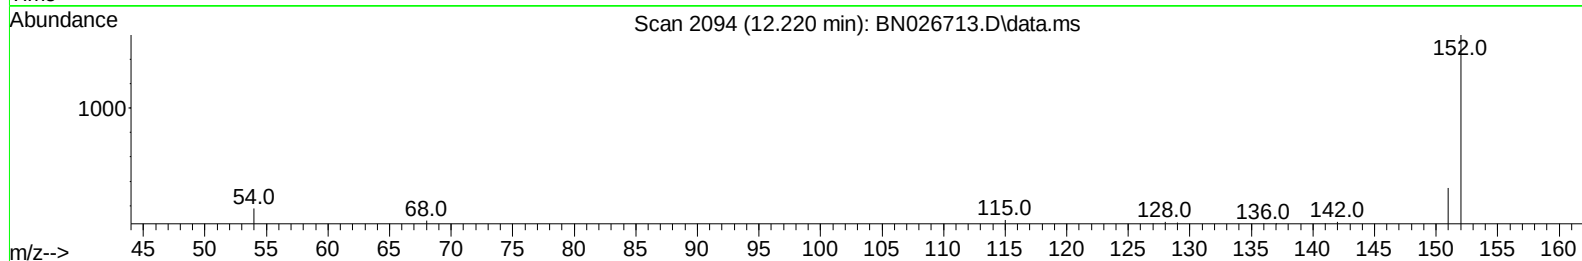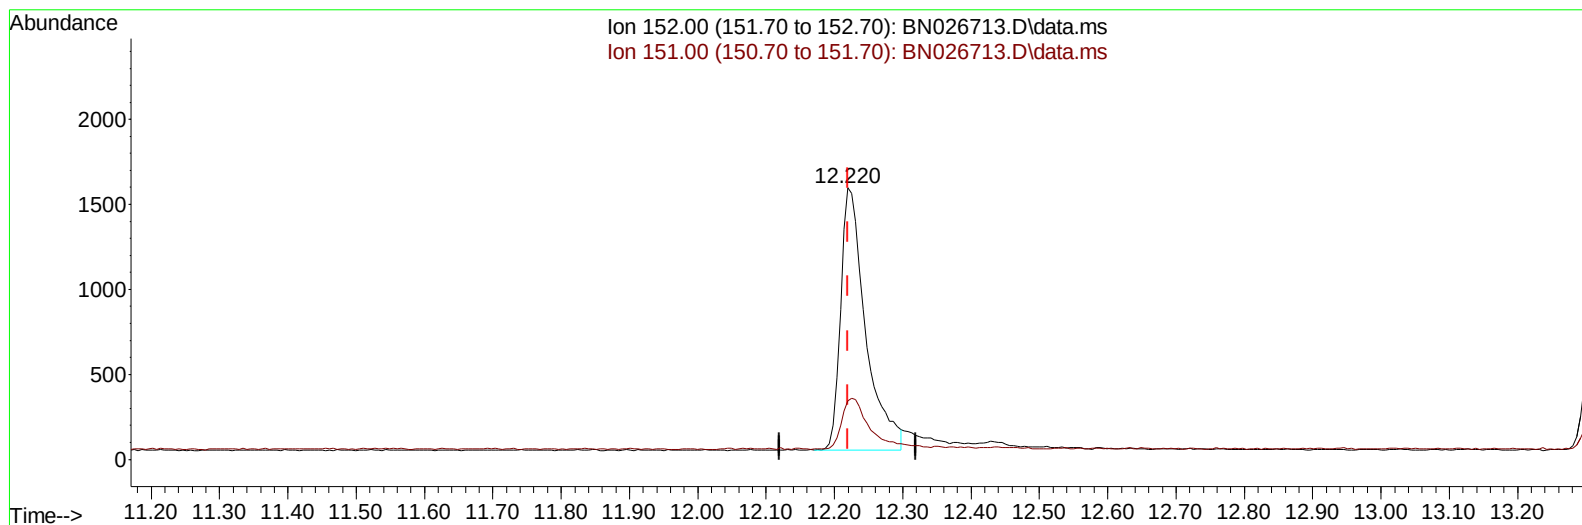

TIC: BN026713.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.220min (+ 0.000) 0.44 ng/u1

response 3926

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	20.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

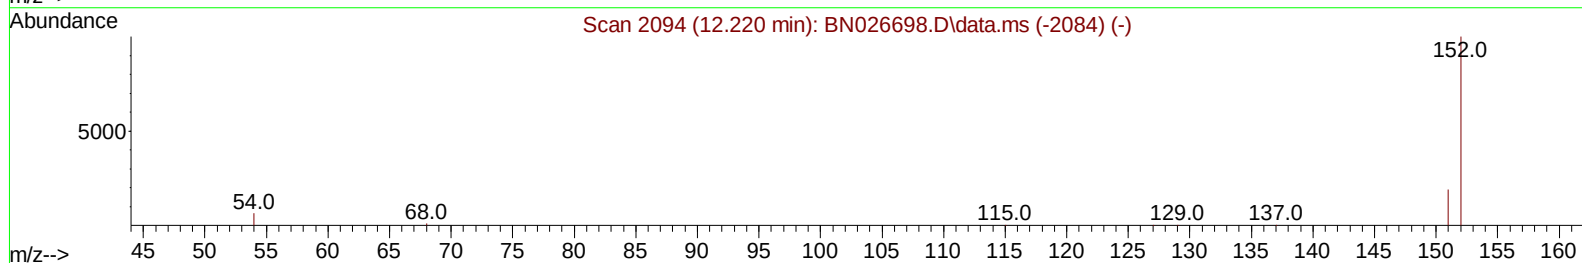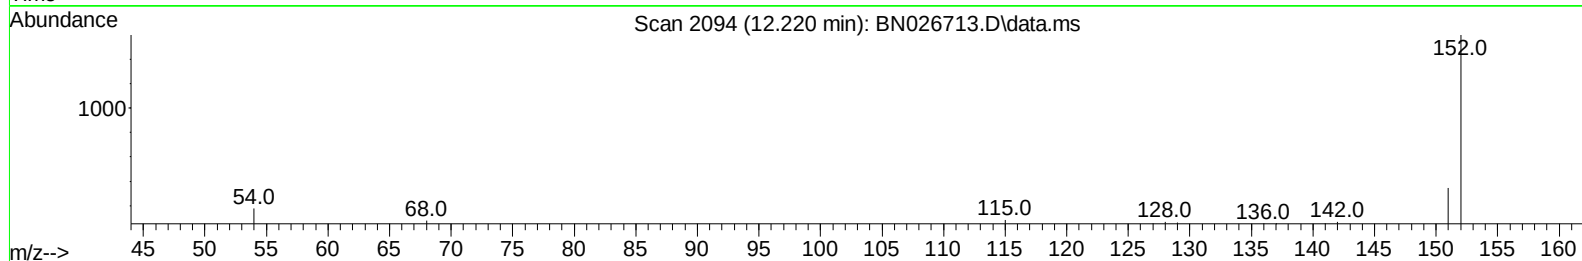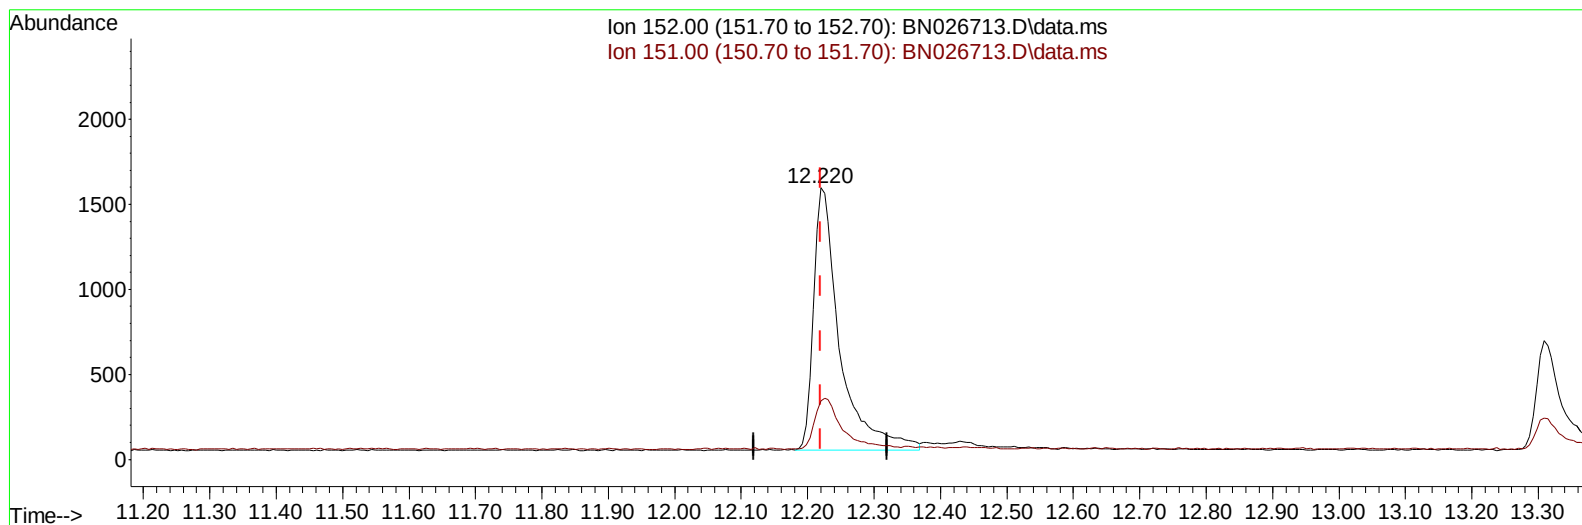

TIC: BN026713.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.220min (+ 0.000) 0.48 ng/ul m

response 4243

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	18.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

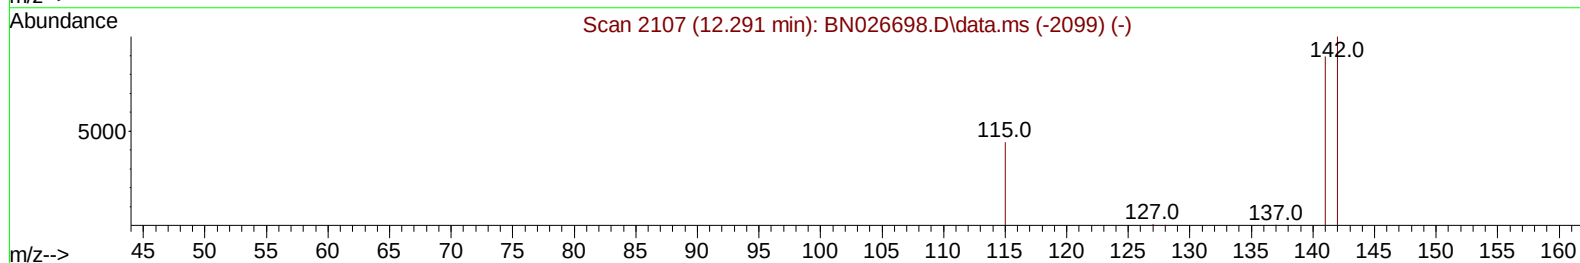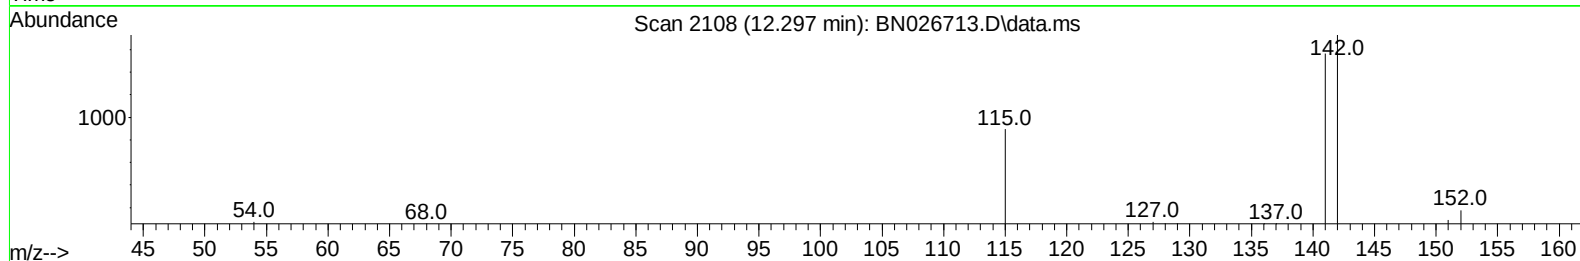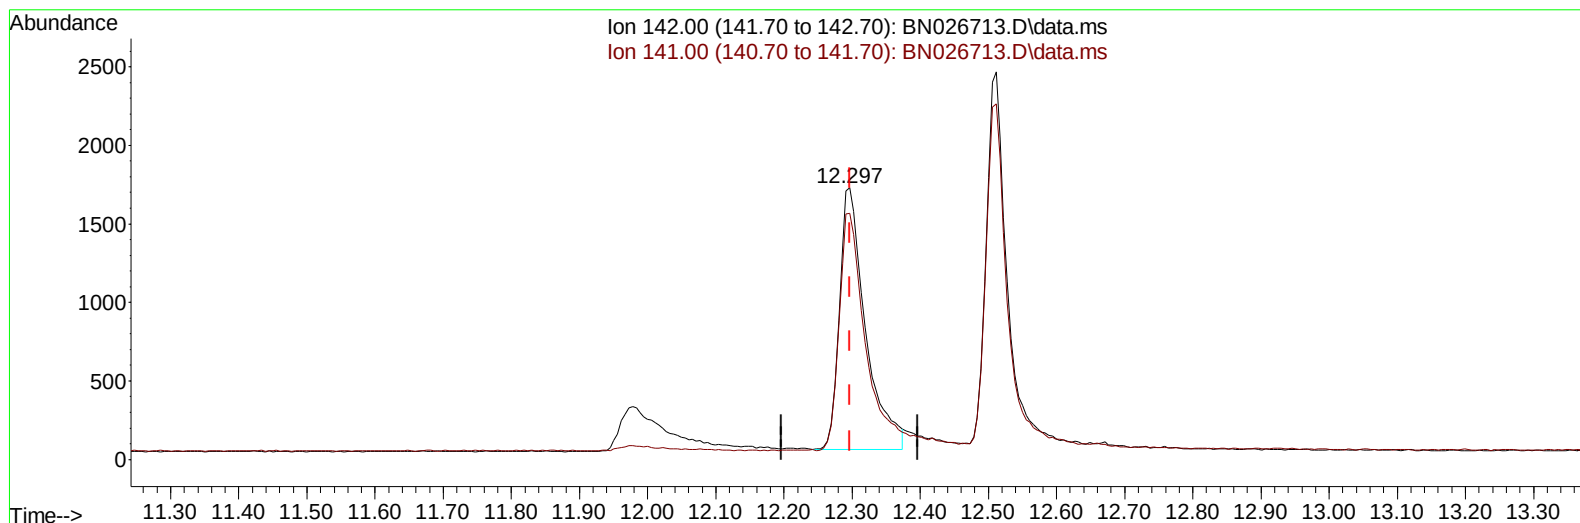

TIC: BN026713.D\data.ms

(7) 2-Methylnaphthalene

12.297min (+ 0.000) 0.44 ng/ul

response 4433

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.40	91.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026713.D
Acq On : 24 Jul 2023 14:39
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

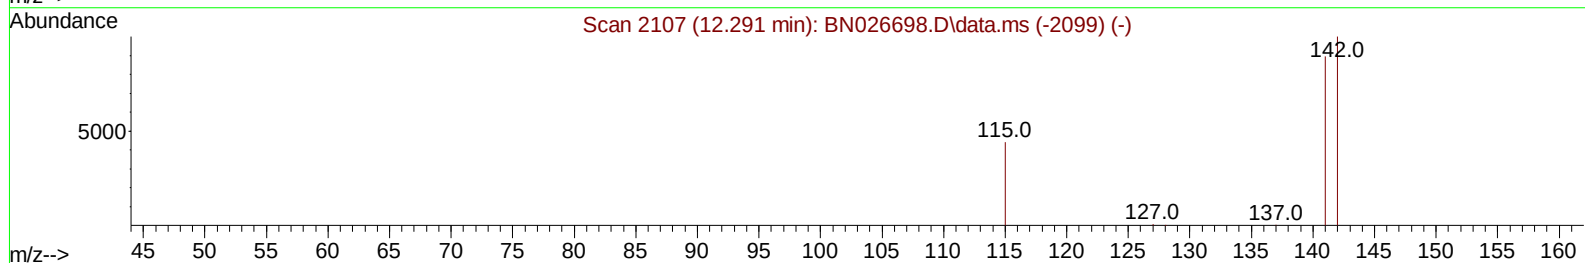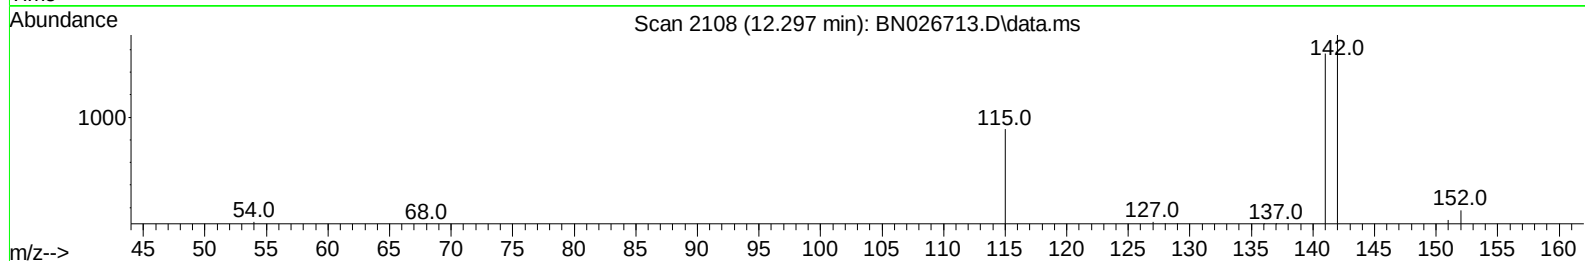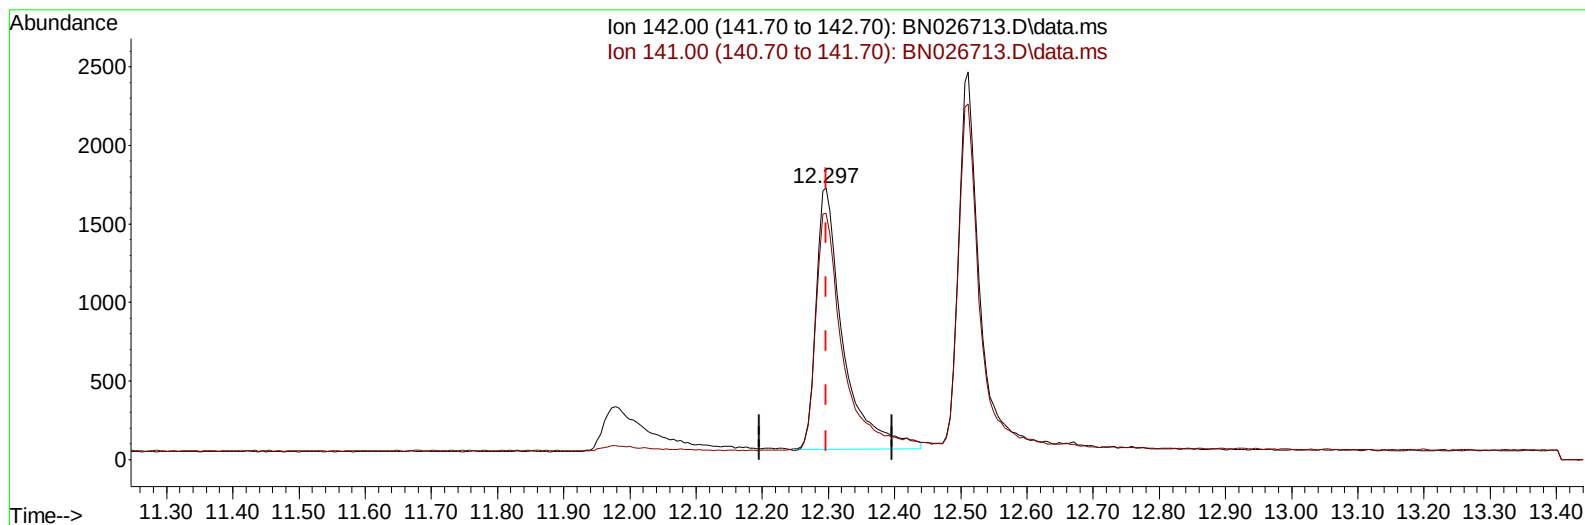

TIC: BN026713.D\data.ms

(7) 2-Methylnaphthalene

12.297min (+ 0.000) 0.46 ng/ul m

response 4723

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	90.40	85.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

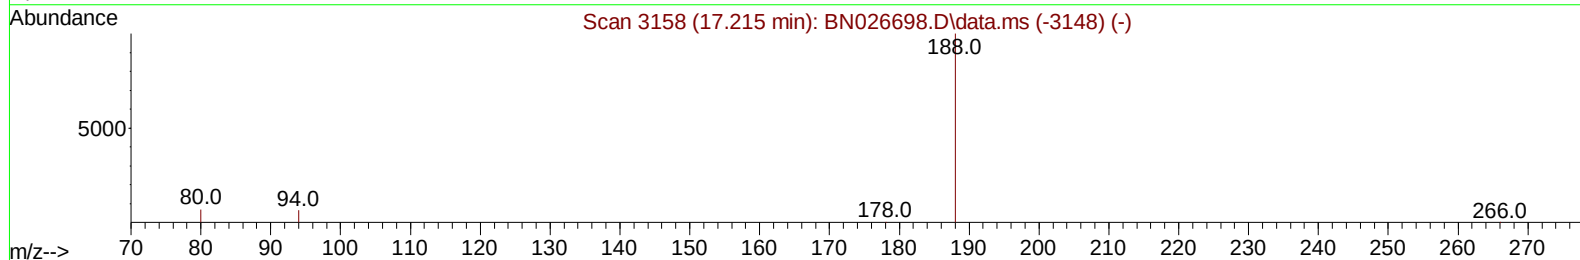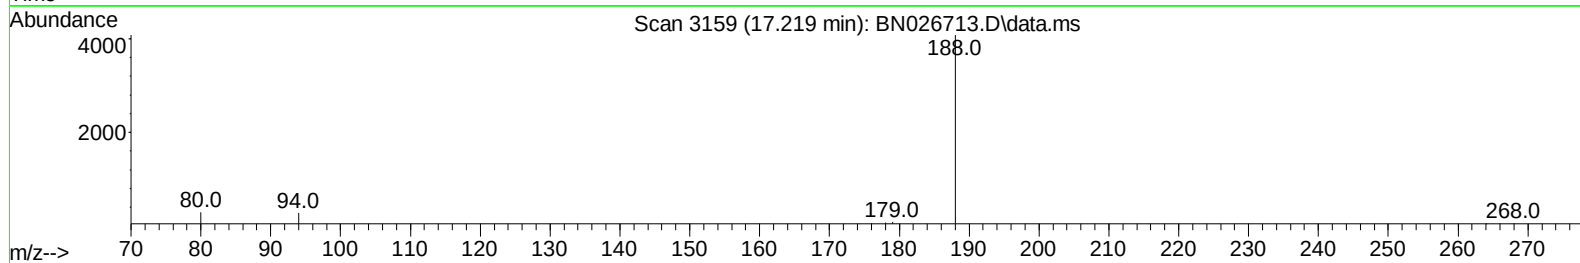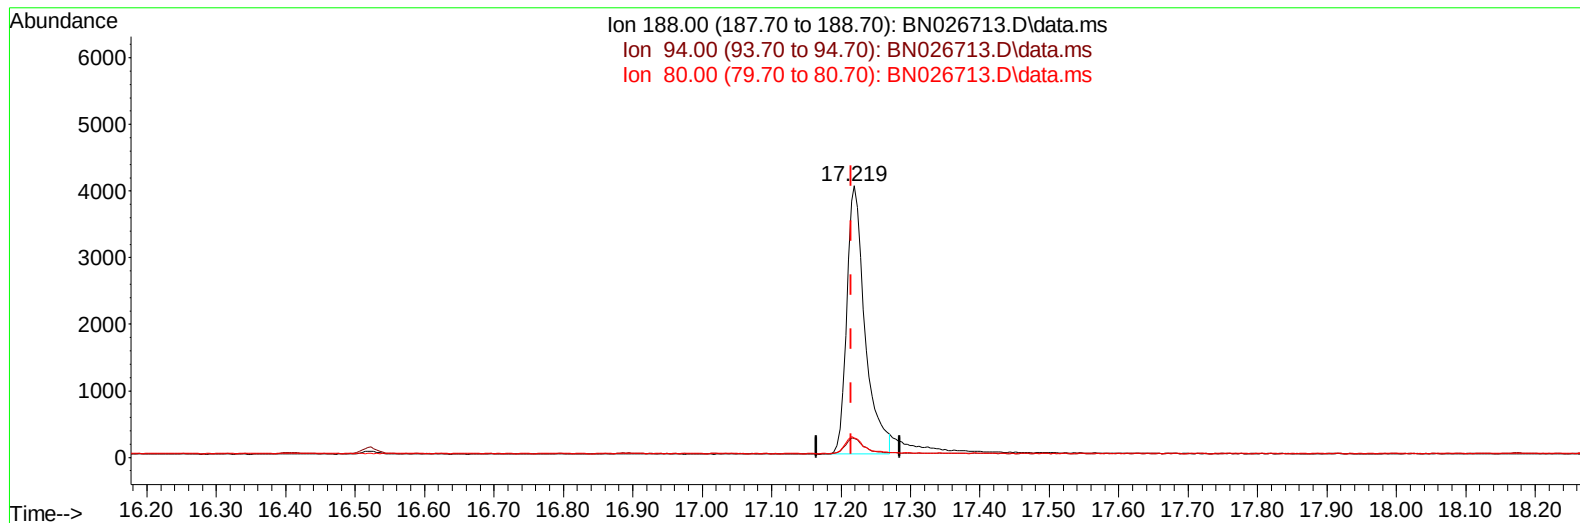

TIC: BN026713.D\data.ms

(13) Phenanthrene-d10 (I)

17.219min (+ 0.004) 0.40 ng/u1

response 7370

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.20	7.01#
80.00	9.40	7.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

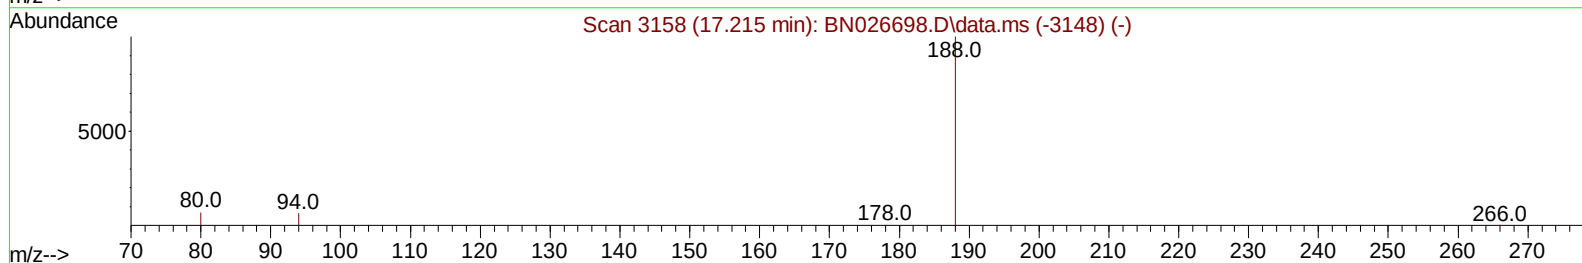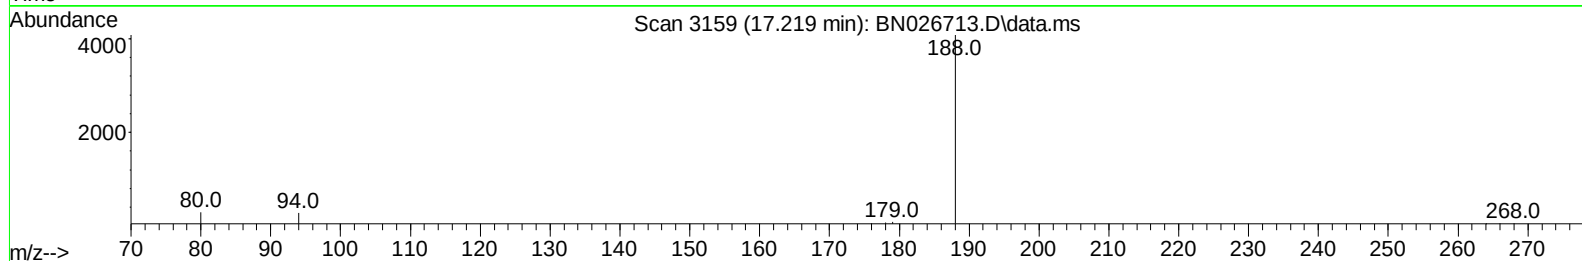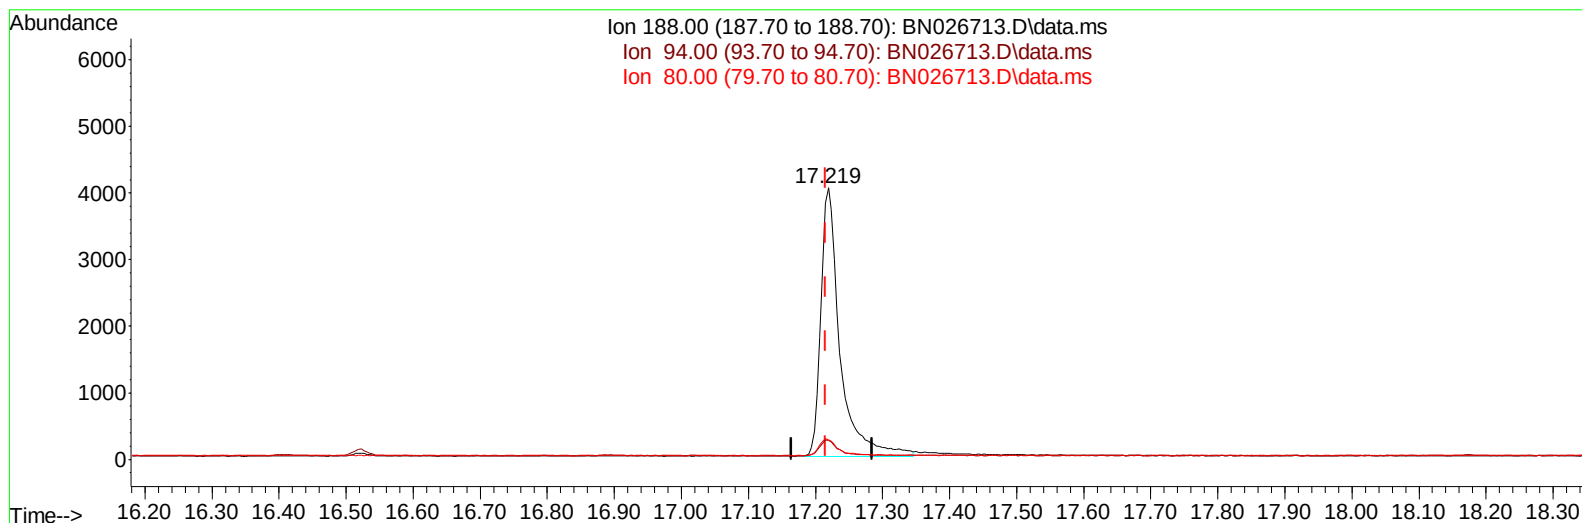

TIC: BN026713.D\data.ms

(13) Phenanthrene-d10 (I)

17.219min (+ 0.004) 0.40 ng/ul m

response 8002

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.20	7.01#
80.00	9.40	7.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

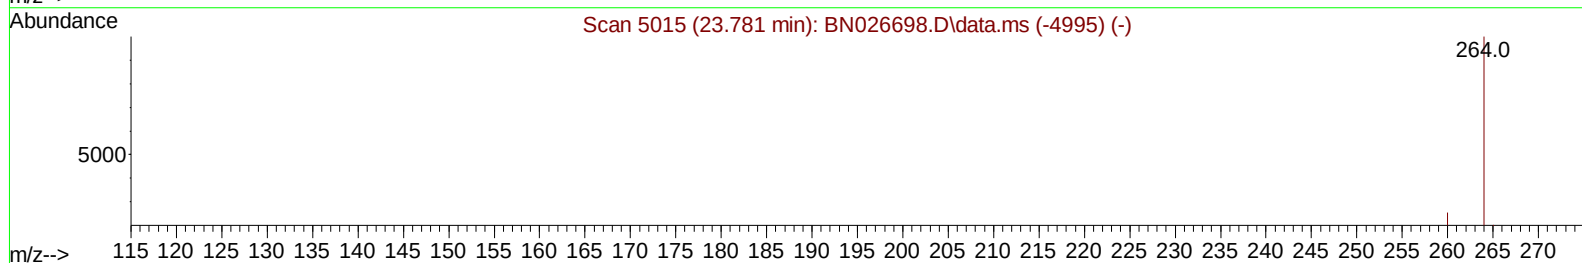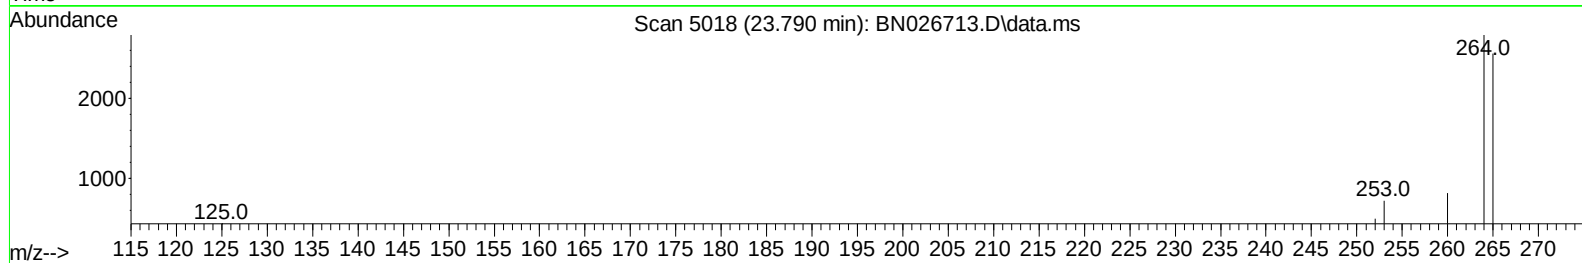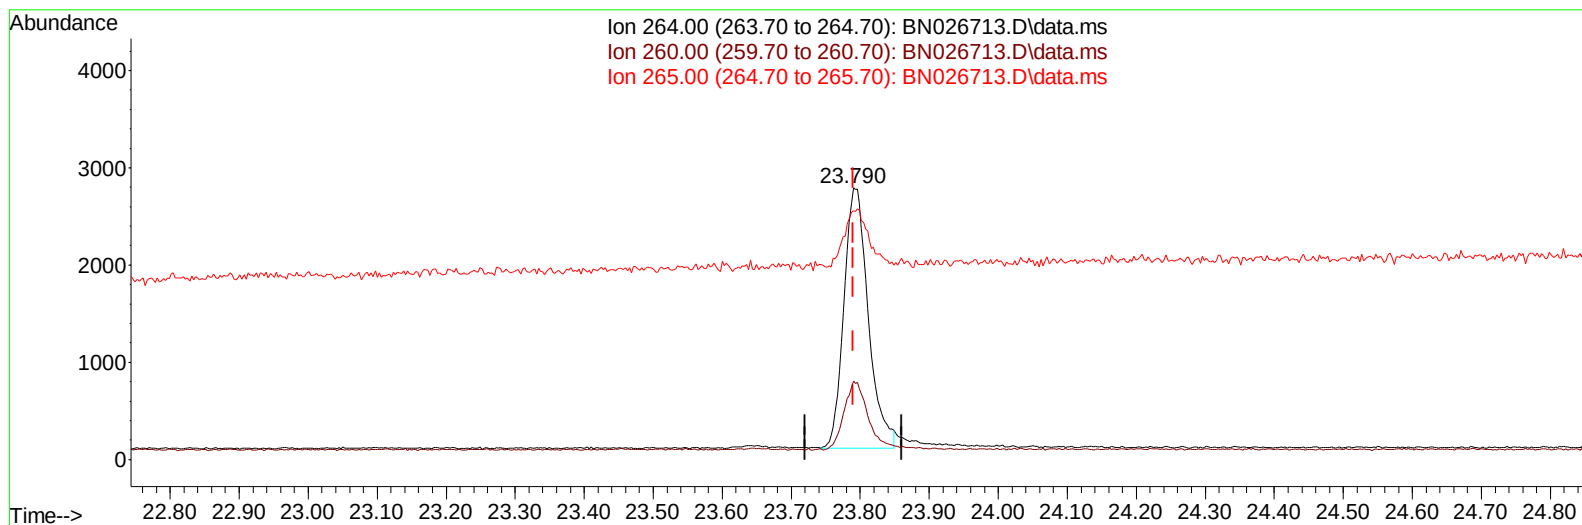

TIC: BN026713.D\data.ms

(23) Perylene-d12 (I)

23.790min (+ 0.000) 0.40 ng/ul

response 6580

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.90	29.00
265.00	117.70	91.69#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

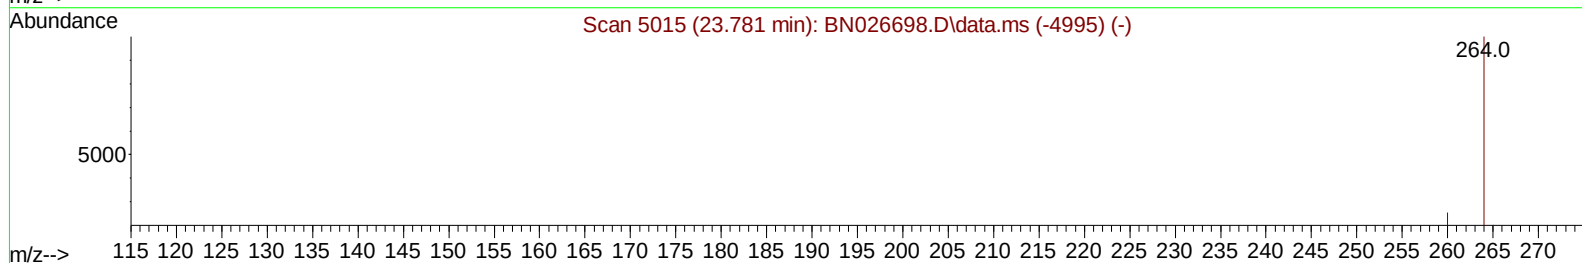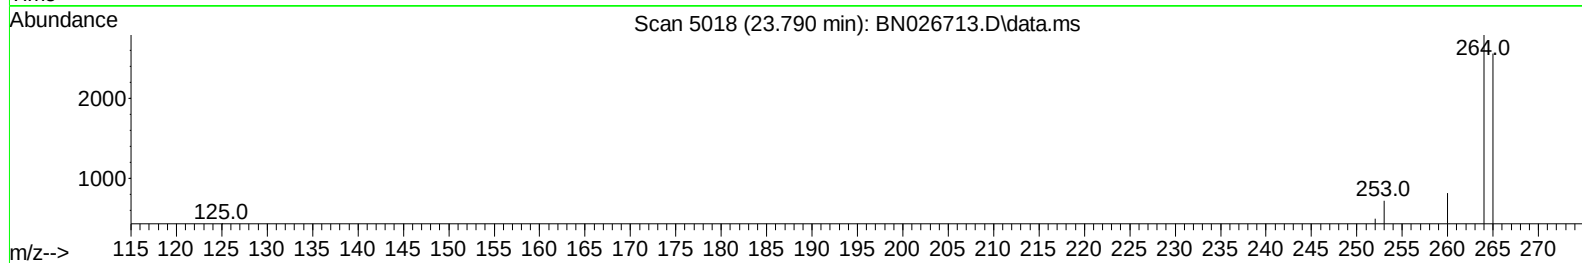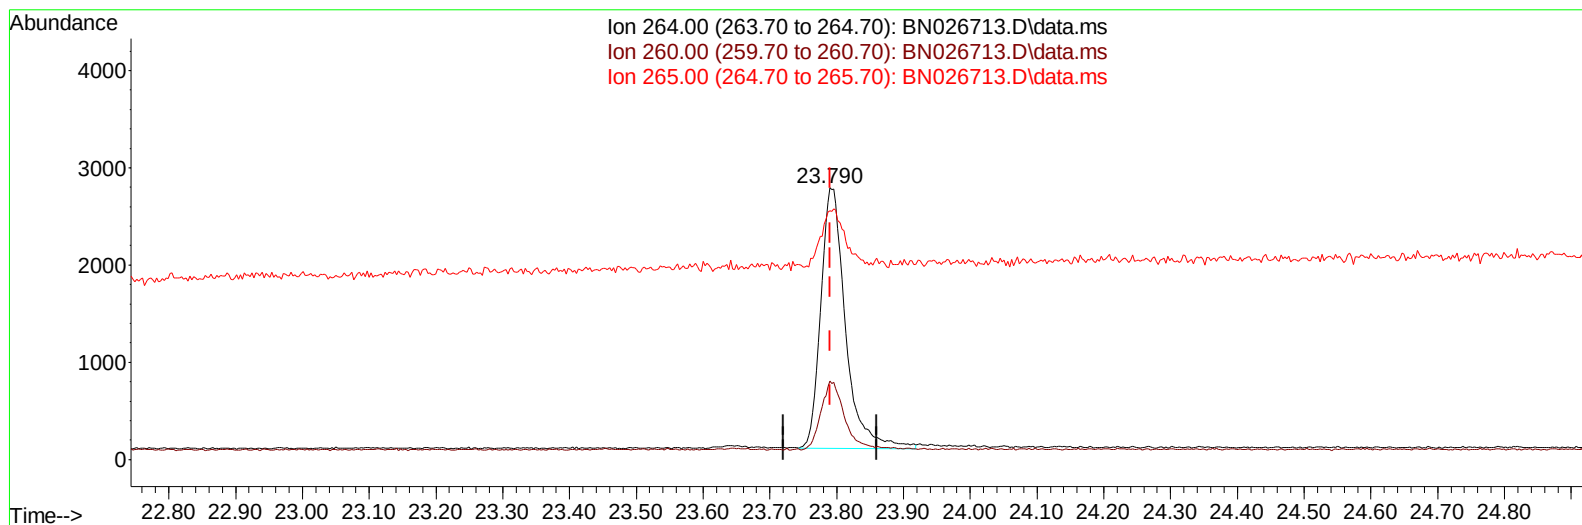

TIC: BN026713.D\data.ms

(23) Perylene-d12 (I)

23.790min (+ 0.000) 0.40 ng/ul m

response 6899

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.90	29.00
265.00	117.70	91.69#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026713.D
 Acq On : 24 Jul 2023 14:39
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.836	152	2521	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	6537	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	4155	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.219	188	8002m	0.400	ng/ul	0.00
17) Chrysene-d12	21.417	240	5260	0.400	ng/ul	# 0.00
23) Perylene-d12	23.790	264	6899m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	1102	0.332	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.220	152	4243m	0.477	ng/ul	0.00
18) Fluoranthene-d10	19.250	212	7577	0.416	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.229	88	1145	0.364	ng/ul#	86
5) Naphthalene	10.675	128	7107	0.396	ng/ul	98
7) 2-Methylnaphthalene	12.297	142	4723m	0.464	ng/ul	
8) 1-Methylnaphthalene	12.511	142	4902	0.449	ng/ul	100
10) Acenaphthylene	14.189	152	8254	0.406	ng/ul	99
11) Acenaphthene	14.527	153	6082	0.392	ng/ul	99
12) Fluorene	15.522	166	6595	0.406	ng/ul	100
14) Pentachlorophenol	16.890	266	660	0.327	ng/ul	97
15) Phenanthrene	17.262	178	9163	0.360	ng/ul	99
16) Anthracene	17.354	178	8158	0.369	ng/ul	97
19) Fluoranthene	19.278	202	9894	0.401	ng/ul#	94
20) Pyrene	19.646	202	10213	0.381	ng/ul#	94
21) Benzo(a)anthracene	21.405	228	8073	0.418	ng/ul	98
22) Chrysene	21.455	228	8395	0.382	ng/ul	98
24) Benzo(b)fluoranthene	23.071	252	9083	0.338	ng/ul	96
25) Benzo(k)fluoranthene	23.118	252	9991	0.355	ng/ul	96
26) Benzo(a)pyrene	23.691	252	8812	0.368	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	26.244	276	12597	0.402	ng/ul#	76
28) Dibenzo(a,h)anthracene	26.261	278	9972	0.414	ng/ul#	91
29) Benzo(g,h,i)perylene	27.002	276	10690	0.386	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026713.D
Acq On : 24 Jul 2023 14:39
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 24 15:17:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

