




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026714.D
Acq On : 24 Jul 2023 15:16
Operator : MA/JU
Sample : PB154169BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK169

Manual IntegrationsAPPROVED

Quant Time: Jul 24 16:13:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

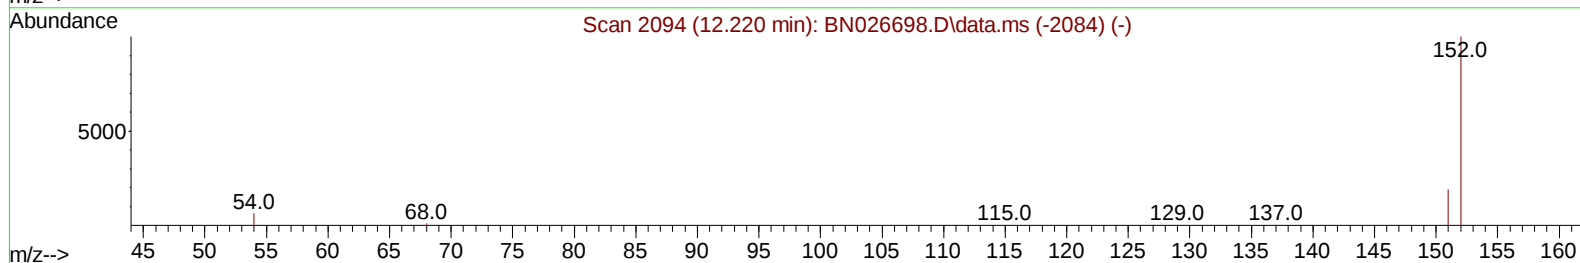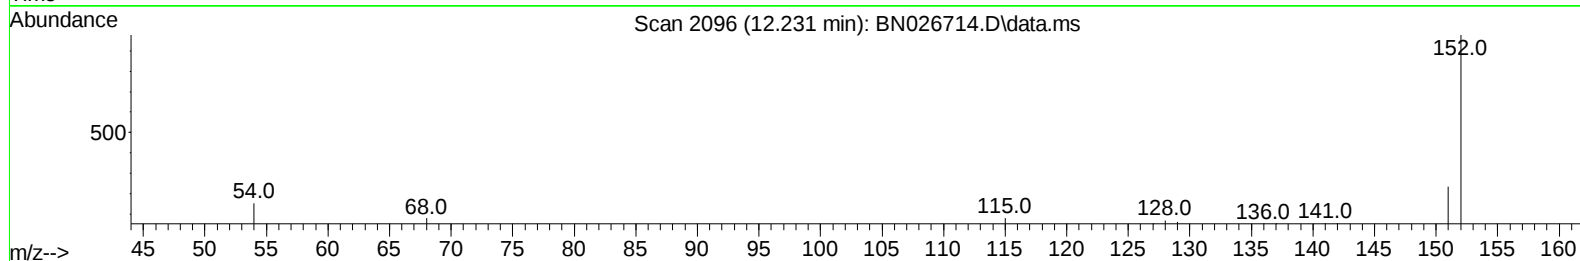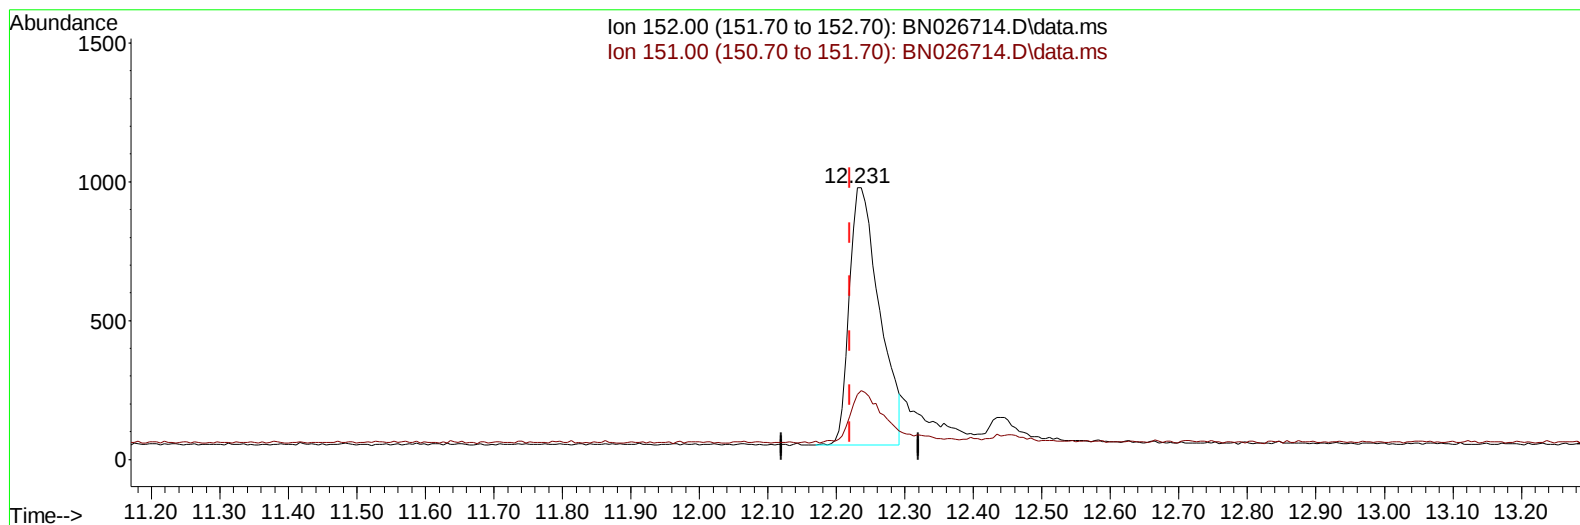

TIC: BN026714.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.231min (+ 0.011) 0.27 ng/u1

response 2815

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	21.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026714.D
 Acq On : 24 Jul 2023 15:16
 Operator : MA/JU
 Sample : PB154169BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK169

Manual IntegrationsAPPROVED

Quant Time: Jul 24 16:13:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

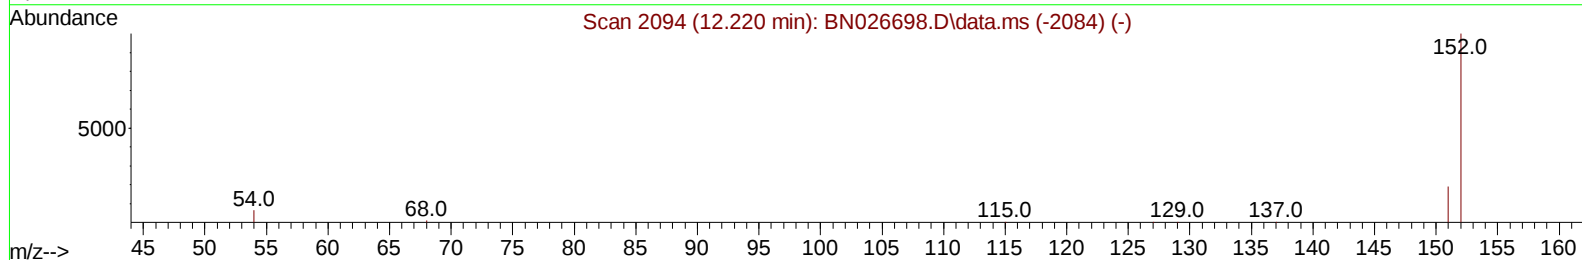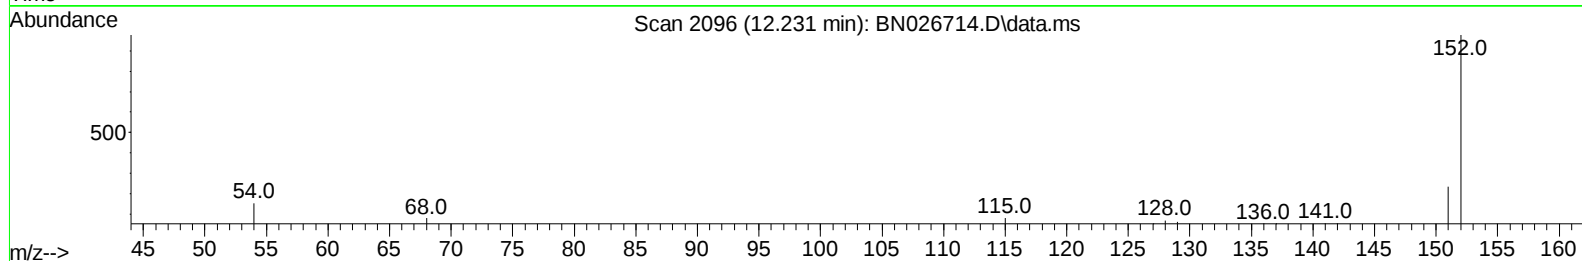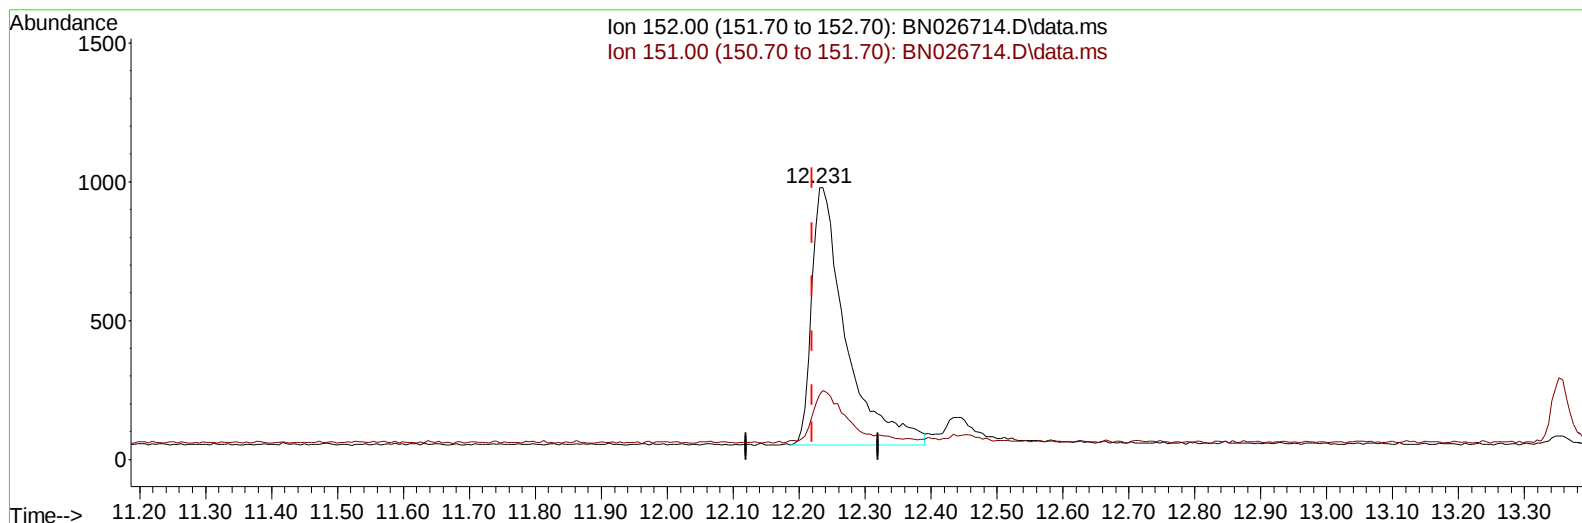

TIC: BN026714.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.231min (+ 0.011) 0.32 ng/ul m

response 3335

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	18.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026714.D
 Acq On : 24 Jul 2023 15:16
 Operator : MA/JU
 Sample : PB154169BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK169

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

Quant Time: Jul 24 16:13:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	2348	0.400	ng/ul	0.00
4) Naphthalene-d8	10.619	136	7609	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	5002	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	9981	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.425	240	6180	0.400	ng/ul	# 0.00
23) Perylene-d12	23.793	264	8214	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.195	96	12291	3.975	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.231	152	3335m	0.322	ng/ul	0.01
18) Fluoranthene-d10	19.250	212	6414	0.299	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026714.D
Acq On : 24 Jul 2023 15:16
Operator : MA/JU
Sample : PB154169BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK169

Manual IntegrationsAPPROVED

Quant Time: Jul 24 16:13:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

