

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026683.D
 Acq On : 23 Jul 2023 18:57
 Operator : MA/JU
 Sample : 03472-32DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46S7DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

Quant Time: Jul 24 00:42:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	4266	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	14019	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	8675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	18257	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.414	240	12423	0.400	ng/ul	# 0.00
23) Perylene-d12	23.784	264	14341	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	1101	0.196	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.225	152	798	0.042	ng/ul	0.00
18) Fluoranthene-d10	19.246	212	1761	0.041	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.674	128	3089	0.080	ng/ul#	95
7) 2-Methylnaphthalene	12.302	142	926	0.042	ng/ul	99
8) 1-Methylnaphthalene	12.517	142	845	0.036	ng/ul	94
10) Acenaphthylene	14.189	152	2885	0.068	ng/ul#	92
11) Acenaphthene	14.527	153	3262	0.101	ng/ul	100
12) Fluorene	15.517	166	4031	0.119	ng/ul	99
15) Phenanthrene	17.257	178	59604	1.025	ng/ul	98
16) Anthracene	17.350	178	11006	0.218	ng/ul	99
19) Fluoranthene	19.274	202	94669	1.626	ng/ul#	94
20) Pyrene	19.641	202	34784	0.550	ng/ul#	95
21) Benzo(a)anthracene	21.396	228	34453	0.755	ng/ul	99
22) Chrysene	21.449	228	34215	0.658	ng/ul	98
24) Benzo(b)fluoranthene	23.065	252	40517m	0.725	ng/ul	
25) Benzo(k)fluoranthene	23.106	252	17270m	0.295	ng/ul	
26) Benzo(a)pyrene	23.679	252	4531	0.091	ng/ul#	80
27) Indeno(1,2,3-cd)pyrene	26.241	276	7404	0.114	ng/ul#	83
28) Dibenzo(a,h)anthracene	26.241	278	5114	0.102	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026683.D
Acq On : 23 Jul 2023 18:57
Operator : MA/JU
Sample : 03472-32DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A46S7DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023


Quant Time: Jul 24 00:42:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

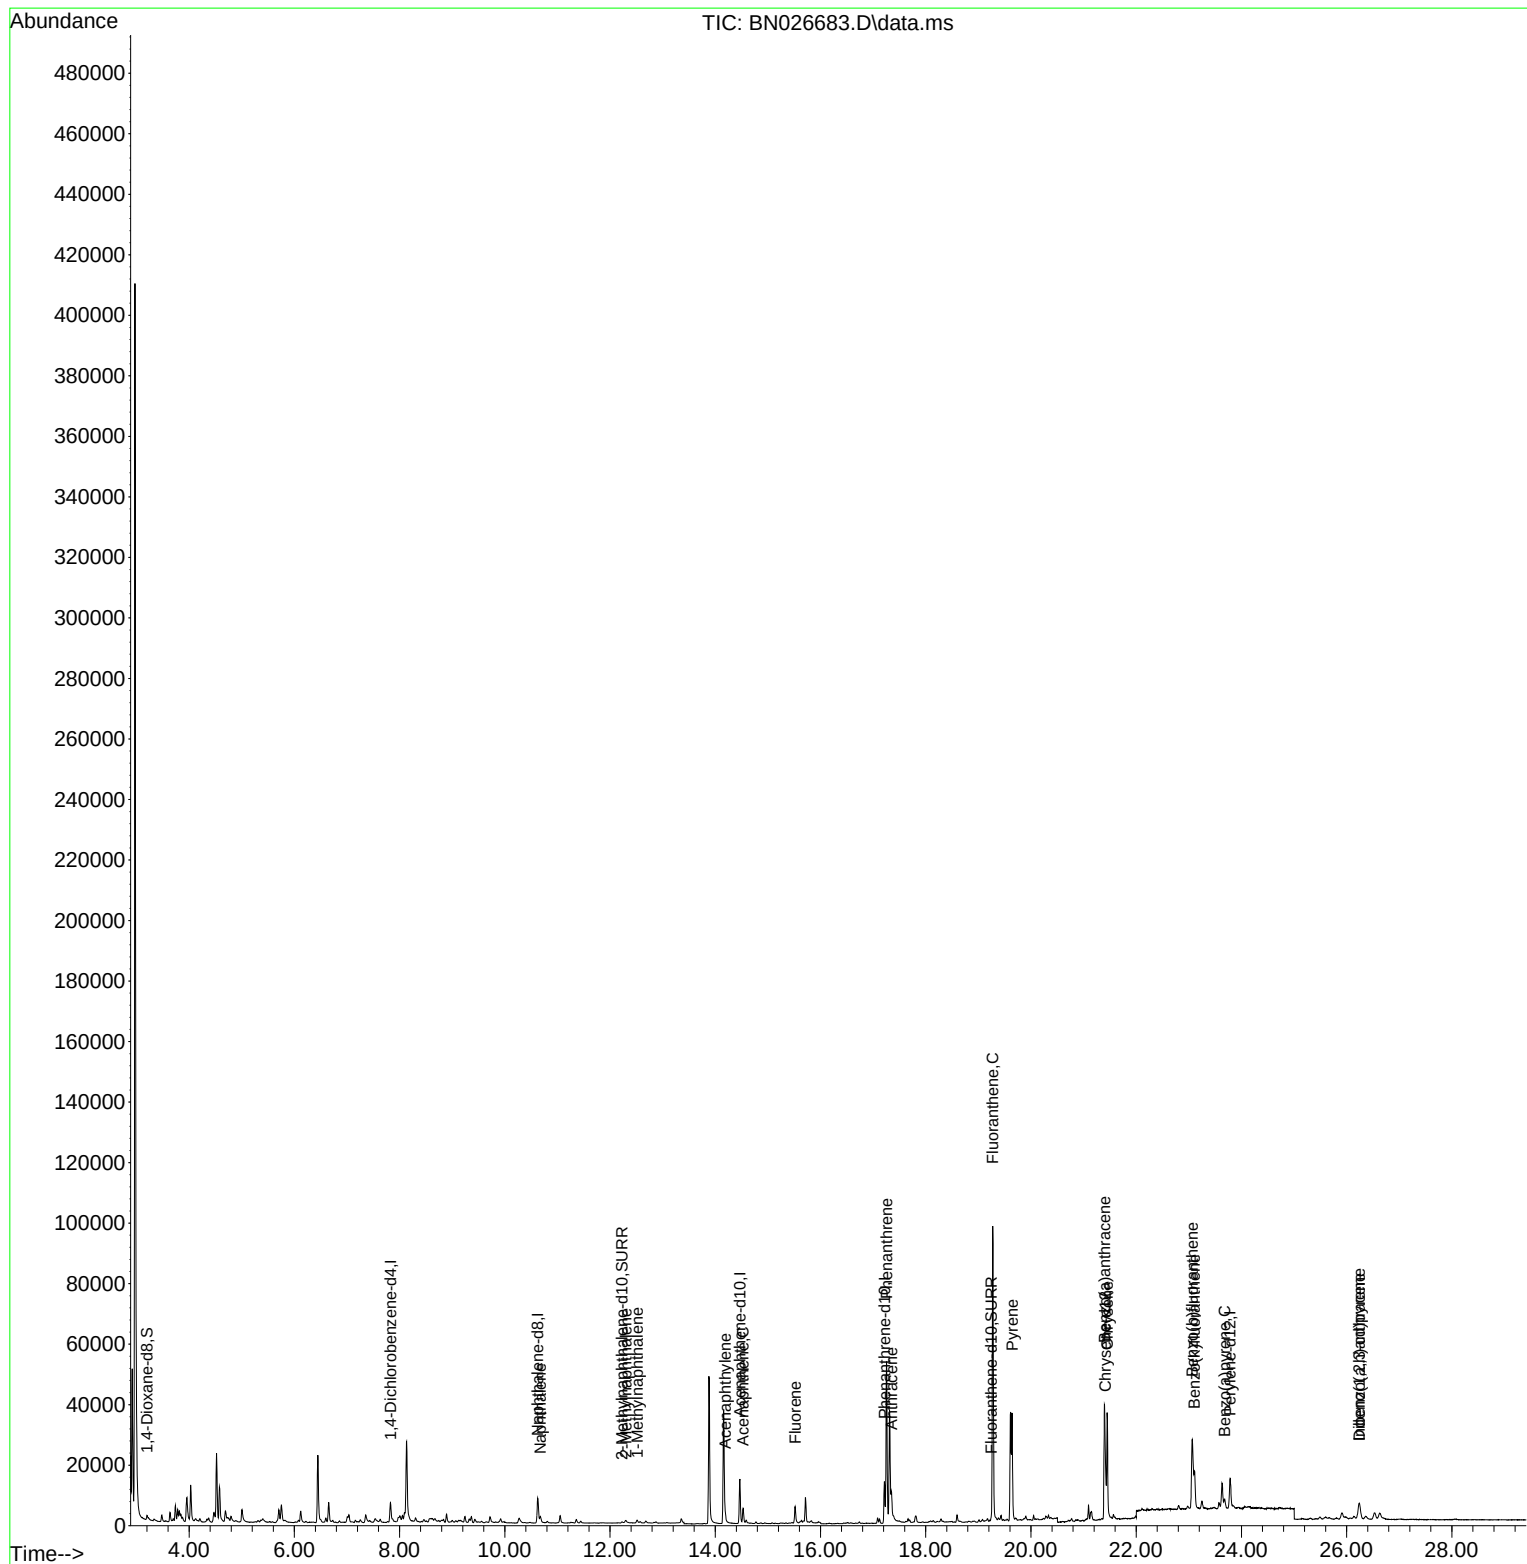

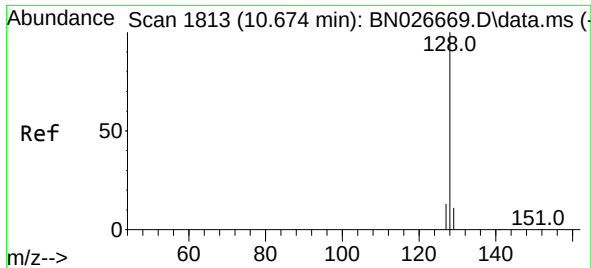

#5
Naphthalene
Concen: 0.080 ng/ul
RT: 10.674 min Scan# 1813
Delta R.T. 0.000 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

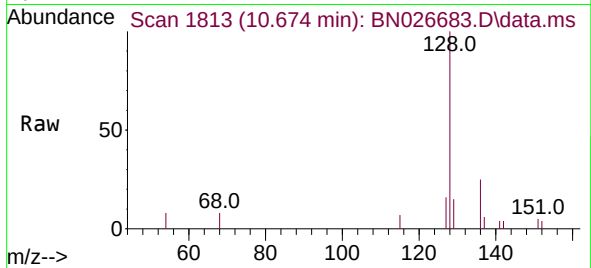

Tgt Ion:128 Resp: 3089
Ion Ratio Lower Upper
128 100
129 15.3 10.2 15.2
127 15.6 11.4 17.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

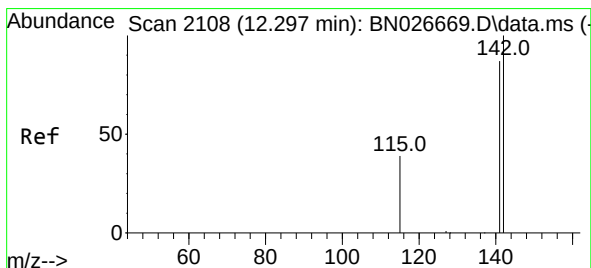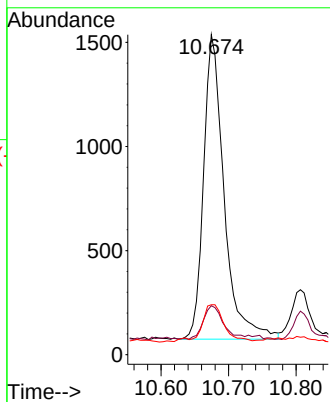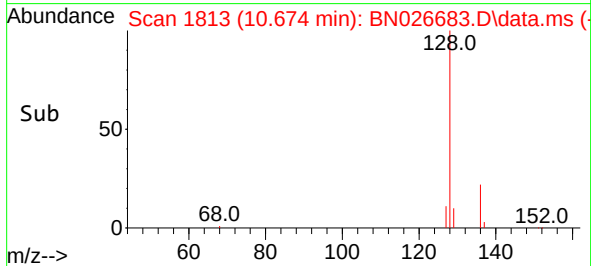

#7
2-Methylnaphthalene
Concen: 0.042 ng/ul
RT: 12.302 min Scan# 2109
Delta R.T. 0.005 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57


Tgt Ion:142 Resp: 926
Ion Ratio Lower Upper
142 100
141 89.8 72.3 108.5

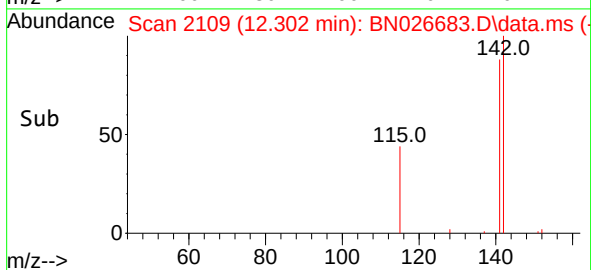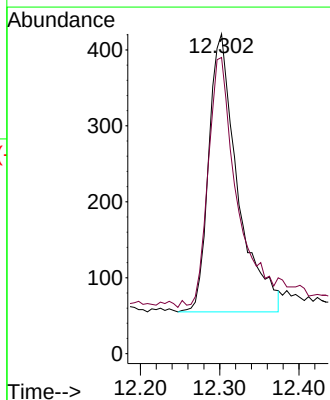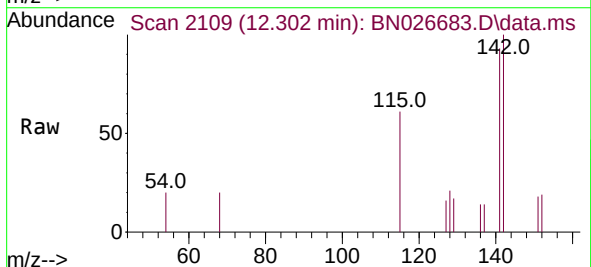

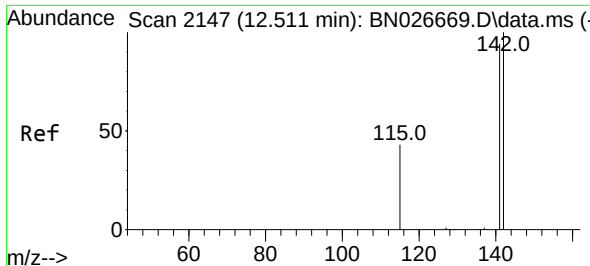

#8
1-Methylnaphthalene
Concen: 0.036 ng/ul
RT: 12.517 min Scan# 2148
Delta R.T. 0.006 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

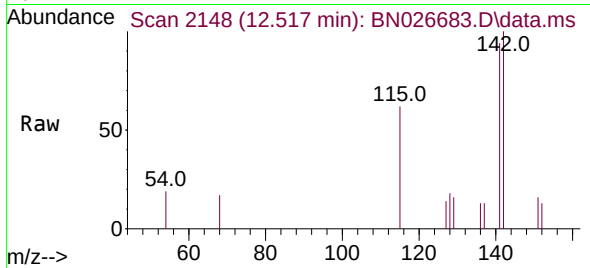

Tgt Ion:142 Resp: 849
Ion Ratio Lower Upper
142 100
141 99.3 74.5 111.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

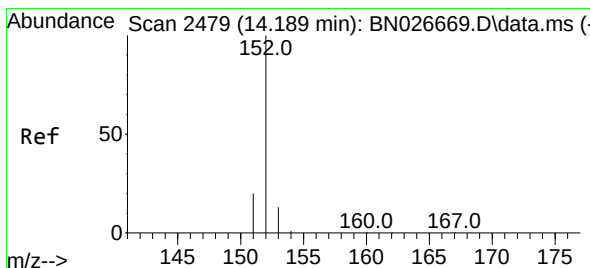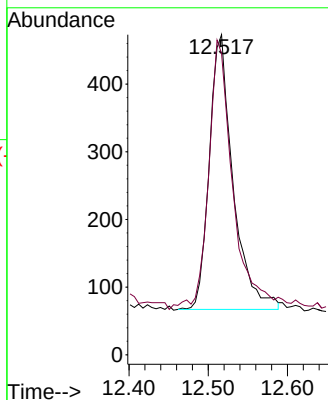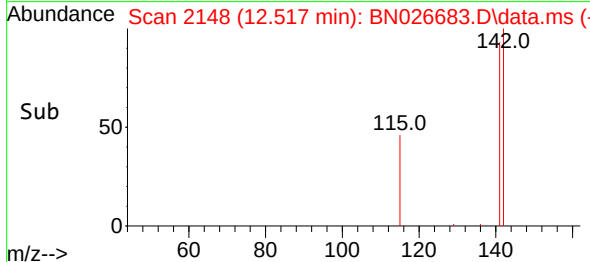

#10
Acenaphthylene
Concen: 0.068 ng/ul
RT: 14.189 min Scan# 2479
Delta R.T. 0.000 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57


Tgt Ion:152 Resp: 2885
Ion Ratio Lower Upper
152 100
151 24.5 17.0 25.6
153 18.7 11.4 17.2#

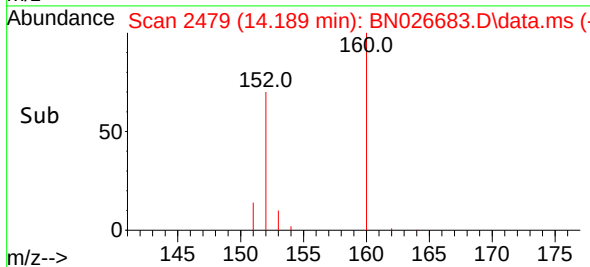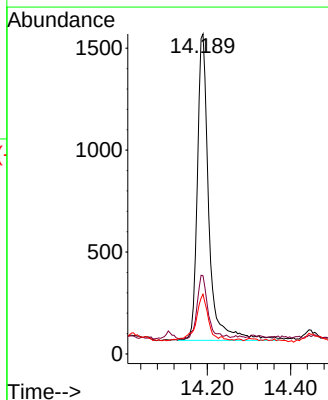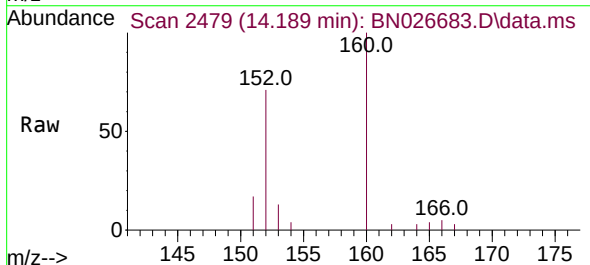

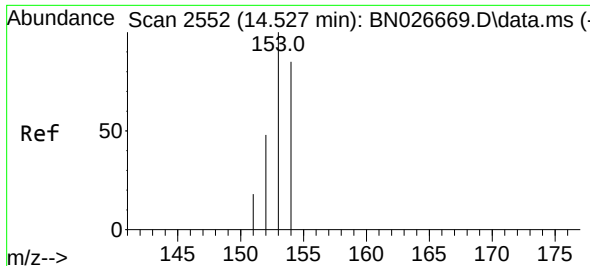

#11
Acenaphthene
Concen: 0.101 ng/u1
RT: 14.527 min Scan# 2552
Delta R.T. 0.000 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

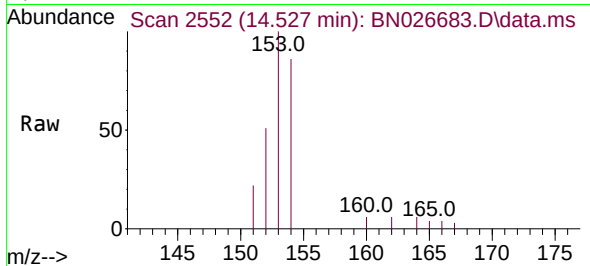

Tgt Ion:153 Resp: 326
Ion Ratio Lower Upper
153 100
152 50.5 40.2 60.4
154 86.3 69.3 103.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

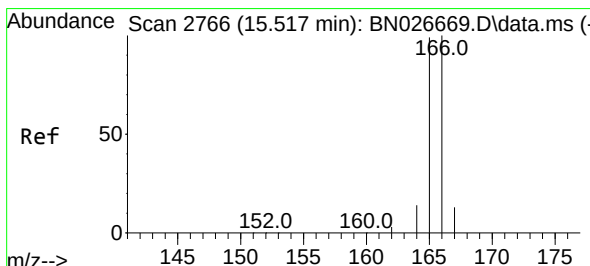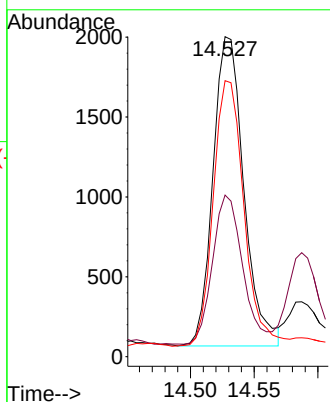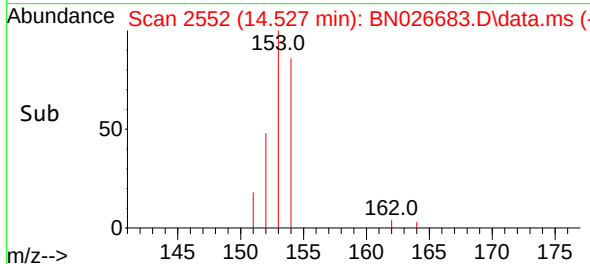

#12
Fluorene
Concen: 0.119 ng/u1
RT: 15.517 min Scan# 2766
Delta R.T. 0.000 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57

Tgt Ion:166 Resp: 4031
Ion Ratio Lower Upper
166 100
165 100.6 80.6 120.8
167 16.5 12.0 18.0

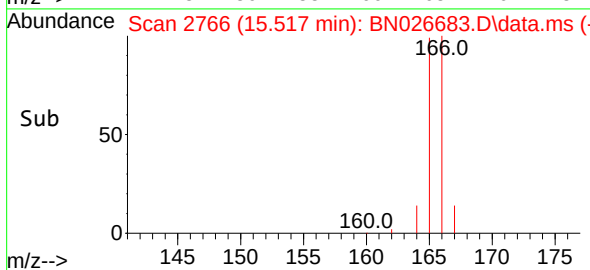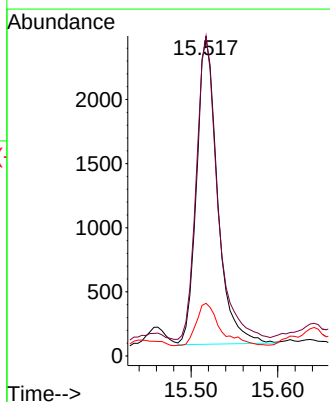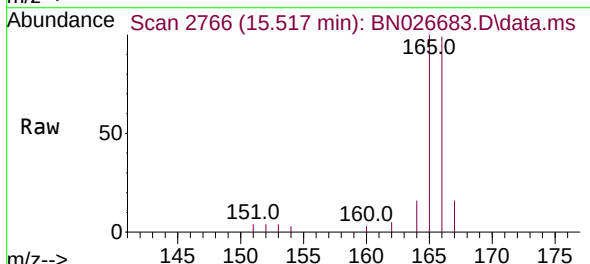

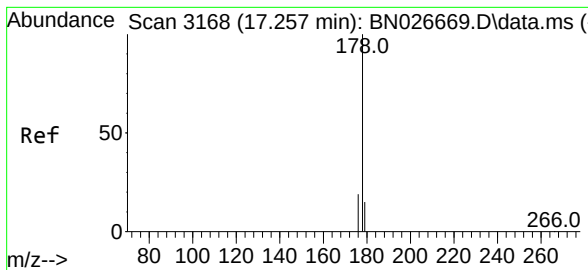

#15

Phenanthrene

Concen: 1.025 ng/u1

RT: 17.257 min Scan# 3168

Delta R.T. 0.000 min

Lab File: BN026683.D

Acq: 23 Jul 2023 18:57

Instrument :

BNA_N

ClientSampleId :

A46S7DL





Tgt Ion:	178	Resp:	59604
Ion Ratio	Lower	Upper	
178	100		
179	15.7	13.7	20.5
176	19.8	16.5	24.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/24/2023

Supervised By :mohammad ahmed 07/24/2023

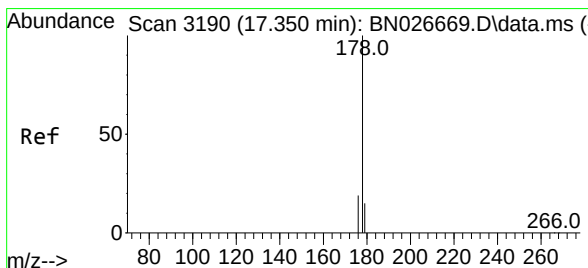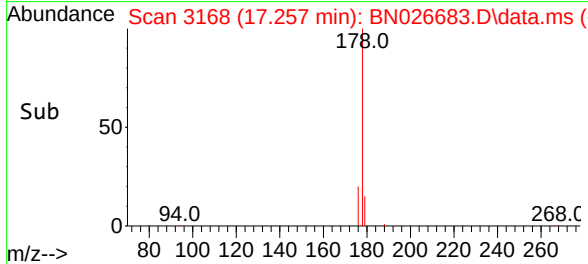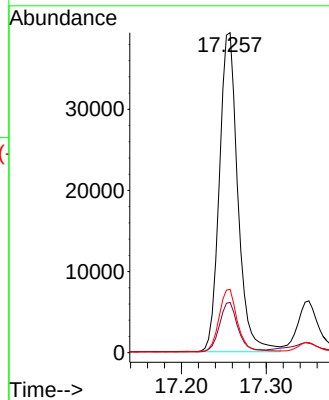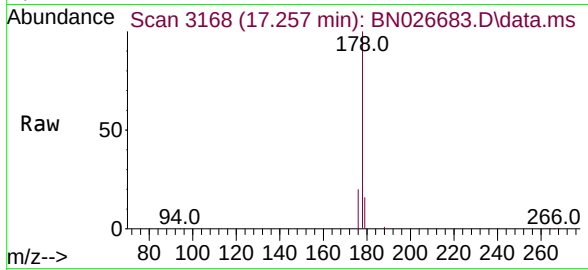

#16

Anthracene

Concen: 0.218 ng/u1




RT: 17.350 min Scan# 3190


Delta R.T. 0.000 min

Lab File: BN026683.D

Acq: 23 Jul 2023 18:57


Tgt Ion:	178	Resp:	11006
Ion Ratio	Lower	Upper	
178	100		
179	18.3	14.8	22.2
176	19.9	16.6	25.0

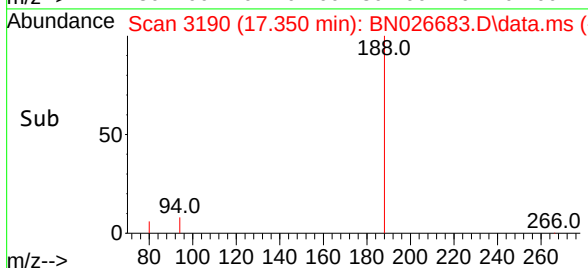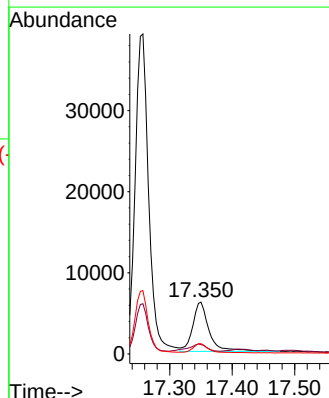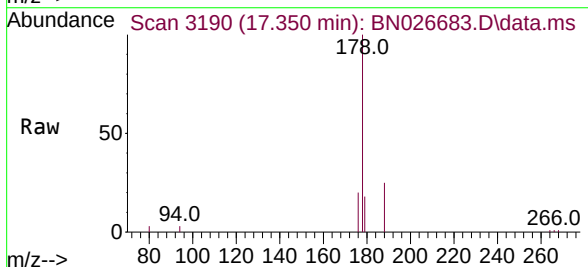

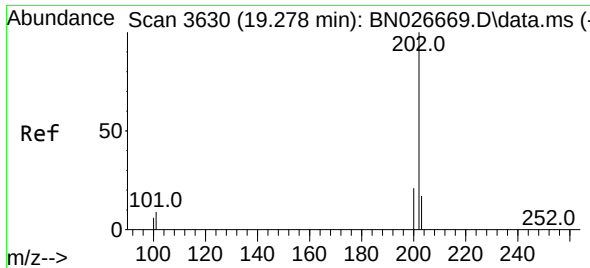

#19
Fluoranthene
Concen: 1.626 ng/u1
RT: 19.274 min Scan# 3629
Delta R.T. -0.005 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

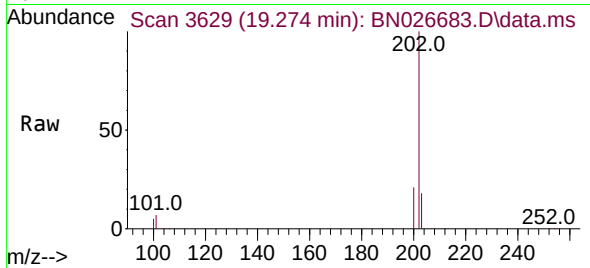

Tgt Ion:202 Resp: 94669
Ion Ratio Lower Upper
202 100
101 6.8 7.0 10.4
100 5.3 6.0 9.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

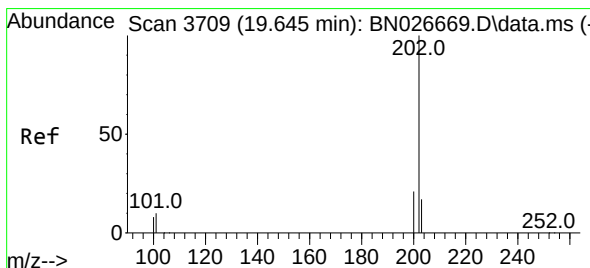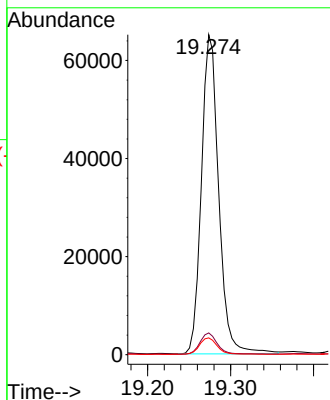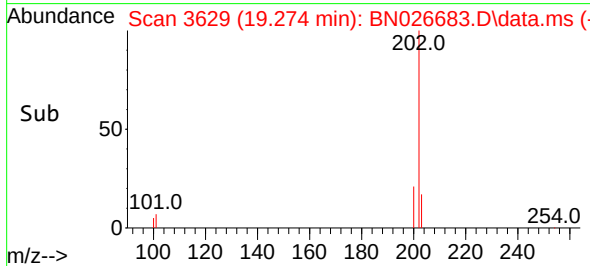

#20
Pyrene
Concen: 0.550 ng/u1
RT: 19.641 min Scan# 3708
Delta R.T. -0.005 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57


Tgt Ion:202 Resp: 34784
Ion Ratio Lower Upper
202 100
101 7.7 8.0 12.0
100 6.5 6.2 9.2

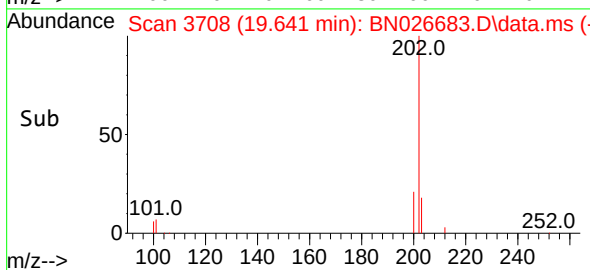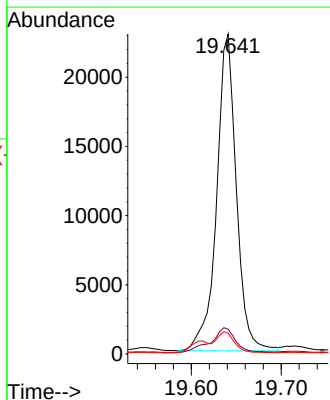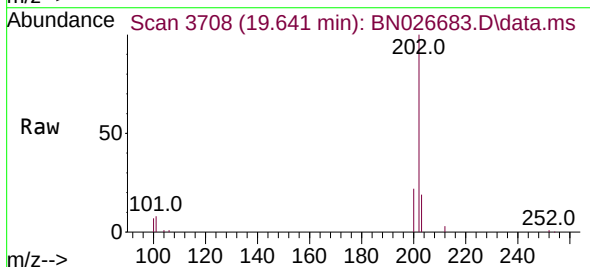

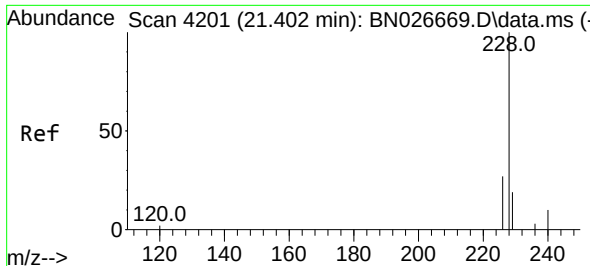

#21
Benzo(a)anthracene
Concen: 0.755 ng/u1
RT: 21.396 min Scan# 4119
Delta R.T. -0.006 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

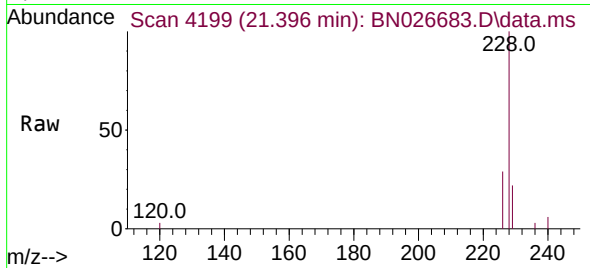

Tgt Ion:228 Resp: 3445
Ion Ratio Lower Upper
228 100
229 21.5 16.7 25.1
226 28.9 23.5 35.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

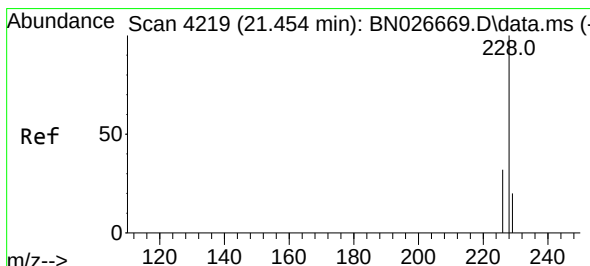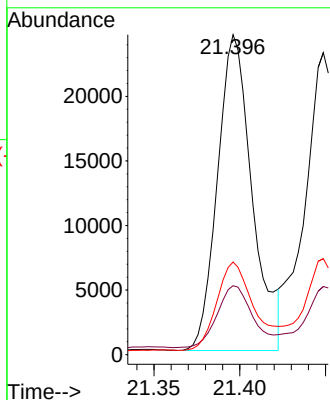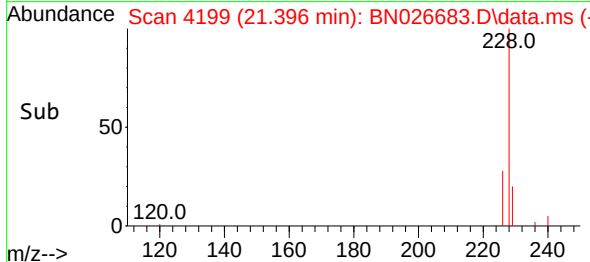

#22
Chrysene
Concen: 0.658 ng/u1
RT: 21.449 min Scan# 4217
Delta R.T. -0.006 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57


Tgt Ion:228 Resp: 34215
Ion Ratio Lower Upper
228 100
226 31.8 25.2 37.8
229 22.6 16.4 24.6

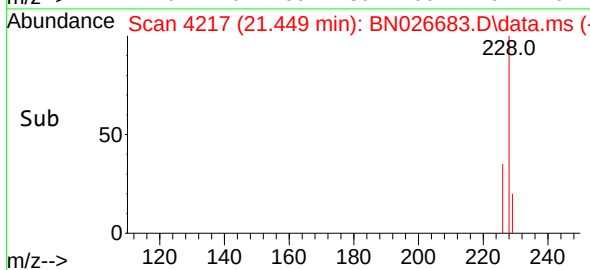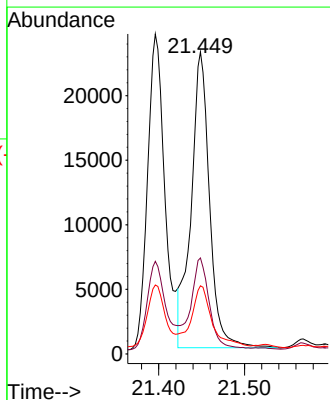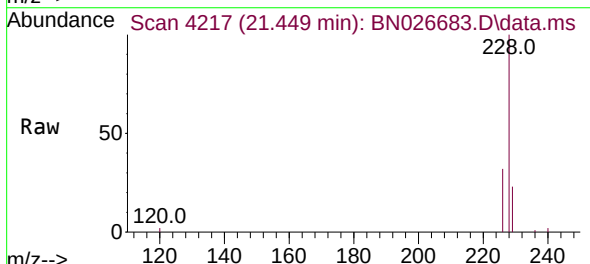

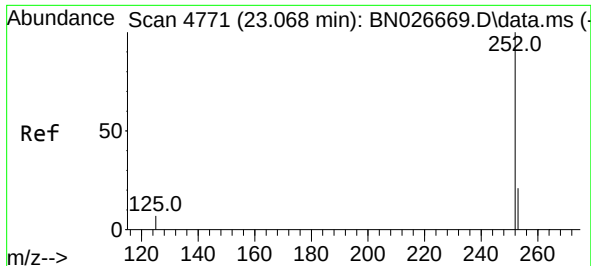

#24
Benzo(b)fluoranthene
Concen: 0.725 ng/ul m
RT: 23.065 min Scan# 4770
Delta R.T. -0.003 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

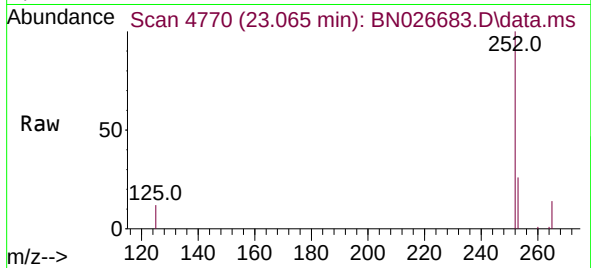

Tgt Ion:252 Resp: 4051
Ion Ratio Lower Upper
252 100
253 26.5 0.0 68.6
125 12.3 0.0 34.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

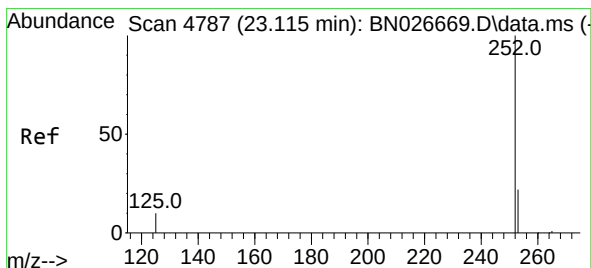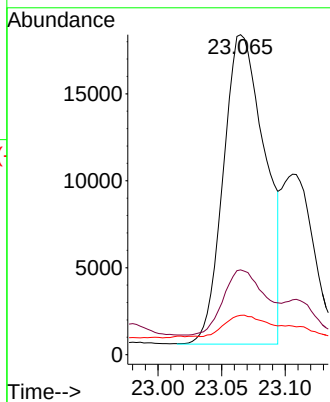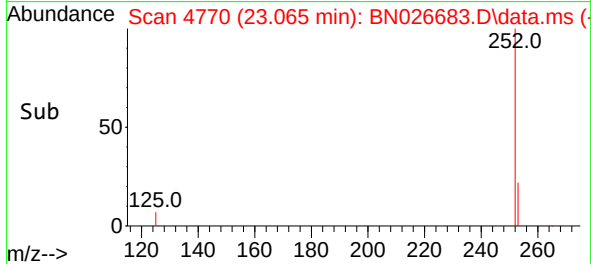

#25
Benzo(k)fluoranthene
Concen: 0.295 ng/ul m
RT: 23.106 min Scan# 4784
Delta R.T. -0.009 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57


Tgt Ion:252 Resp: 17270
Ion Ratio Lower Upper
252 100
253 30.4 27.2 40.8
125 15.9 13.4 20.2

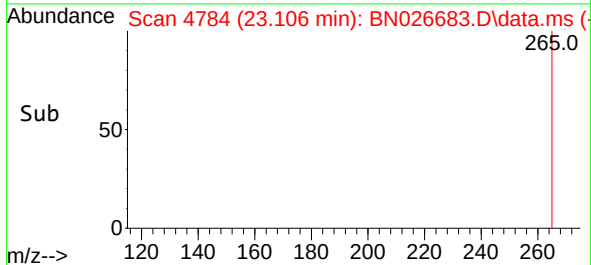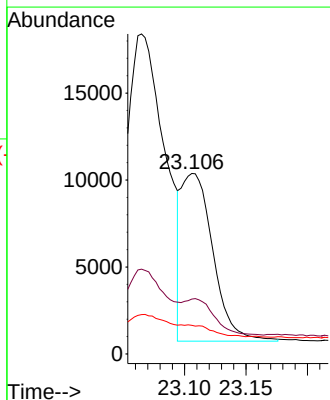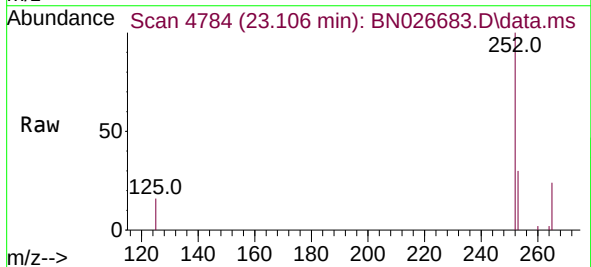

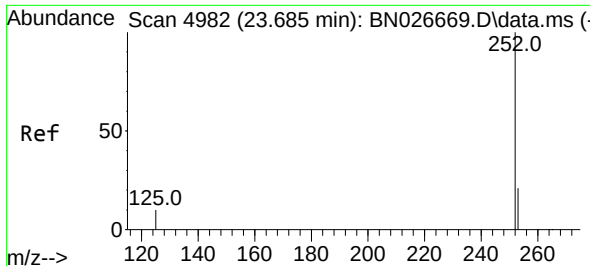

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.679 min Scan# 4982
Delta R.T. -0.006 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57




Instrument :
BNA_N
ClientSampleId :
A46S7DL

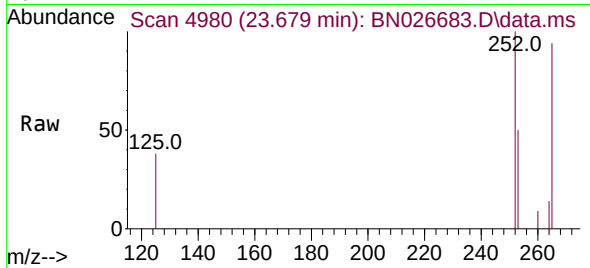


Tgt Ion:252 Resp: 453
Ion Ratio Lower Upper
252 100
253 50.4 32.6 49.0
125 37.9 19.3 28.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

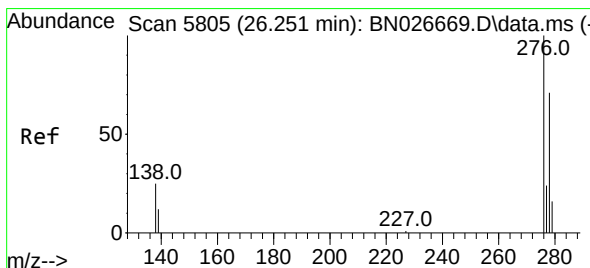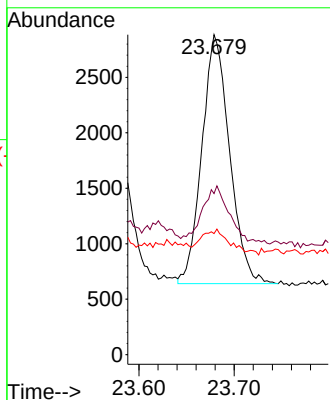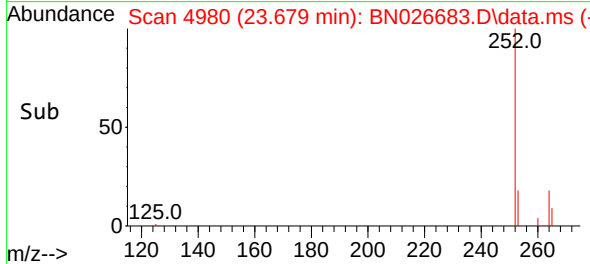


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.114 ng/ul
RT: 26.241 min Scan# 5802
Delta R.T. -0.010 min
Lab File: BN026683.D
Acq: 23 Jul 2023 18:57

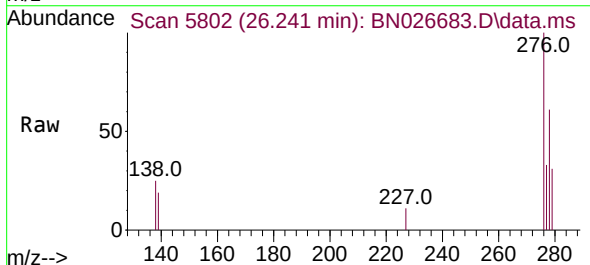


Tgt Ion:276 Resp: 7404
Ion Ratio Lower Upper
276 100
138 18.8 22.2 33.4
227 0.1 0.1 0.1

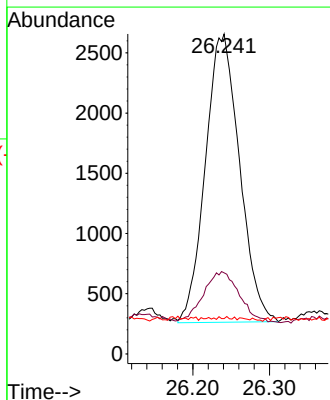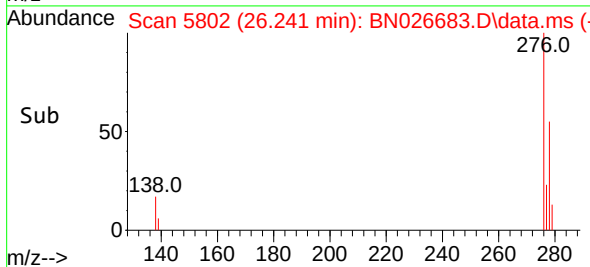

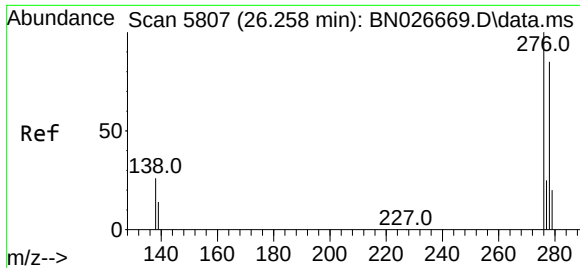

#28
 Dibenzo(a,h)anthracene
 Concen: 0.102 ng/ul
 RT: 26.241 min Scan# 5114
 Delta R.T. -0.017 min
 Lab File: BN026683.D
 Acq: 23 Jul 2023 18:57

Instrument :
 BNA_N
 ClientSampleId :
 A46S7DL

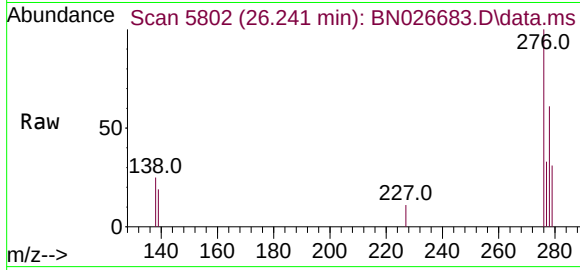

Tgt Ion:278 Resp: 5114
 Ion Ratio Lower Upper
 278 100
 139 32.0 18.9 28.3
 279 51.2 31.3 46.9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

