

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
 Data File : BN026686.D
 Acq On : 23 Jul 2023 21:23
 Operator : MA/JU
 Sample : 03472-33DL 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46TODL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

Quant Time: Jul 24 00:43:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.827	152	3176	0.400	ng/ul	0.00
4) Naphthalene-d8	10.625	136	11097	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.467	164	6505	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.215	188	14416	0.400	ng/ul	0.00
17) Chrysene-d12	21.411	240	9673	0.400	ng/ul	# 0.00
23) Perylene-d12	23.784	264	10396	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	686	0.164	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.236	152	566	0.038	ng/ul	0.02
18) Fluoranthene-d10	19.246	212	1543	0.046	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.674	128	1991	0.065	ng/ul#	89
7) 2-Methylnaphthalene	12.302	142	471	0.027	ng/ul	96
8) 1-Methylnaphthalene	12.517	142	456	0.025	ng/ul	94
10) Acenaphthylene	14.189	152	2186	0.069	ng/ul#	91
11) Acenaphthene	14.527	153	3200	0.132	ng/ul	99
12) Fluorene	15.517	166	3512	0.138	ng/ul	97
15) Phenanthrene	17.253	178	48190	1.050	ng/ul	98
16) Anthracene	17.350	178	9178	0.230	ng/ul	98
19) Fluoranthene	19.274	202	79293	1.749	ng/ul	97
20) Pyrene	19.641	202	46987	0.954	ng/ul	97
21) Benzo(a)anthracene	21.396	228	26837	0.755	ng/ul	99
22) Chrysene	21.446	228	24489	0.605	ng/ul	97
24) Benzo(b)fluoranthene	23.065	252	29734m	0.734	ng/ul	
25) Benzo(k)fluoranthene	23.109	252	11694m	0.275	ng/ul	
26) Benzo(a)pyrene	23.679	252	6066	0.168	ng/ul	96
27) Indeno(1,2,3-cd)pyrene	26.230	276	9018	0.191	ng/ul#	80
28) Dibenzo(a,h)anthracene	26.240	278	3428	0.095	ng/ul#	71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072323\
Data File : BN026686.D
Acq On : 23 Jul 2023 21:23
Operator : MA/JU
Sample : 03472-33DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A46T0DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023


Quant Time: Jul 24 00:43:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

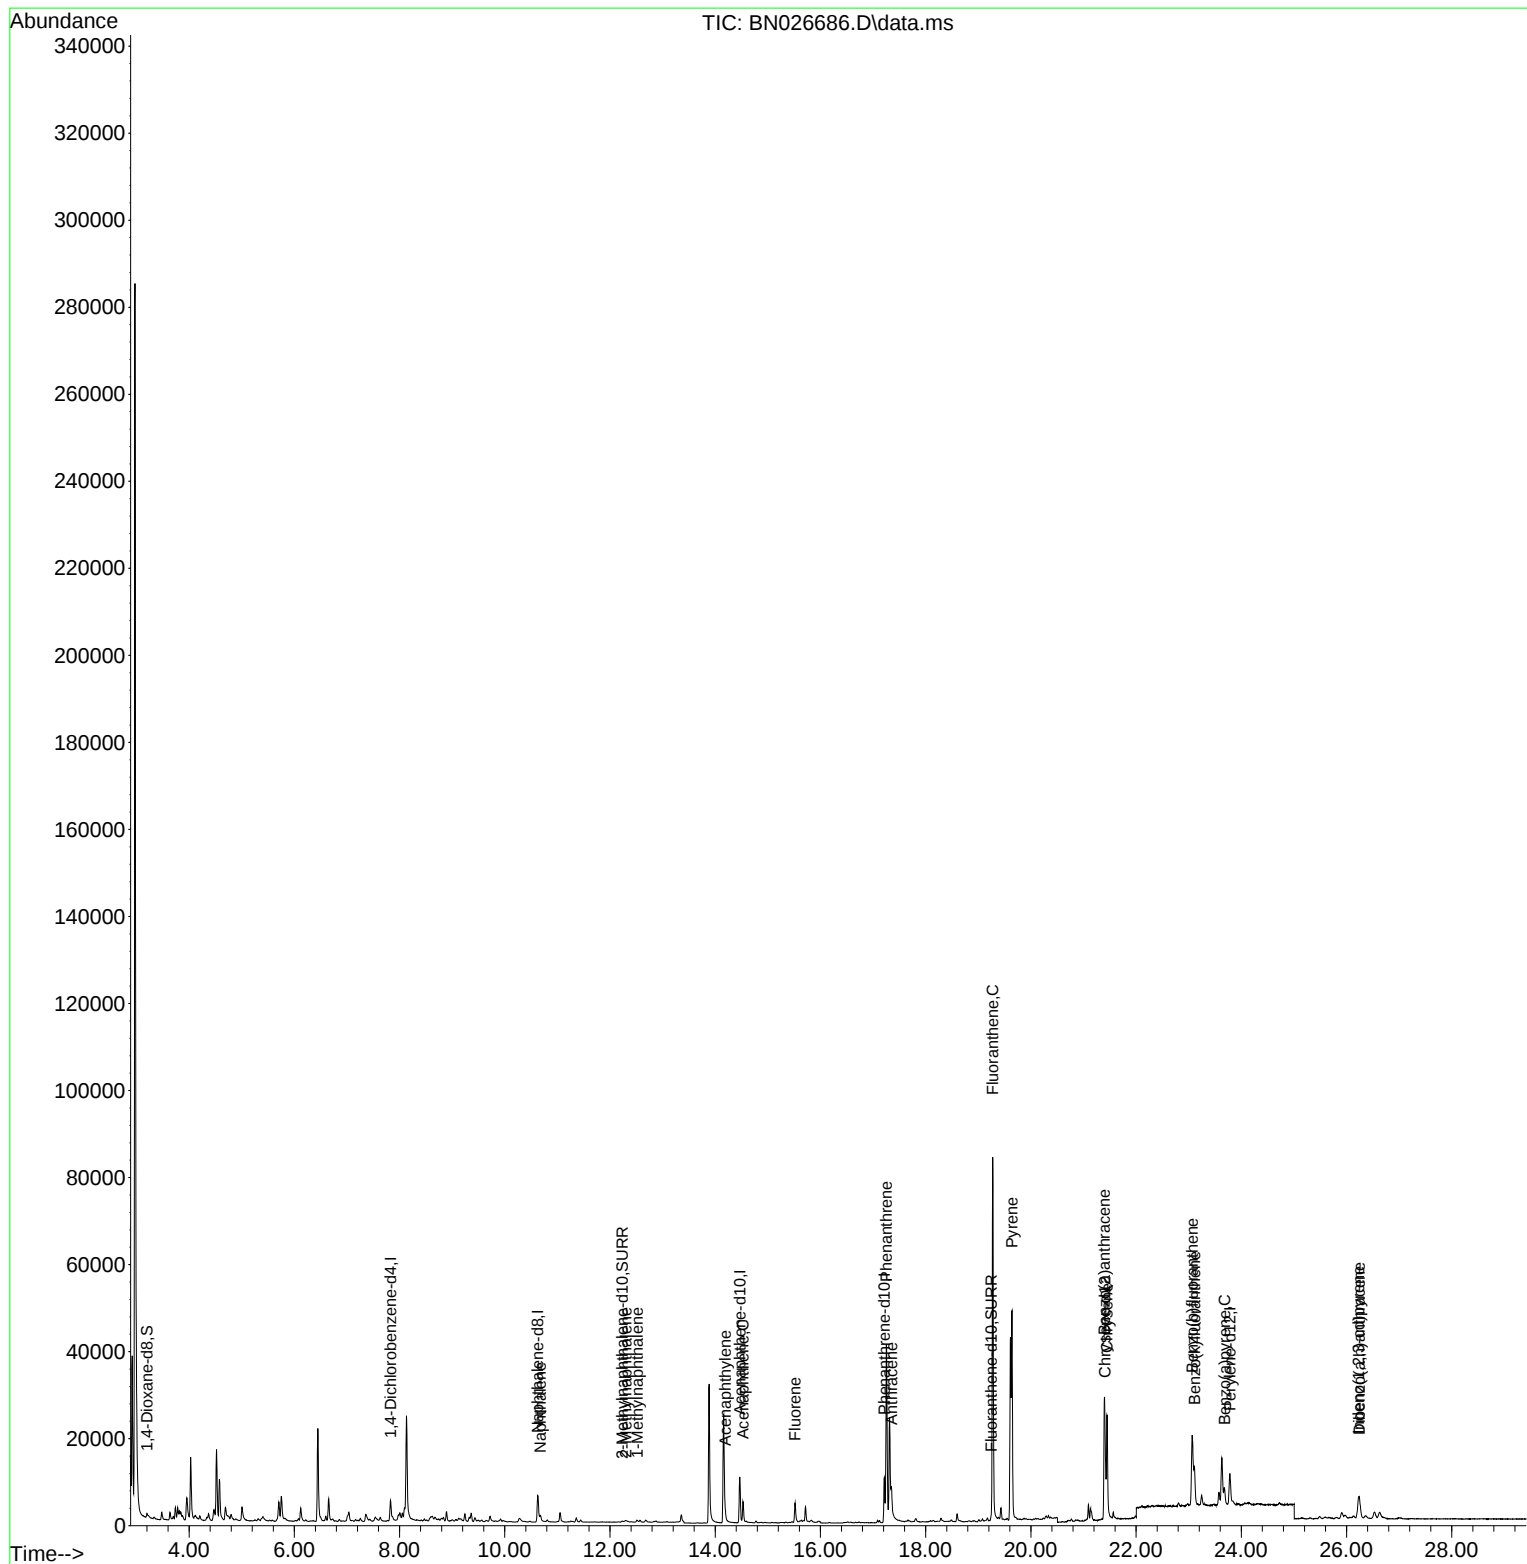

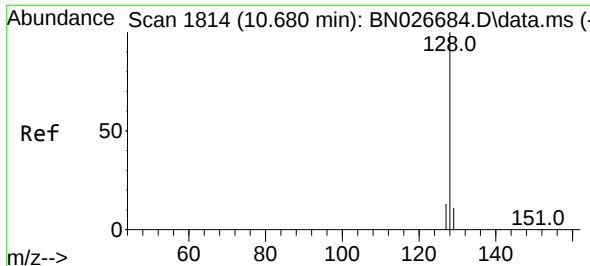

#5
Naphthalene
Concen: 0.065 ng/ul
RT: 10.674 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL



Tgt Ion:128 Resp: 199
Ion Ratio Lower Upper
128 100
129 17.5 10.2 15.2
127 18.4 11.4 17.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

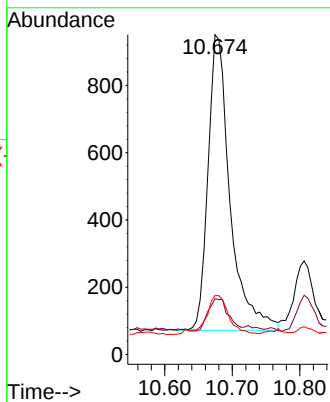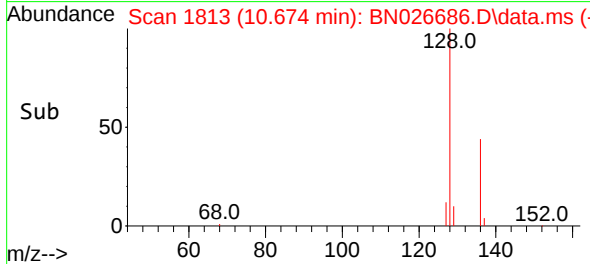

#7
2-Methylnaphthalene
Concen: 0.027 ng/ul
RT: 12.302 min Scan# 2109
Delta R.T. 0.005 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23

Tgt Ion:142 Resp: 471
Ion Ratio Lower Upper
142 100
141 94.1 72.3 108.5

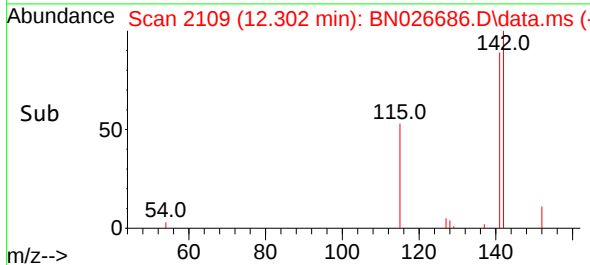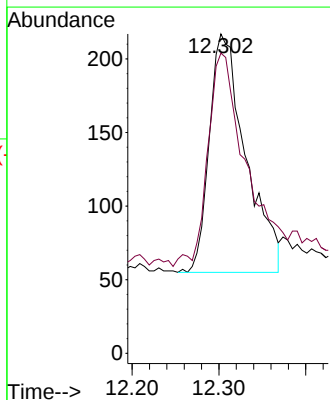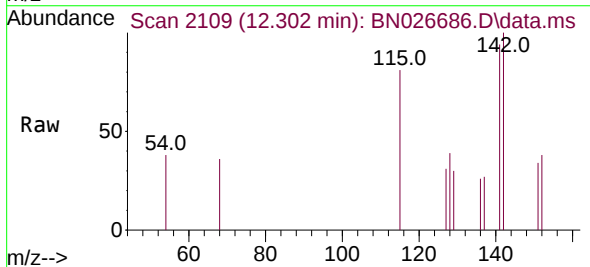

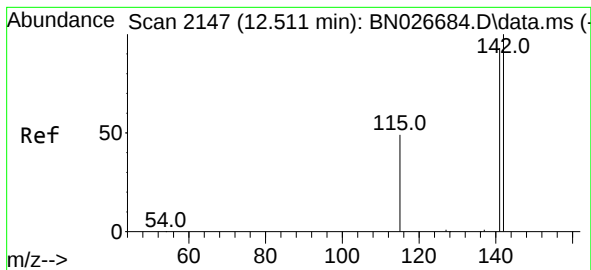

#8

1-Methylnaphthalene

Concen: 0.025 ng/ul

RT: 12.517 min Scan# 2148

Delta R.T. 0.005 min

Lab File: BN026686.D

Acq: 23 Jul 2023 21:23

Instrument :

BNA_N

ClientSampleId :

A46TODL

Tgt Ion:142 Resp: 450

Ion Ratio Lower Upper

142 100





141 87.5 74.5 111.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/24/2023

Supervised By :mohammad ahmed 07/24/2023

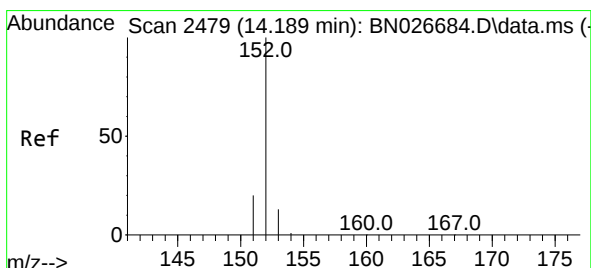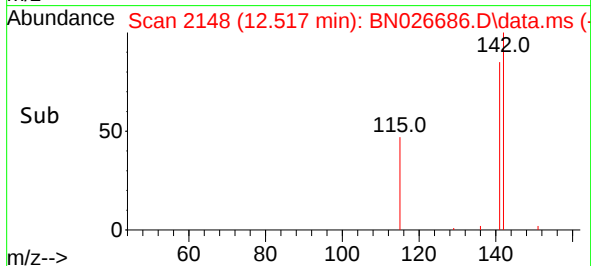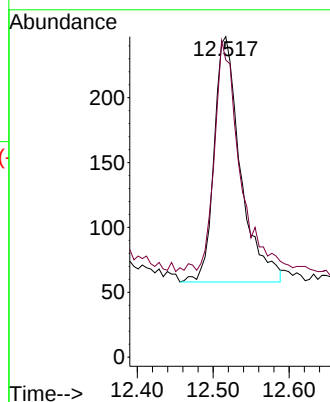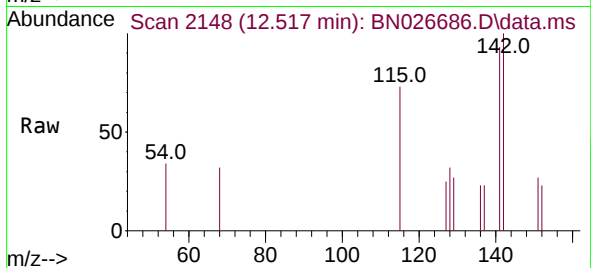

#10

Acenaphthylene

Concen: 0.069 ng/ul

RT: 14.189 min Scan# 2479

Delta R.T. -0.000 min

Lab File: BN026686.D

Acq: 23 Jul 2023 21:23




Tgt Ion:152 Resp: 2186


Ion Ratio Lower Upper

152 100

151 24.7 17.0 25.6


153 18.6 11.4 17.2#

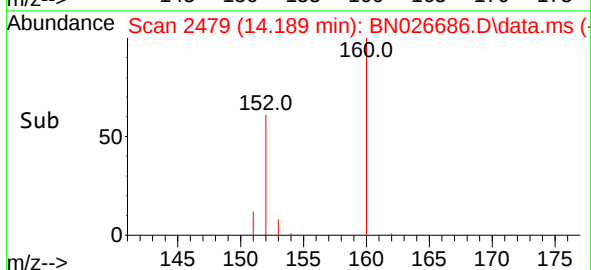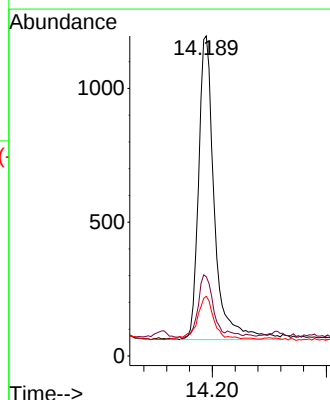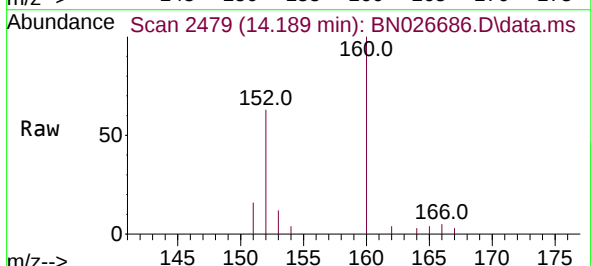

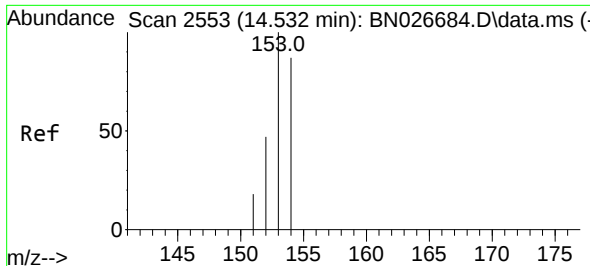

#11
Acenaphthene
Concen: 0.132 ng/u1
RT: 14.527 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL



Tgt Ion:153 Resp: 3200
Ion Ratio Lower Upper
153 100
152 49.2 40.2 60.4
154 85.5 69.3 103.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

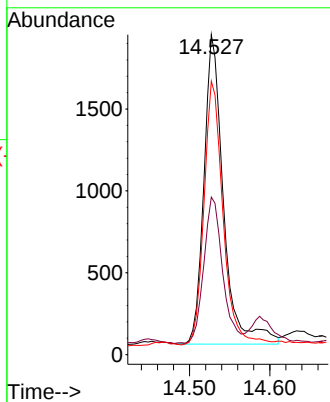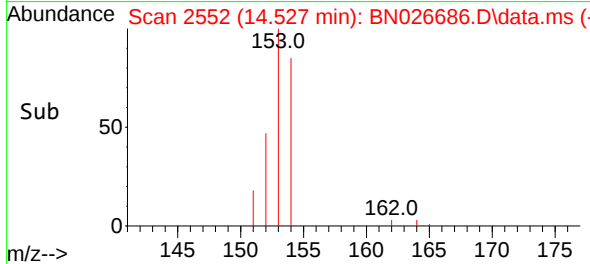

#12
Fluorene
Concen: 0.138 ng/u1
RT: 15.517 min Scan# 2766
Delta R.T. -0.000 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23


Tgt Ion:166 Resp: 3512
Ion Ratio Lower Upper
166 100
165 98.2 80.6 120.8
167 16.7 12.0 18.0

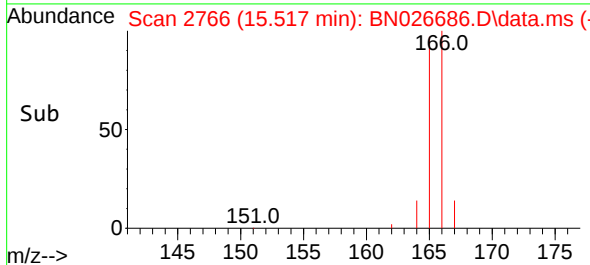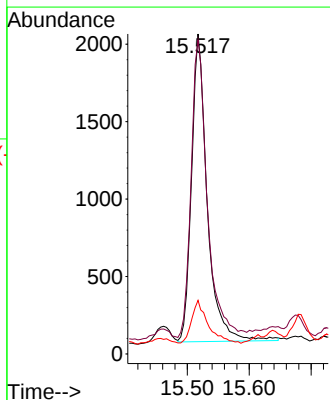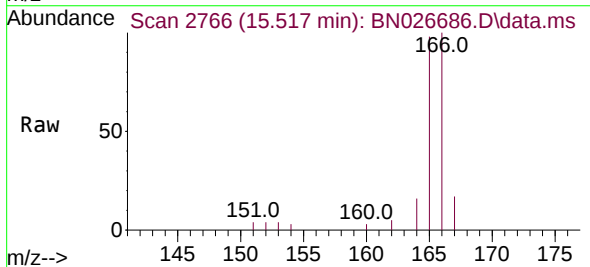

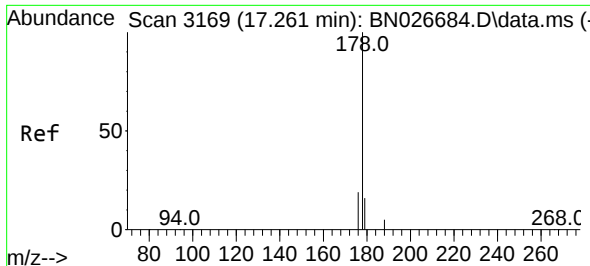

#15
Phenanthrene
Concen: 1.050 ng/ul
RT: 17.253 min Scan# 3169
Delta R.T. -0.004 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL



Tgt Ion:178 Resp: 48190
Ion Ratio Lower Upper
178 100
179 15.6 13.7 20.5
176 19.8 16.5 24.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

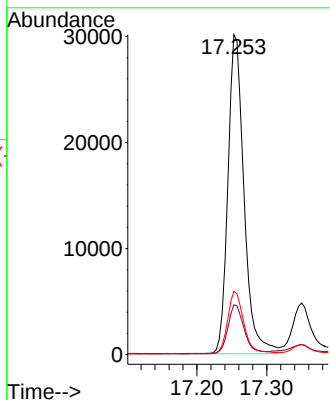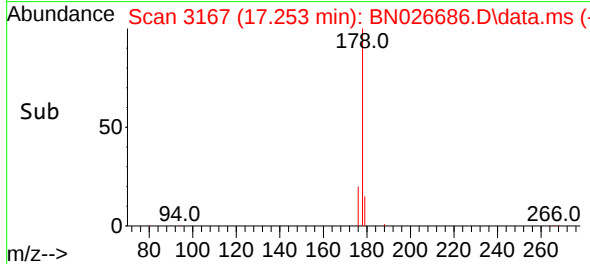

#16
Anthracene
Concen: 0.230 ng/ul
RT: 17.350 min Scan# 3190
Delta R.T. -0.000 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23


Tgt Ion:178 Resp: 9178
Ion Ratio Lower Upper
178 100
179 19.6 14.8 22.2
176 19.7 16.6 25.0

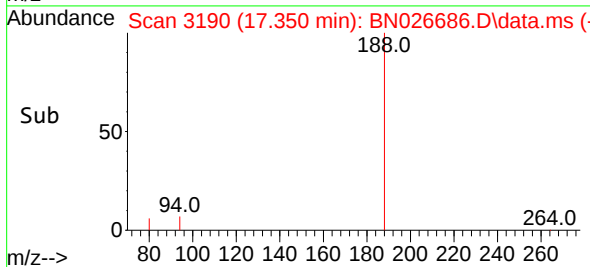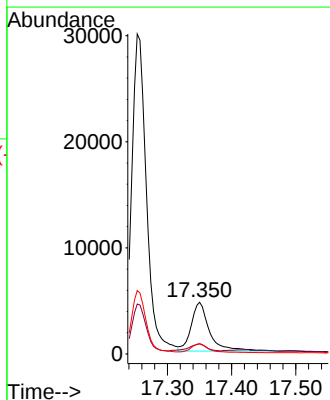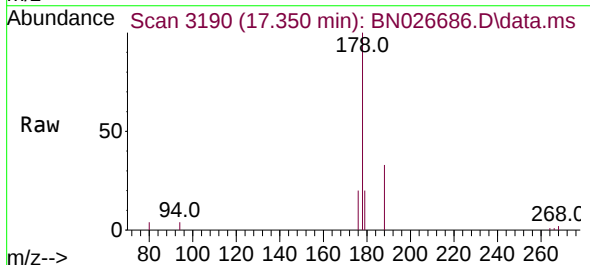

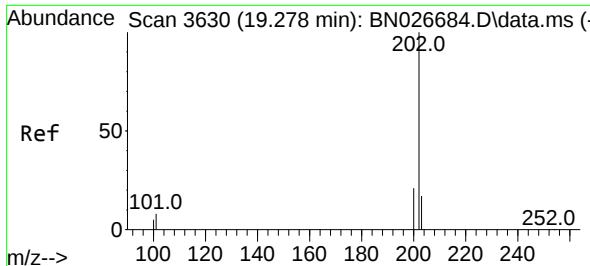

#19
Fluoranthene
Concen: 1.749 ng/ul
RT: 19.274 min Scan# 30
Delta R.T. -0.005 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL

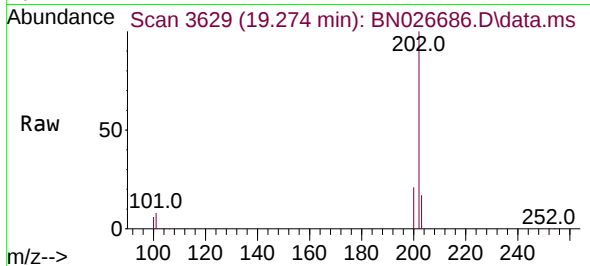

Tgt Ion:202 Resp: 7929
Ion Ratio Lower Upper
202 100
101 7.8 7.0 10.4
100 6.0 6.0 9.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

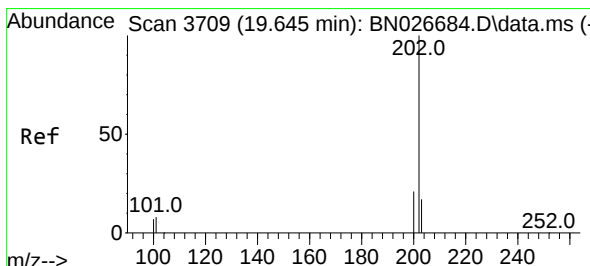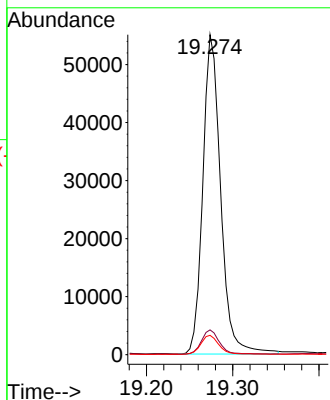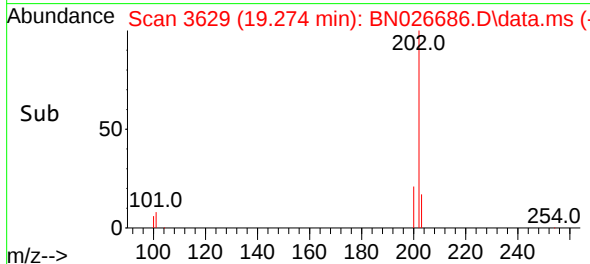

#20
Pyrene
Concen: 0.954 ng/ul
RT: 19.641 min Scan# 3708
Delta R.T. -0.005 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23


Tgt Ion:202 Resp: 46987
Ion Ratio Lower Upper
202 100
101 8.5 8.0 12.0
100 7.1 6.2 9.2

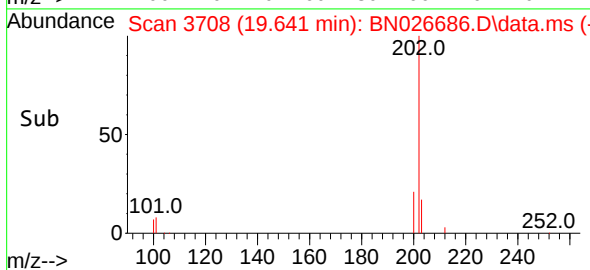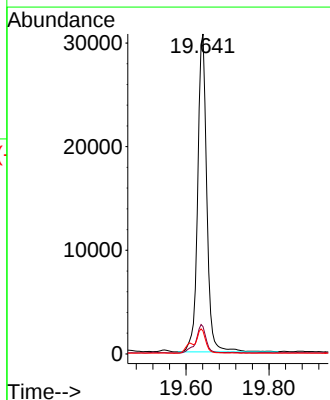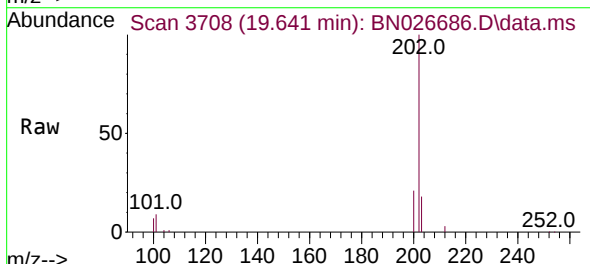



#21
Benzo(a)anthracene
Concen: 0.755 ng/u1
RT: 21.396 min Scan# 4199
Delta R.T. -0.006 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL




Tgt Ion:228 Resp: 2683
Ion Ratio Lower Upper
228 100
229 21.5 16.7 25.1
226 28.8 23.5 35.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

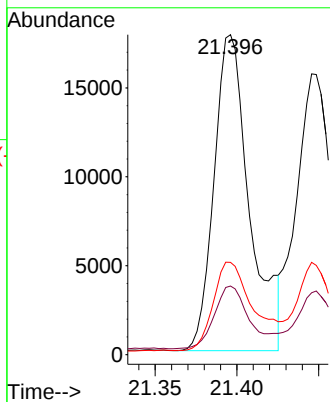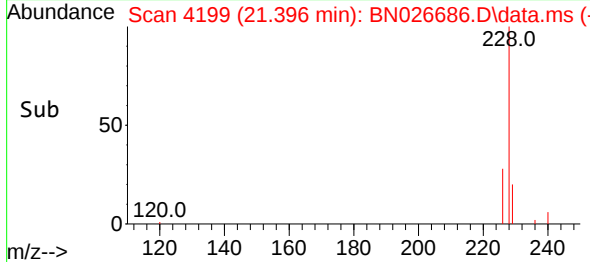


#22
Chrysene
Concen: 0.605 ng/u1
RT: 21.446 min Scan# 4216
Delta R.T. -0.009 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23

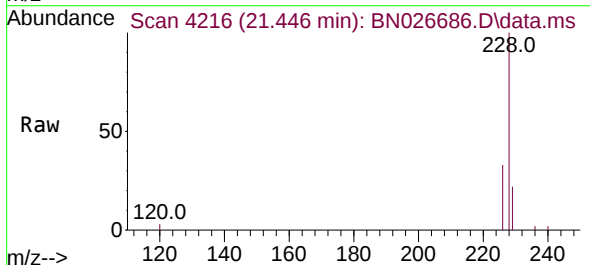


Tgt Ion:228 Resp: 24489
Ion Ratio Lower Upper
228 100
226 32.9 25.2 37.8
229 22.1 16.4 24.6

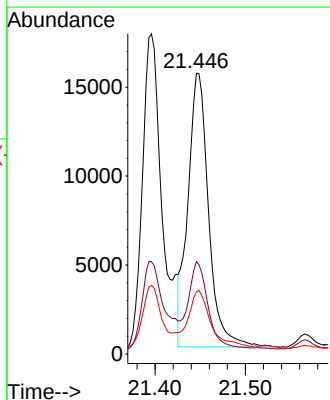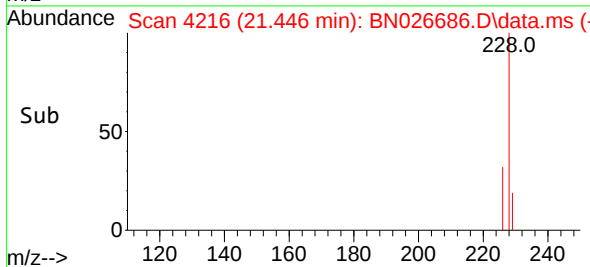



#24
Benzo(b)fluoranthene
Concen: 0.734 ng/ul m
RT: 23.065 min Scan# 4770
Delta R.T. -0.003 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23




Instrument :
BNA_N
ClientSampleId :
A46TODL




Tgt Ion:252 Resp: 29734
Ion Ratio Lower Upper
252 100
253 27.0 0.0 68.6
125 12.1 0.0 34.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

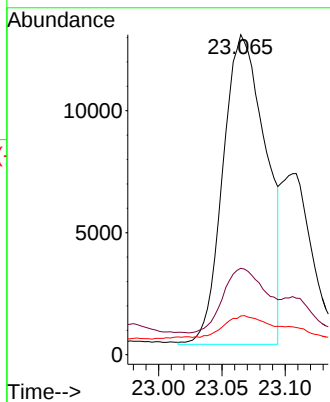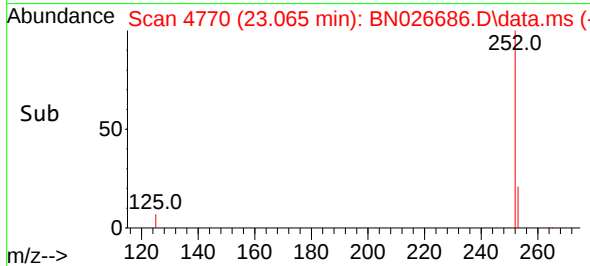


#25
Benzo(k)fluoranthene
Concen: 0.275 ng/ul m
RT: 23.109 min Scan# 4785
Delta R.T. -0.006 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23

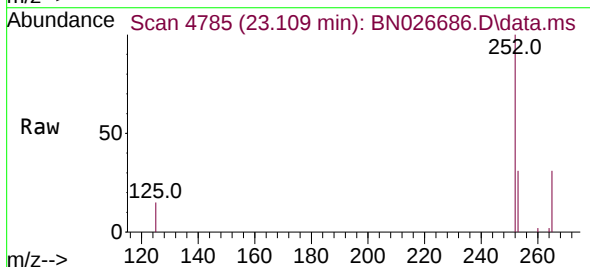

Tgt Ion:252 Resp: 11694
Ion Ratio Lower Upper
252 100
253 31.2 27.2 40.8
125 15.0 13.4 20.2

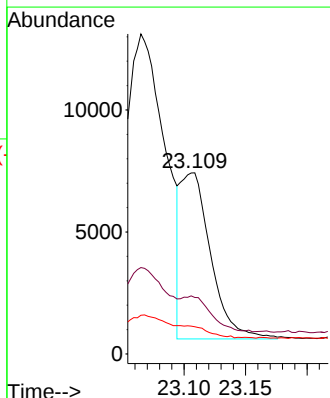

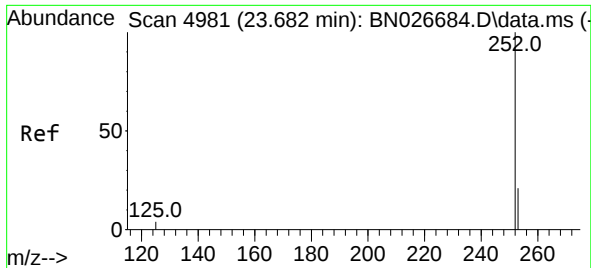





#26
Benzo(a)pyrene
Concen: 0.168 ng/ul
RT: 23.679 min Scan# 4981
Delta R.T. -0.006 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23

Instrument :
BNA_N
ClientSampleId :
A46T0DL

Tgt Ion:252 Resp: 606
Ion Ratio Lower Upper
252 100
253 43.9 32.6 49.0
125 25.6 19.3 28.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

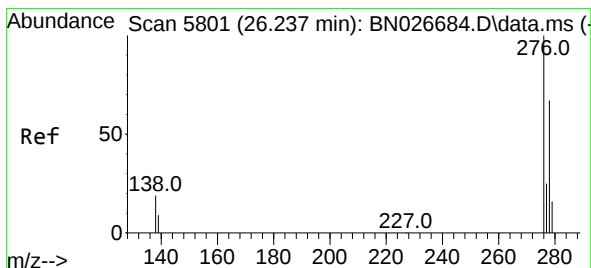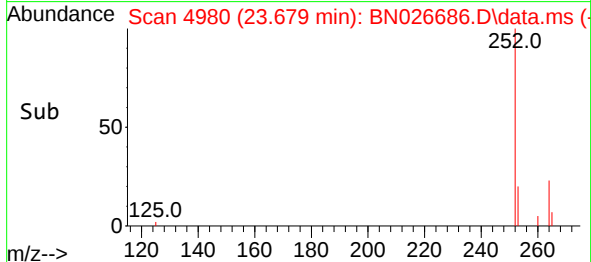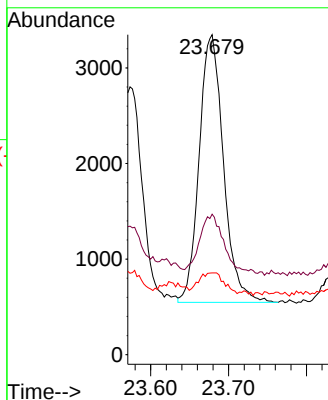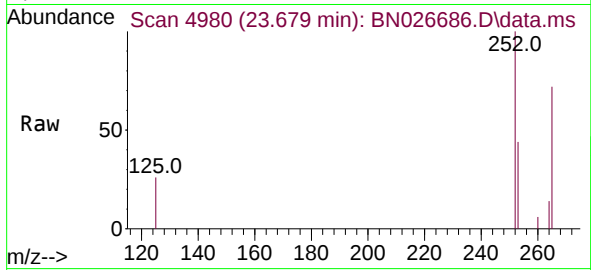

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.191 ng/ul
RT: 26.230 min Scan# 5799
Delta R.T. -0.021 min
Lab File: BN026686.D
Acq: 23 Jul 2023 21:23


Tgt Ion:276 Resp: 9018
Ion Ratio Lower Upper
276 100
138 17.3 22.2 33.4#
227 0.2 0.1 0.1#

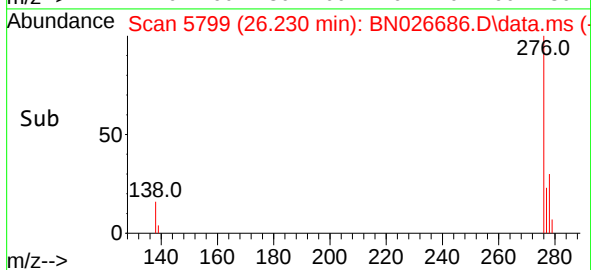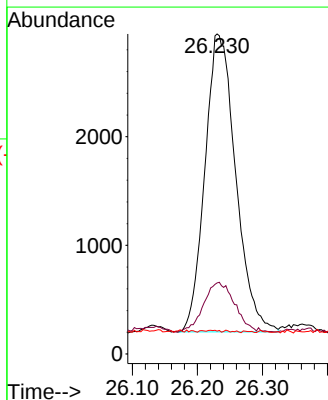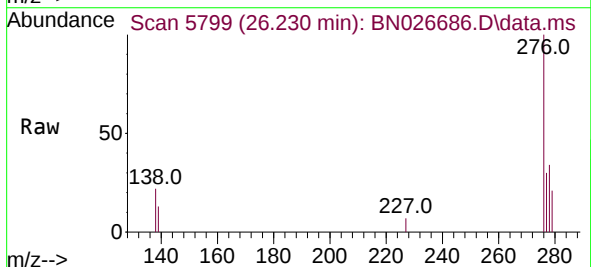

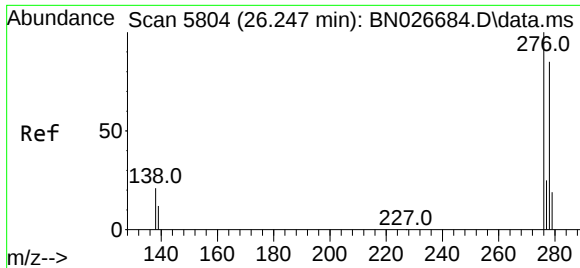

#28
 Dibenzo(a,h)anthracene
 Concen: 0.095 ng/ul
 RT: 26.240 min Scan# 5802
 Delta R.T. -0.017 min
 Lab File: BN026686.D
 Acq: 23 Jul 2023 21:23

Instrument :
 BNA_N
 ClientSampleId :
 A46T0DL

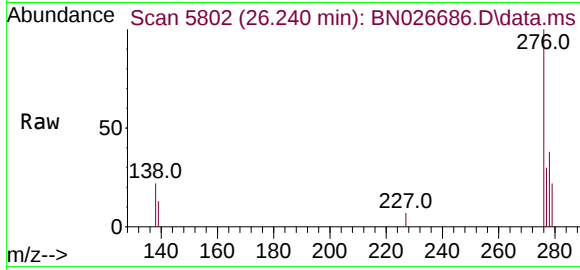

Tgt Ion: 278 Resp: 3428
 Ion Ratio Lower Upper
 278 100
 139 35.3 18.9 28.3
 279 58.6 31.3 46.9

Manual Integrations
 APPROVED

Reviewed By : Yogesh Patel 07/24/2023
 Supervised By : mohammad ahmed 07/24/2023

