

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
 Data File : BN026732.D
 Acq On : 25 Jul 2023 03:39
 Operator : MA/JU
 Sample : 03611-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-RW5A-20230712

Quant Time: Jul 25 04:07:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 23:51:48 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.842	152	5	0.400	ng	# 0.00
7) Naphthalene-d8	10.682	136	37	0.400	ng	# 0.05
13) Acenaphthene-d10	14.501	164	6	0.400	ng	# 0.04
19) Phenanthrene-d10	17.244	188	13	0.400	ng	# 0.02
29) Chrysene-d12	21.417	240	42	0.400	ng	# 0.00
35) Perylene-d12	23.797	264	14	0.400	ng	# 0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.408	112	98	8.079	ng	0.00
5) Phenol-d6	7.033	99	151	9.767	ng	0.00
8) Nitrobenzene-d5	9.048	82	780	24.649	ng	0.01
11) 2-Methylnaphthalene-d10	12.222	152	2817	52.071	ng	0.00
14) 2,4,6-Tribromophenol	16.003	330	7	3.207	ng	0.02
15) 2-Fluorobiphenyl	13.090	172	4717	203.631	ng	-0.01
27) Fluoranthene-d10	19.249	212	7164	260.086	ng	0.00
31) Terphenyl-d14	19.839	244	5777	53.747	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.227	88	9327	1763.476	ng	# 90
3) n-Nitrosodimethylamine	3.610	42	289	53.939	ng	# 1
6) bis(2-Chloroethyl)ether	7.315	93	56	4.398	ng	# 1
9) Naphthalene	10.703	128	68	0.679	ng	# 1
10) Hexachlorobutadiene	10.981	225	8	0.414	ng	# 51
12) 2-Methylnaphthalene	12.366	142	3	0.043	ng	# 31
16) Acenaphthylene	14.191	152	61	2.168	ng	# 66
17) Acenaphthene	14.534	154	28	1.541	ng	# 1
18) Fluorene	15.519	166	33	1.393	ng	# 72
20) 4,6-Dinitro-2-methylph...	16.164	198	17	9.068	ng	# 1
21) 4-Bromophenyl-phenylether	16.400	248	4	0.539	ng	# 52
22) Hexachlorobenzene	16.574	284	4	0.538	ng	# 1
23) Atrazine	16.698	200	17	2.667	ng	# 1
24) Pentachlorophenol	16.934	266	46	13.131	ng	# 42
25) Phenanthrene	17.269	178	271	7.115	ng	# 84
26) Anthracene	17.381	178	264	7.698	ng	# 1
28) Fluoranthene	19.277	202	288	7.200	ng	# 72
30) Pyrene	19.648	202	319	1.371	ng	96
32) Benzo(a)anthracene	21.426	228	102	0.675	ng	# 1
33) Chrysene	21.462	228	64	0.380	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.300	149	14187	105.204	ng	# 95
36) Indeno(1,2,3-cd)pyrene	26.261	276	16	0.278	ng	# 17
37) Benzo(b)fluoranthene	23.078	252	118	2.324	ng	# 1
38) Benzo(k)fluoranthene	23.113	252	39	0.710	ng	# 1
39) Benzo(a)pyrene	23.697	252	18	0.361	ng	# 1
40) Dibenzo(a,h)anthracene	26.267	278	5	0.111	ng	# 1
41) Benzo(g,h,i)perylene	27.010	276	14	0.267	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026732.D
Acq On : 25 Jul 2023 03:39
Operator : MA/JU
Sample : 03611-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712

Quant Time: Jul 25 04:07:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 23:51:48 2023
Response via : Initial Calibration




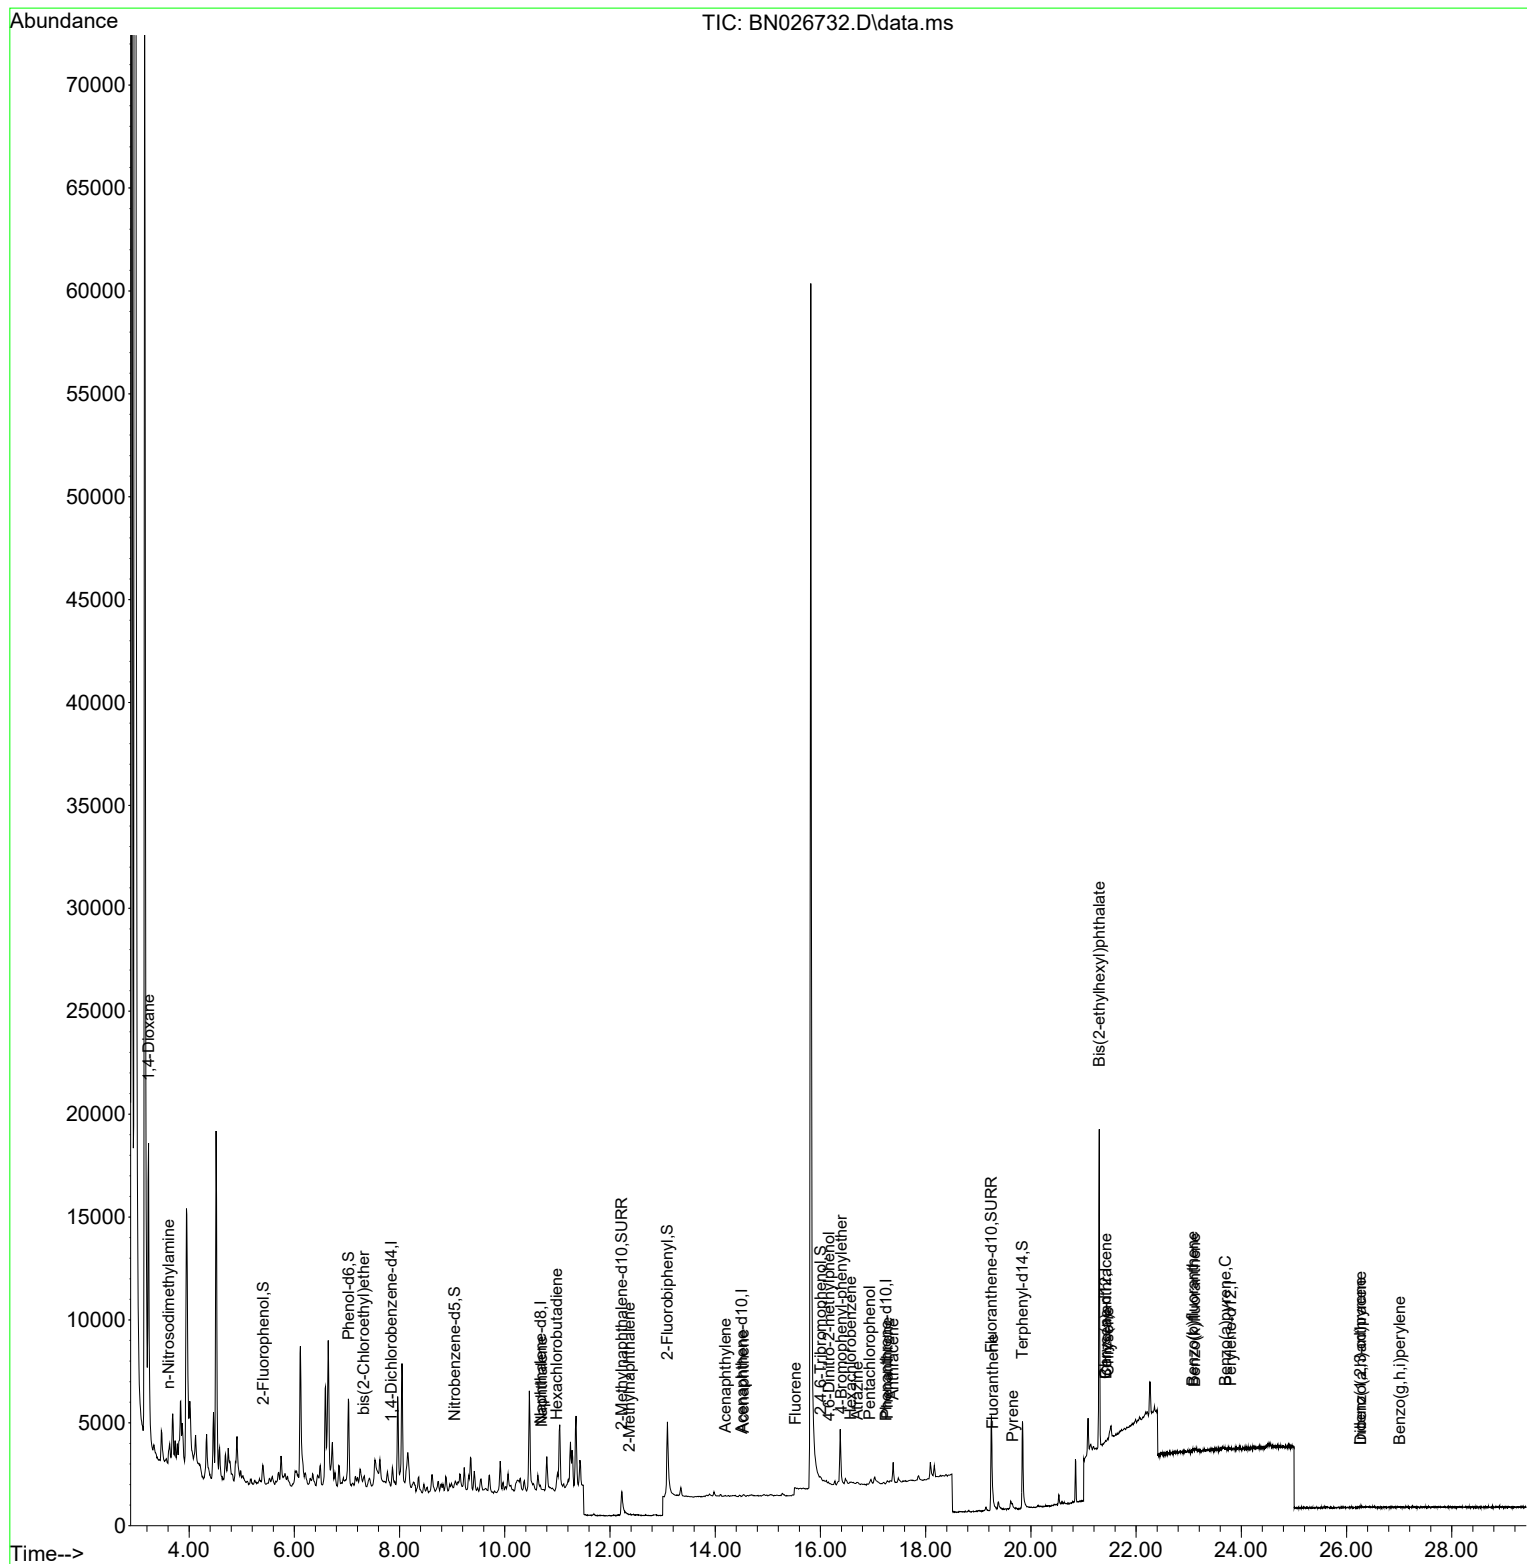




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.842 min Scan# 61
Delta R.T. 0.007 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion:152 Resp: 5
Ion Ratio Lower Upper
152 100
150 86.9 124.7 187.1#
115 149.2 48.2 72.4#

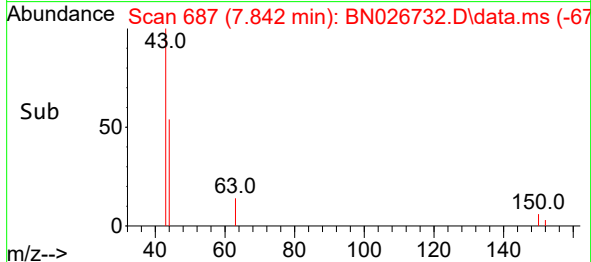

#2
1,4-Dioxane
Concen: 1763.476 ng
RT: 3.227 min Scan# 48
Delta R.T. -0.007 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion: 88 Resp: 9327
Ion Ratio Lower Upper
88 100
43 46.5 24.2 36.4#
58 66.0 53.3 79.9


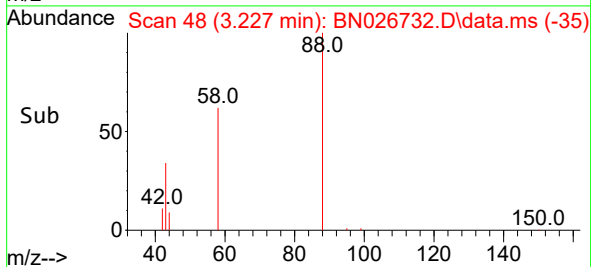

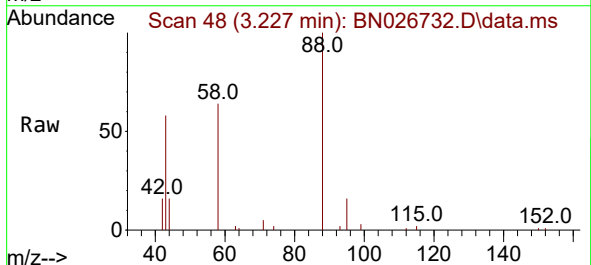




#3
n-Nitrosodimethylamine
Concen: 53.939 ng
RT: 3.610 min Scan# 101
Delta R.T. -0.022 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion: 42 Resp: 289
Ion Ratio Lower Upper
42 100
74 12.8 93.8 140.8#
44 128.7 3.0 4.4#

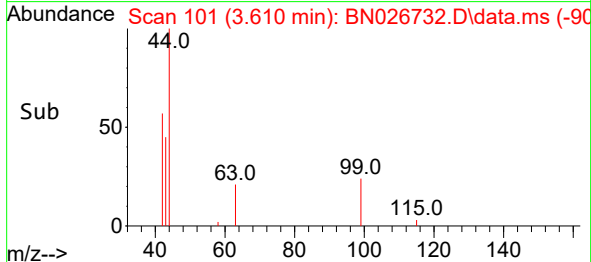

#4
2-Fluorophenol
Concen: 8.079 ng
RT: 5.408 min Scan# 350
Delta R.T. -0.007 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion: 112 Resp: 98
Ion Ratio Lower Upper
112 100
64 19.4 45.8 68.6#
63 43.9 27.4 41.2#

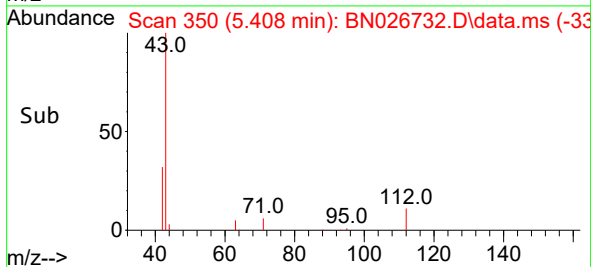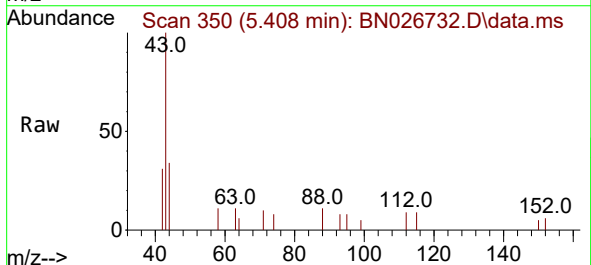



#5

Phenol-d6

Concen: 9.767 ng

RT: 7.033 min Scan# 51

Delta R.T. -0.007 min

Lab File: BN026732.D


Acq: 25 Jul 2023 03:39

Instrument :




BNA_N

ClientSampleId :

BP-TT-RW5A-20230712

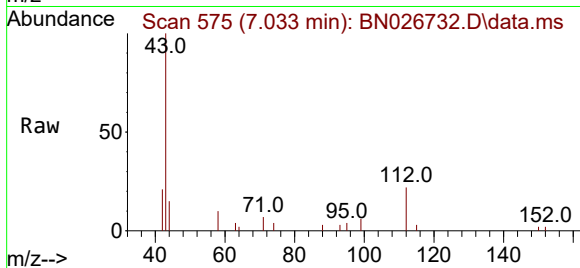

Tgt Ion:	99	Resp:	151
Ion	Ratio	Lower	Upper
99	100		
42	581.5	18.4	27.6#
71	176.2	30.6	46.0#

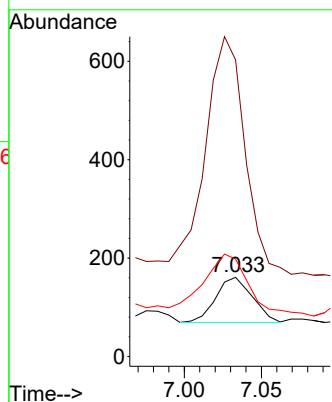

#6

bis(2-Chloroethyl)ether

Concen: 4.398 ng




RT: 7.315 min Scan# 614


Delta R.T. 0.022 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Tgt Ion:	93	Resp:	56
Ion	Ratio	Lower	Upper
93	100		
63	0.0	58.8	88.2#
95	214.3	29.2	43.8#


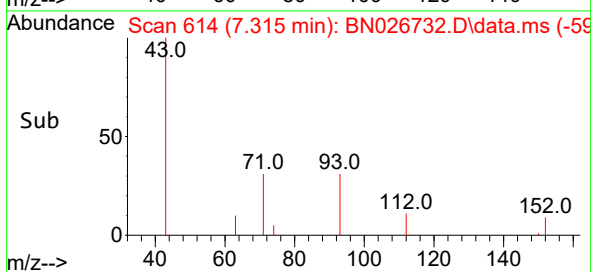

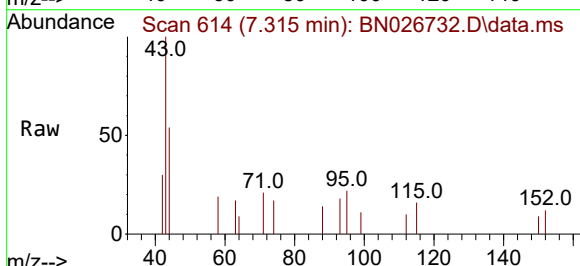


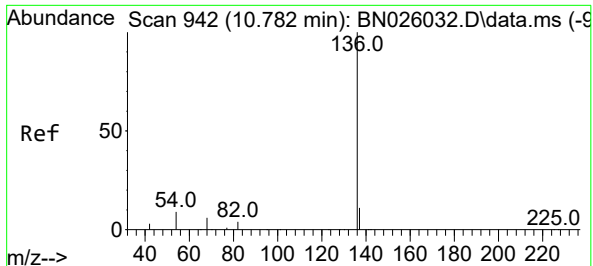

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.682 min Scan# 91
Delta R.T. 0.053 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion:	136	Resp:	37
Ion Ratio	Lower	Upper	
136	100		
137	84.1	9.0	13.4#
54	123.8	7.8	11.6#
68	139.7	5.8	8.8#

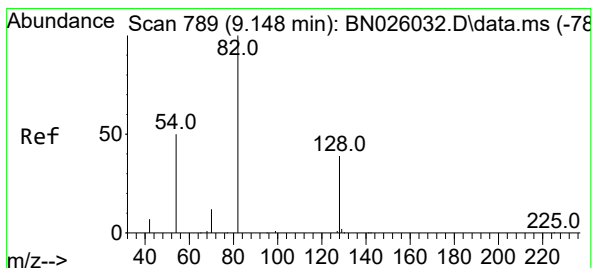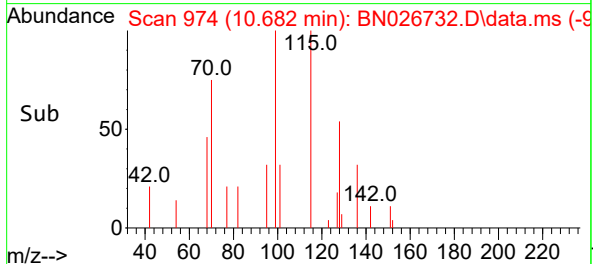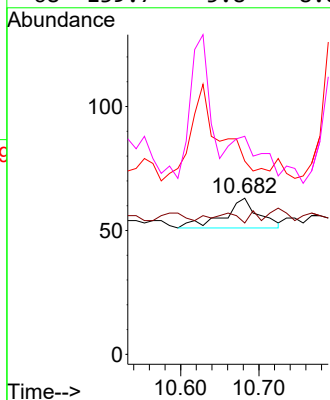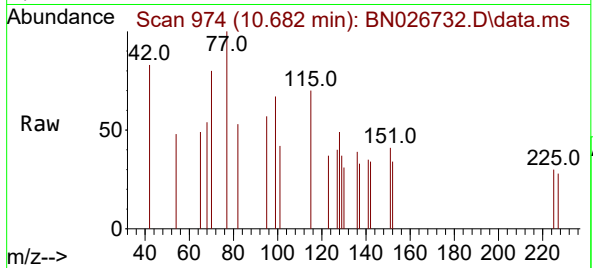

#8
Nitrobenzene-d5
Concen: 24.649 ng
RT: 9.048 min Scan# 821
Delta R.T. 0.011 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion:	82	Resp:	780
Ion Ratio	Lower	Upper	
82	100		
128	57.1	33.4	50.2#
54	82.9	41.7	62.5#

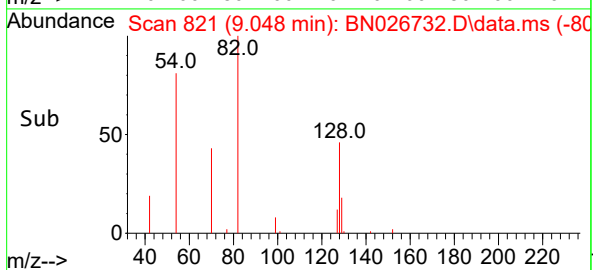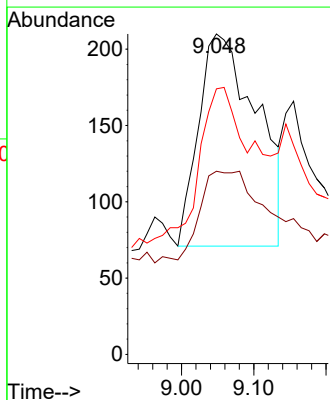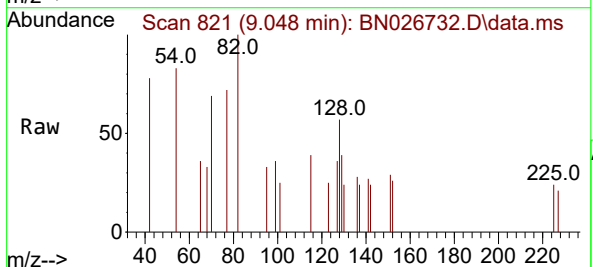

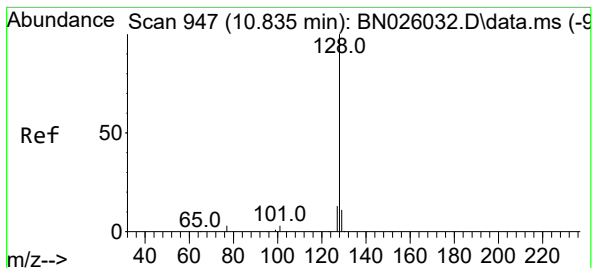

#9

Naphthalene

Concen: 0.679 ng

RT: 10.703 min Scan# 91

Delta R.T. 0.021 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:128 Resp: 68

Ion Ratio Lower Upper

128 100

129 68.1 9.1 13.7#

127 64.9 10.9 16.3#

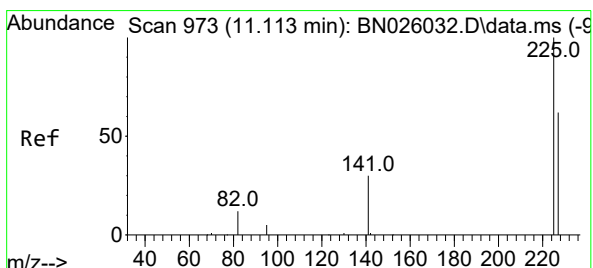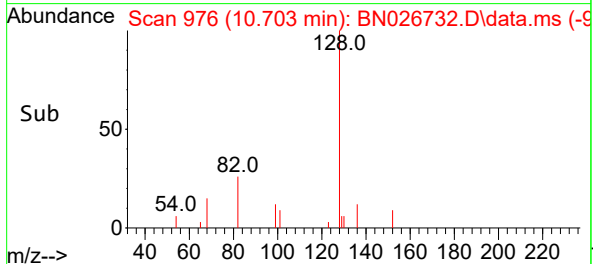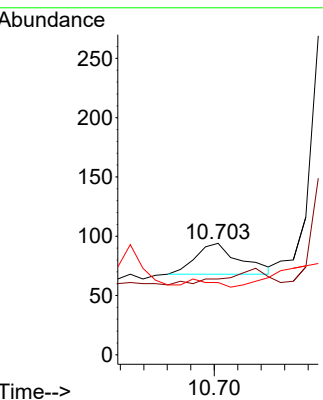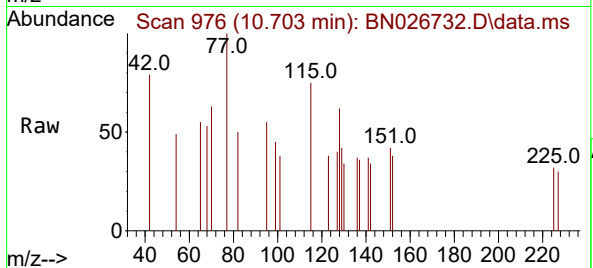

#10

Hexachlorobutadiene

Concen: 0.414 ng

RT: 10.981 min Scan# 1002

Delta R.T. 0.043 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:225 Resp: 8


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 25.0 50.3 75.5#


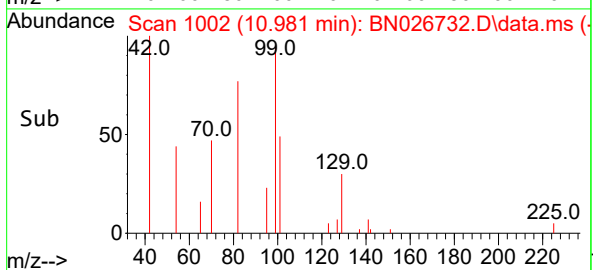
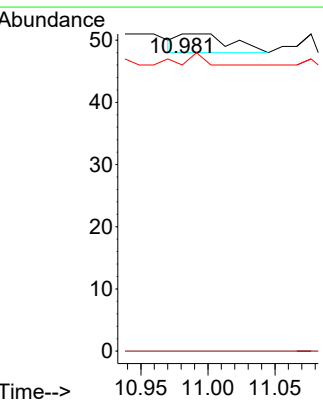
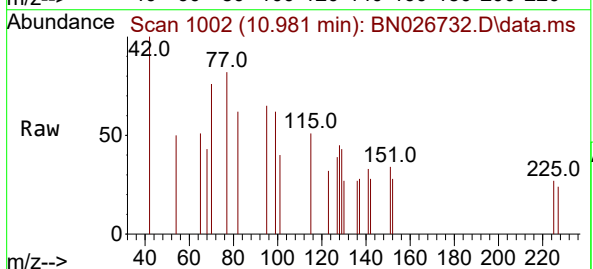




#11
2-Methylnaphthalene-d10
Concen: 52.071 ng
RT: 12.222 min Scan# 11
Delta R.T. -0.007 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion:152 Resp: 2817
Ion Ratio Lower Upper
152 100
151 18.7 16.2 24.2

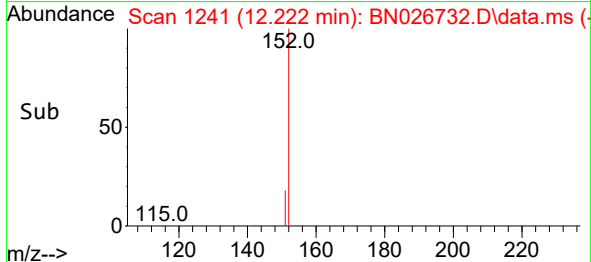

#12
2-Methylnaphthalene
Concen: 0.043 ng
RT: 12.366 min Scan# 1279
Delta R.T. 0.064 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion:142 Resp: 3
Ion Ratio Lower Upper
142 100
141 103.5 71.7 107.5
115 157.9 33.4 50.0#

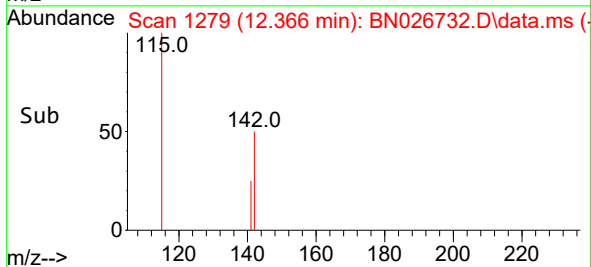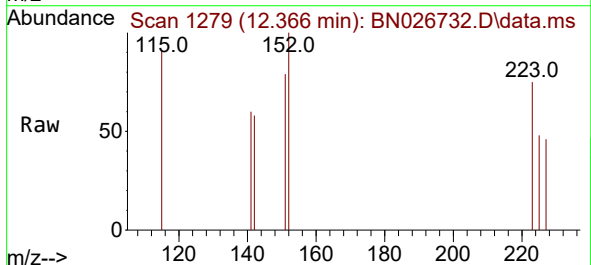



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.501 min Scan# 1

Delta R.T. 0.043 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:164 Resp: 6

Ion Ratio Lower Upper

164 100

162 92.7 85.3 127.9

160 90.9 40.0 60.0#

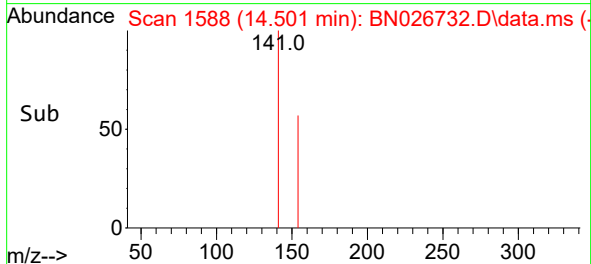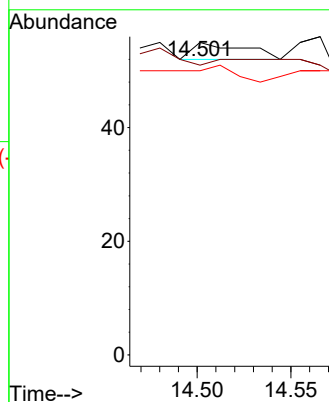

#14

2,4,6-Tribromophenol

Concen: 3.207 ng

RT: 16.003 min Scan# 1722

Delta R.T. 0.025 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:330 Resp: 7


Ion Ratio Lower Upper

330 100

332 0.0 76.0 114.0#

141 0.0 42.8 64.2#

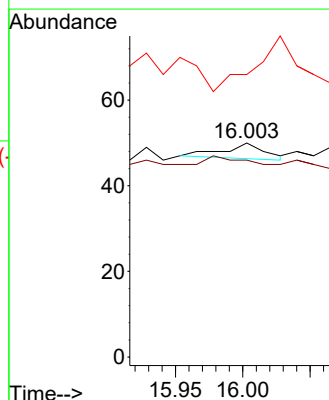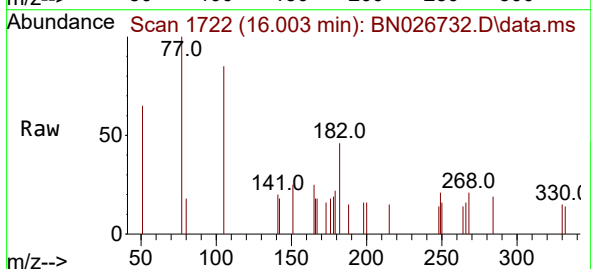

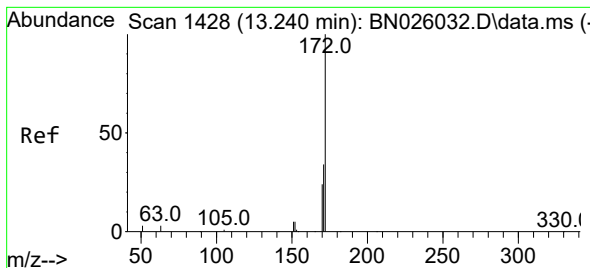

#15

2-Fluorobiphenyl

Concen: 203.631 ng

RT: 13.090 min Scan# 1428

Delta R.T. -0.011 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:172 Resp: 4717

Ion Ratio Lower Upper

172 100

171 37.0 27.8 41.8

170 24.4 19.3 28.9

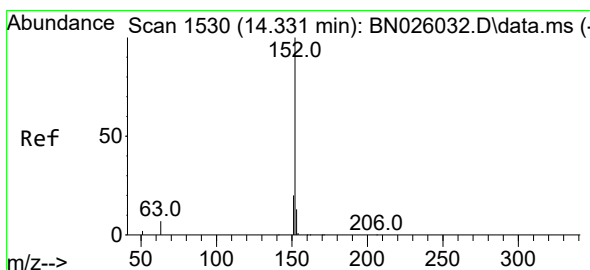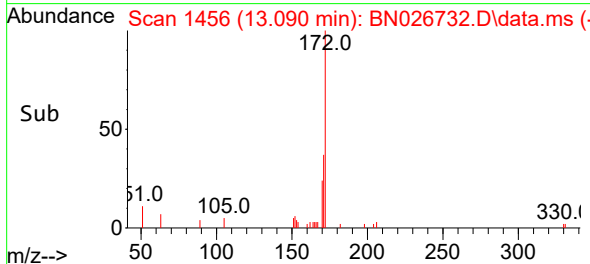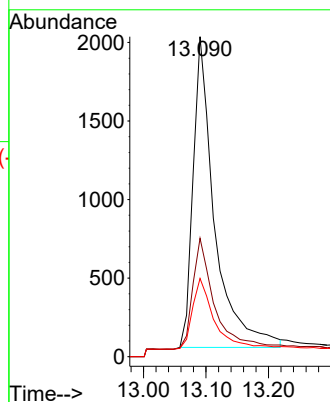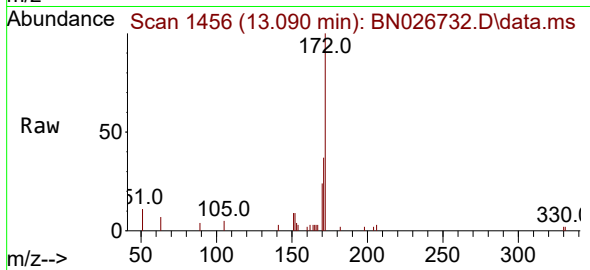

#16

Acenaphthylene

Concen: 2.168 ng

RT: 14.191 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:152 Resp: 61


Ion Ratio Lower Upper

152 100

151 36.1 15.9 23.9#

153 0.0 10.6 15.8#

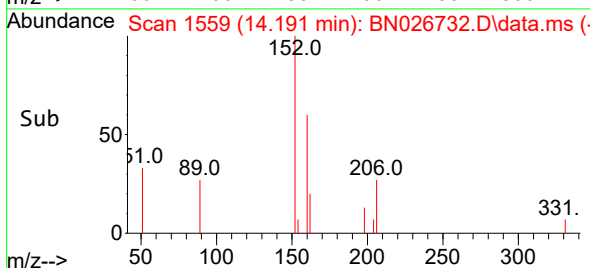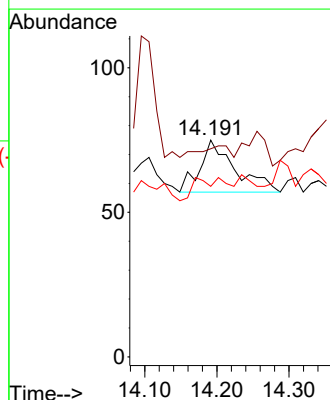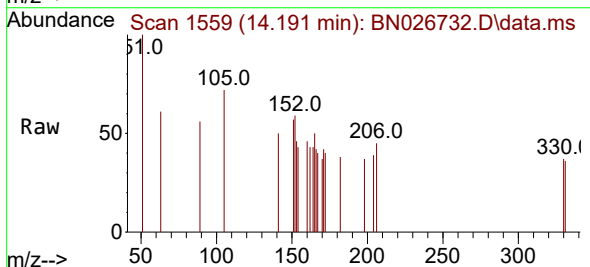



#17

Acenaphthene

Concen: 1.541 ng

RT: 14.534 min Scan# 1591

Delta R.T. 0.011 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:154 Resp: 28

Ion Ratio Lower Upper

154 100

153 332.1 94.4 141.6#

152 0.0 46.1 69.1#

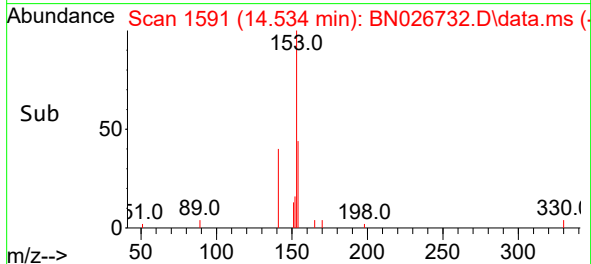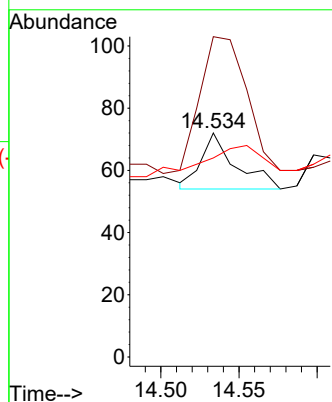

#18

Fluorene

Concen: 1.393 ng

RT: 15.519 min Scan# 1683

Delta R.T. 0.000 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:166 Resp: 33


Ion Ratio Lower Upper

166 100

165 118.2 79.7 119.5

167 51.5 10.6 16.0#



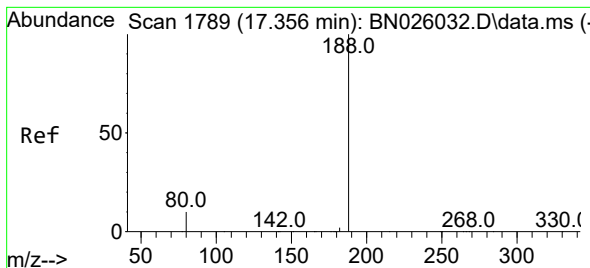

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.244 min Scan# 1735

Delta R.T. 0.025 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:188 Resp: 13

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 118.2 8.6 13.0#

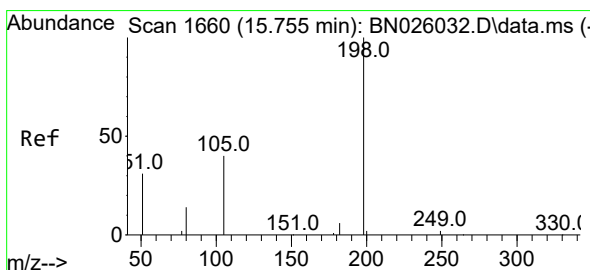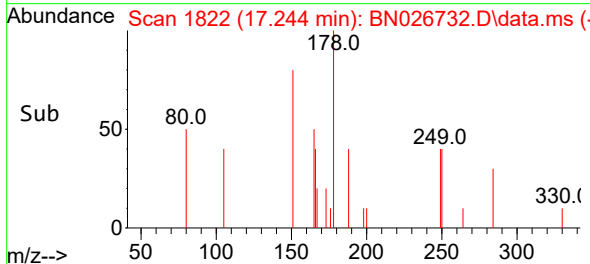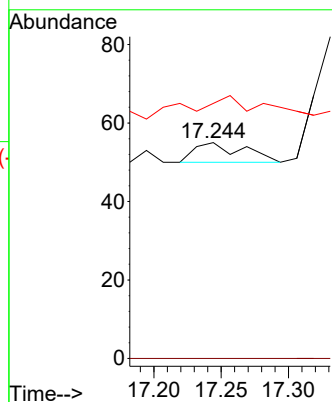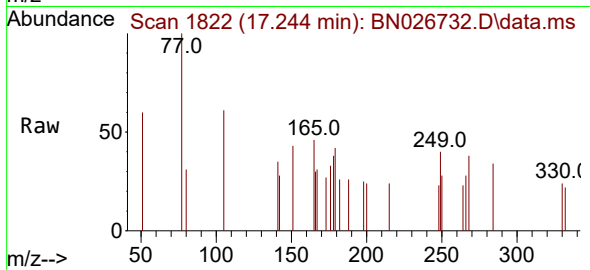

#20

4,6-Dinitro-2-methylphenol

Concen: 9.068 ng

RT: 16.164 min Scan# 1735

Delta R.T. 0.013 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:198 Resp: 17


Ion Ratio Lower Upper

198 100

51 274.5 85.8 128.8#

105 287.3 48.2 72.2#


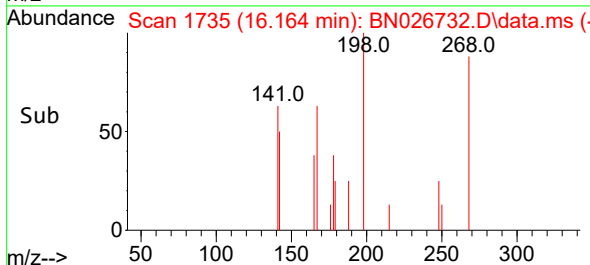

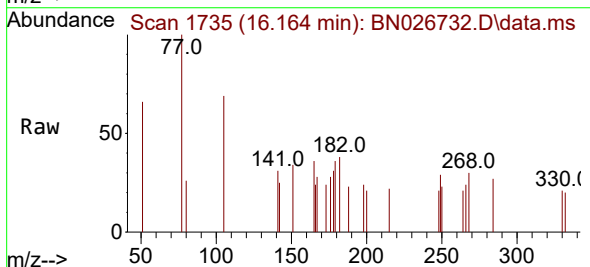




#21
4-Bromophenyl-phenylether
Concen: 0.539 ng
RT: 16.400 min Scan# 1768
Delta R.T. -0.012 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion:248 Resp: 4
Ion Ratio Lower Upper
248 100
250 108.2 79.9 119.9
141 138.8 41.6 62.4#

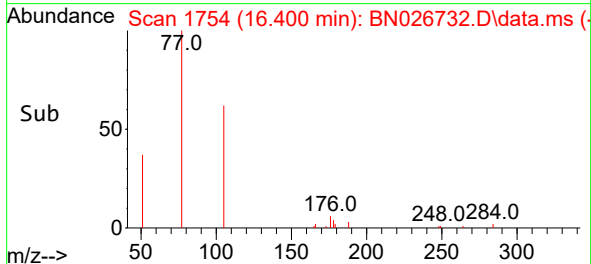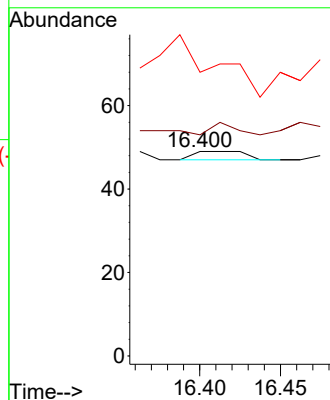

#22
Hexachlorobenzene
Concen: 0.538 ng
RT: 16.574 min Scan# 1768
Delta R.T. 0.050 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion:284 Resp: 4
Ion Ratio Lower Upper
284 100
142 250.0 38.7 58.1#
249 0.0 28.5 42.7#

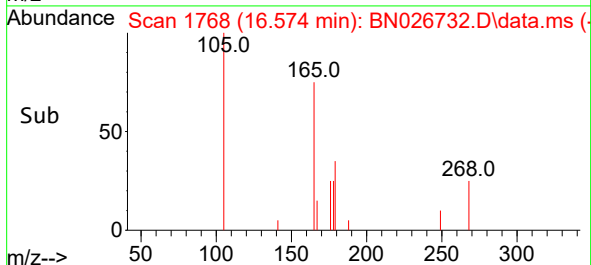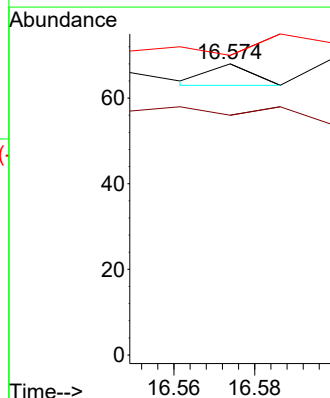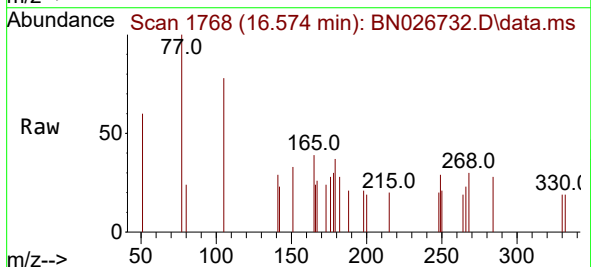



#23

Atrazine

Concen: 2.667 ng

RT: 16.698 min Scan# 11

Delta R.T. 0.012 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:200 Resp: 17

Ion Ratio Lower Upper

200 100

173 103.7 22.9 34.3#

215 103.7 35.5 53.3#

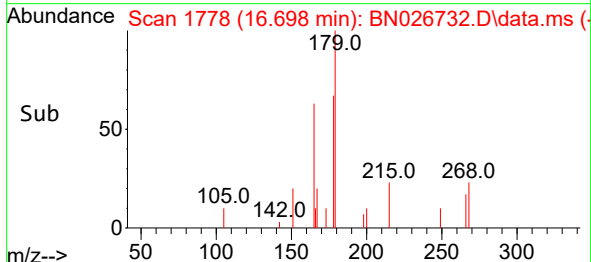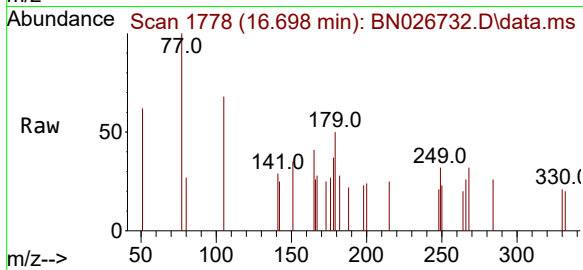

#24

Pentachlorophenol

Concen: 13.131 ng

RT: 16.934 min Scan# 1797

Delta R.T. 0.037 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:266 Resp: 46


Ion Ratio Lower Upper

266 100

264 0.0 49.3 73.9#

268 87.0 48.3 72.5#

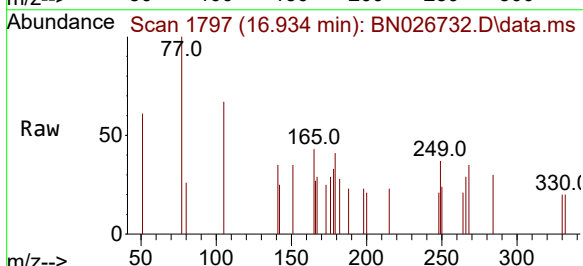

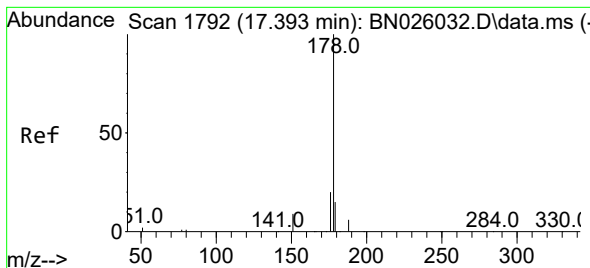

#25

Phenanthrene

Concen: 7.115 ng

RT: 17.269 min Scan# 1824

Delta R.T. 0.013 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:178 Resp: 271

Ion Ratio Lower Upper

178 100

176 22.1 15.6 23.4

179 27.3 12.3 18.5#

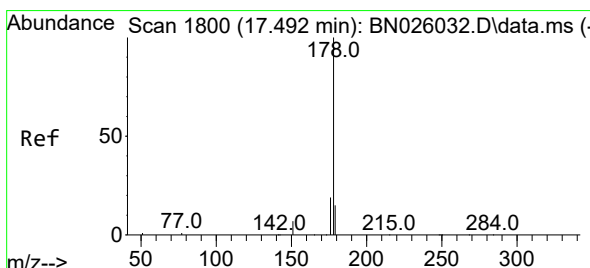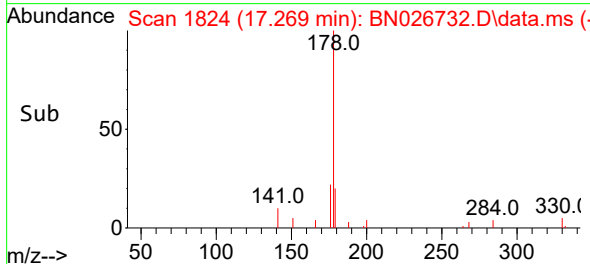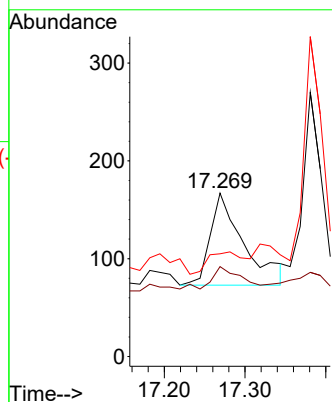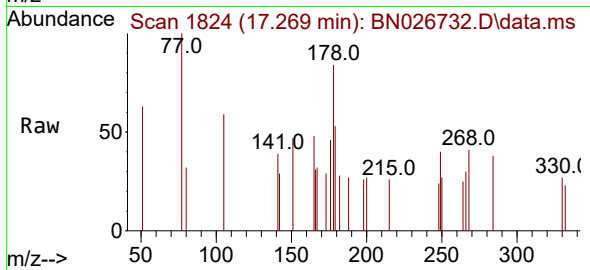

#26

Anthracene

Concen: 7.698 ng

RT: 17.381 min Scan# 1833

Delta R.T. 0.025 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:178 Resp: 264


Ion Ratio Lower Upper

178 100

176 21.2 15.0 22.4

179 136.0 12.4 18.6#

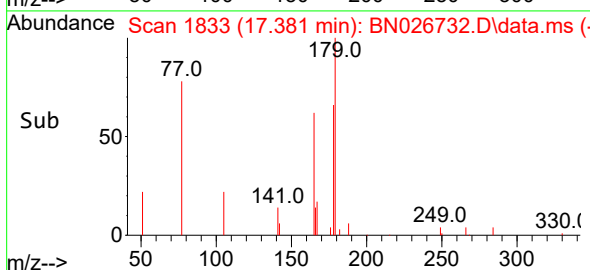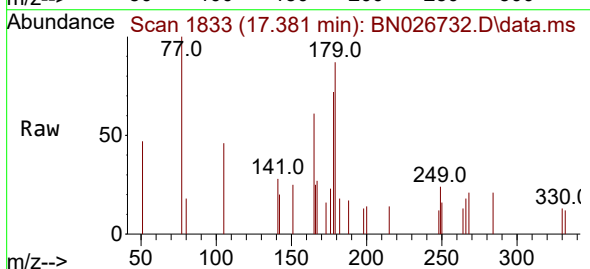



#27

Fluoranthene-d10

Concen: 260.086 ng

RT: 19.249 min Scan# 2083

Delta R.T. 0.000 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:212 Resp: 7164

Ion Ratio Lower Upper

212 100

106 6.8 11.6 17.4#

104 6.8 7.2 10.8#

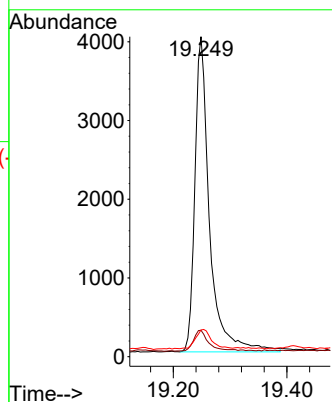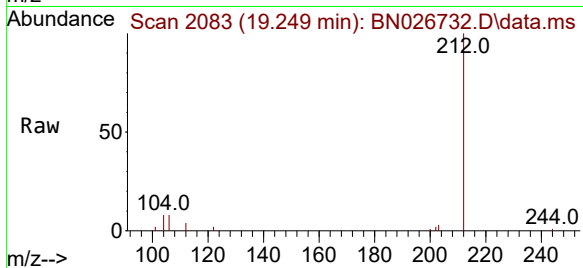

#28

Fluoranthene

Concen: 7.200 ng

RT: 19.277 min Scan# 2089

Delta R.T. -0.005 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:202 Resp: 288


Ion Ratio Lower Upper

202 100

101 36.8 8.3 12.5#

203 17.4 13.5 20.3




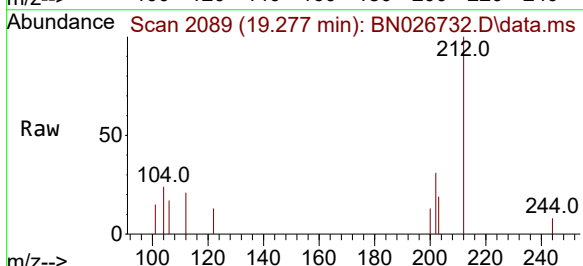


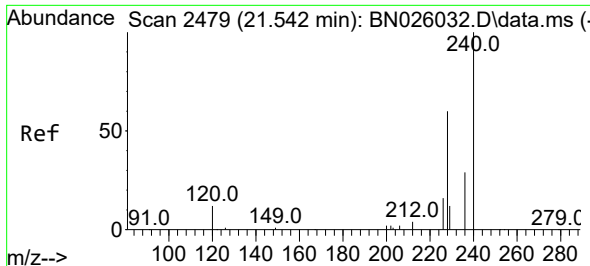

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.417 min Scan# 2169
Delta R.T. 0.009 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5A-20230712


Tgt Ion:240 Resp: 42
Ion Ratio Lower Upper
240 100
120 263.5 14.6 22.0#
236 139.6 24.2 36.2#

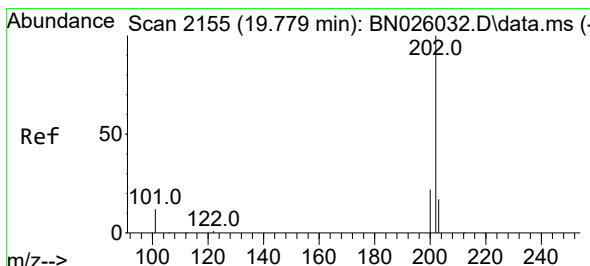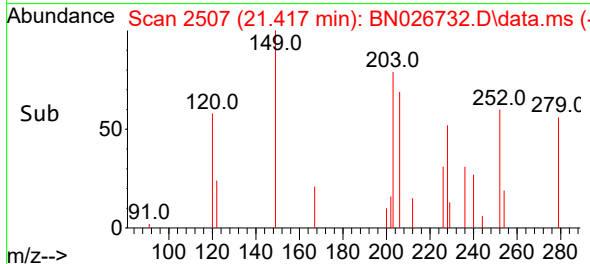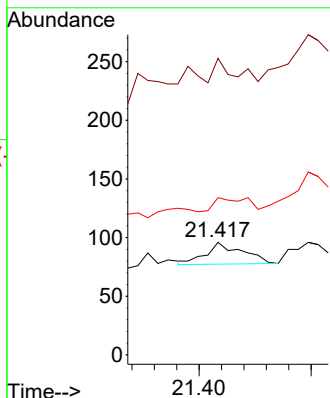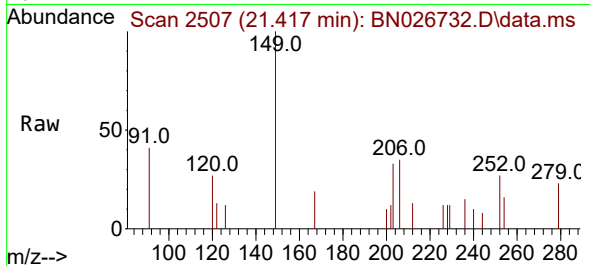

#30
Pyrene
Concen: 1.371 ng
RT: 19.648 min Scan# 2169
Delta R.T. 0.005 min
Lab File: BN026732.D
Acq: 25 Jul 2023 03:39

Tgt Ion:202 Resp: 319
Ion Ratio Lower Upper
202 100
200 22.3 17.0 25.4
203 20.1 14.2 21.4

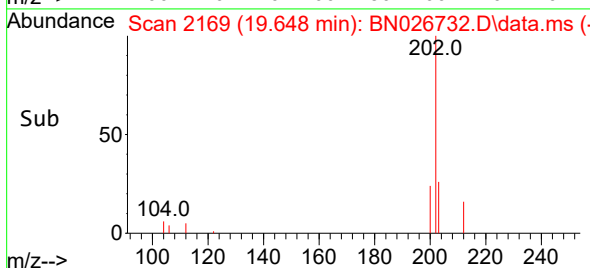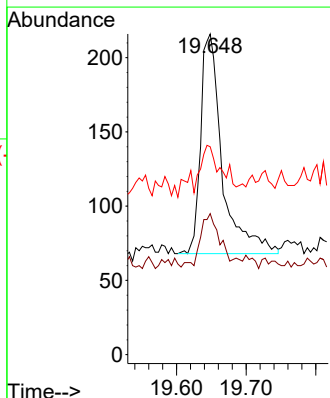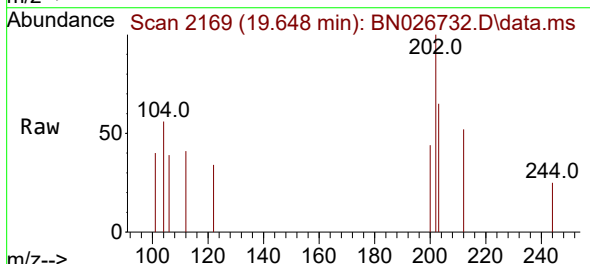



#31

Terphenyl-d14

Concen: 53.747 ng

RT: 19.839 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:244 Resp: 5777

Ion Ratio Lower Upper

244 100

212 11.7 8.7 13.1

122 11.7 13.7 20.5#

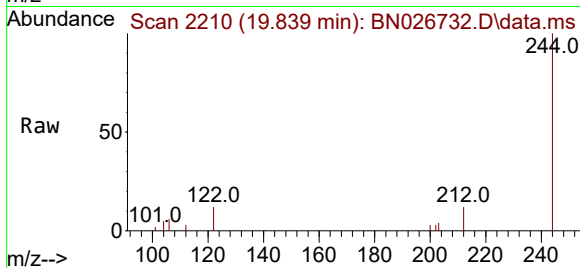

#32

Benzo(a)anthracene

Concen: 0.675 ng

RT: 21.426 min Scan# 2508

Delta R.T. 0.027 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:228 Resp: 102


Ion Ratio Lower Upper

228 100

226 98.3 23.0 34.6#

229 94.8 15.9 23.9#

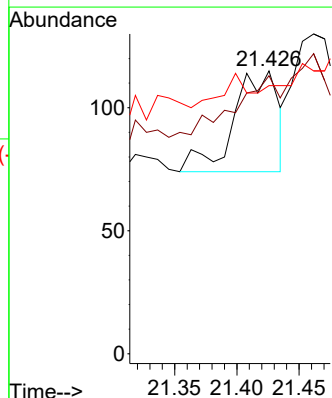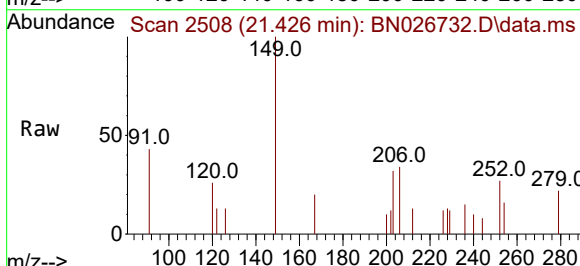



#33

Chrysene

Concen: 0.380 ng

RT: 21.462 min Scan# 21

Delta R.T. 0.018 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:228 Resp: 64

Ion Ratio Lower Upper

228 100

226 93.8 24.8 37.2#

229 88.5 15.6 23.4#

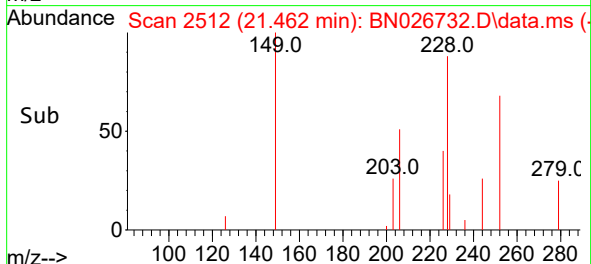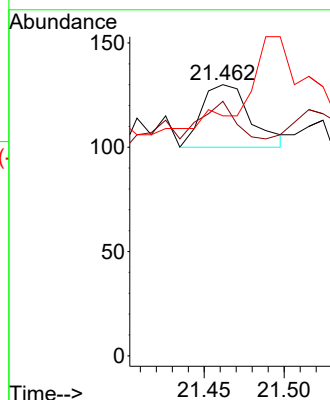

#34

Bis(2-ethylhexyl)phthalate

Concen: 105.204 ng

RT: 21.300 min Scan# 2494

Delta R.T. 0.000 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:149 Resp: 14187


Ion Ratio Lower Upper

149 100

167 27.9 20.2 30.4


279 4.5 2.4 3.6#

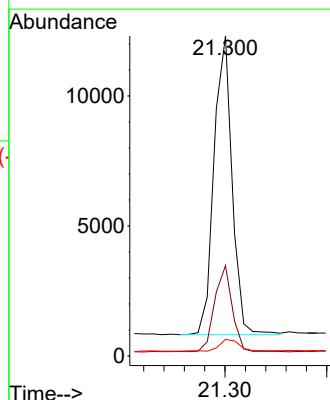






#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.797 min Scan# 3092
 Delta R.T. 0.015 min
 Lab File: BN026732.D
 Acq: 25 Jul 2023 03:39

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-RW5A-20230712







Tgt Ion:264 Resp: 14
 Ion Ratio Lower Upper
 264 100
 260 72.2 21.9 32.9#
 265 1663.5 80.3 120.5#

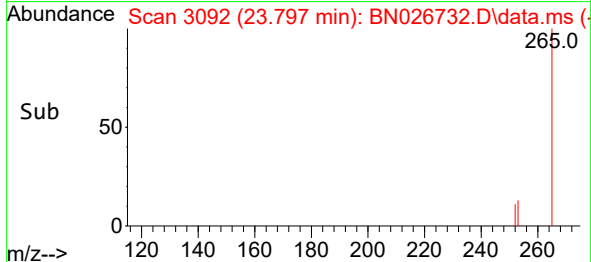

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.278 ng
 RT: 26.261 min Scan# 3935
 Delta R.T. 0.021 min
 Lab File: BN026732.D
 Acq: 25 Jul 2023 03:39

Tgt Ion:276 Resp: 16
 Ion Ratio Lower Upper
 276 100
 138 37.5 21.4 32.2#
 277 100.0 19.6 29.4#

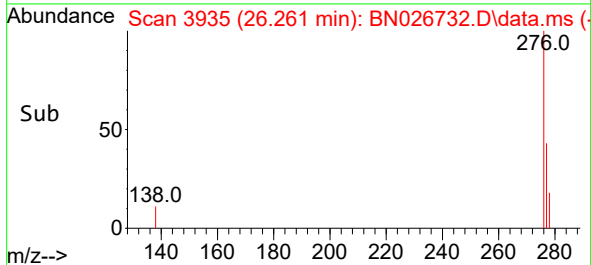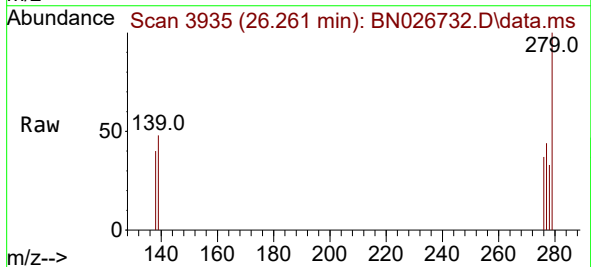



#37

Benzo(b)fluoranthene

Concen: 2.324 ng

RT: 23.078 min Scan# 2846

Delta R.T. 0.018 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712





Tgt Ion:252 Resp: 118

Ion Ratio Lower Upper

252 100

253 147.5 24.1 36.1#

125 82.9 15.4 23.0#



#38

Benzo(k)fluoranthene

Concen: 0.710 ng

RT: 23.113 min Scan# 2858

Delta R.T. 0.006 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:252 Resp: 39


Ion Ratio Lower Upper

252 100

253 161.7 23.6 35.4#

125 90.2 15.8 23.8#





#39

Benzo(a)pyrene

Concen: 0.361 ng

RT: 23.697 min Scan# 3089

Delta R.T. 0.018 min

Lab File: BN026732.D


Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712






Tgt Ion:252 Resp: 18

Ion Ratio Lower Upper

252 100

253 166.0 26.2 39.4#

125 84.2 18.7 28.1#

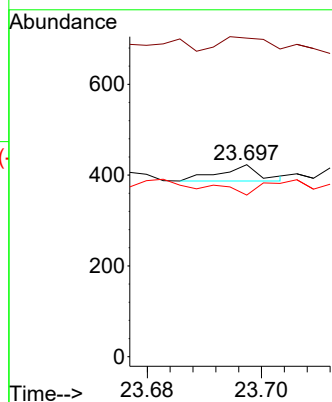

#40

Dibenzo(a,h)anthracene

Concen: 0.111 ng

RT: 26.267 min Scan# 3937

Delta R.T. 0.015 min

Lab File: BN026732.D

Acq: 25 Jul 2023 03:39




Tgt Ion:278 Resp: 5


Ion Ratio Lower Upper

278 100

139 143.3 18.1 27.1#

279 308.7 25.4 38.0#

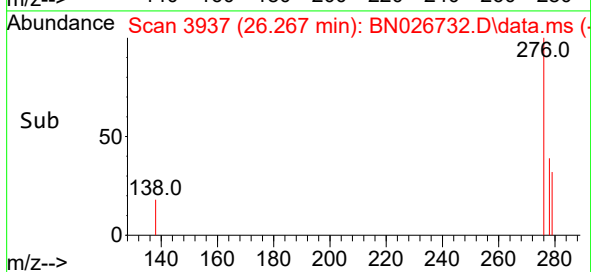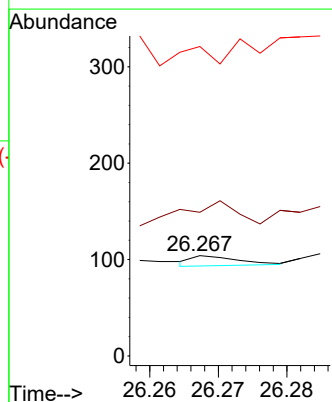

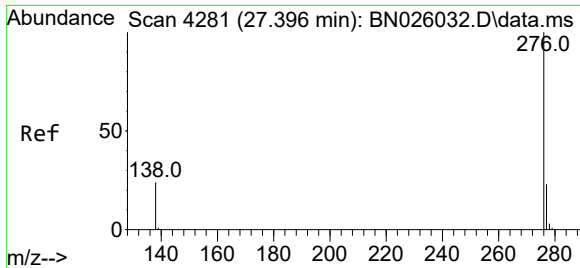

#41

Benzo(g,h,i)perylene

Concen: 0.267 ng

RT: 27.010 min Scan# 41

Delta R.T. 0.018 min

Lab File: BN026732.D


Acq: 25 Jul 2023 03:39

Instrument :

BNA_N

ClientSampleId :

BP-TT-RW5A-20230712

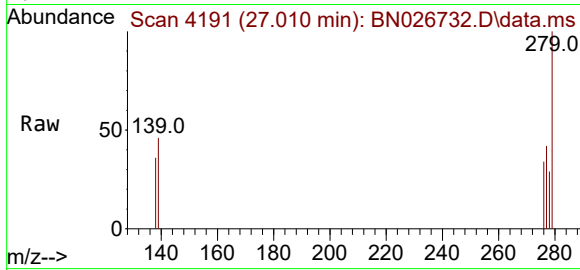

Tgt Ion:276 Resp: 14

Ion Ratio Lower Upper

276 100

277 121.8 20.3 30.5#

138 103.6 21.5 32.3#

