
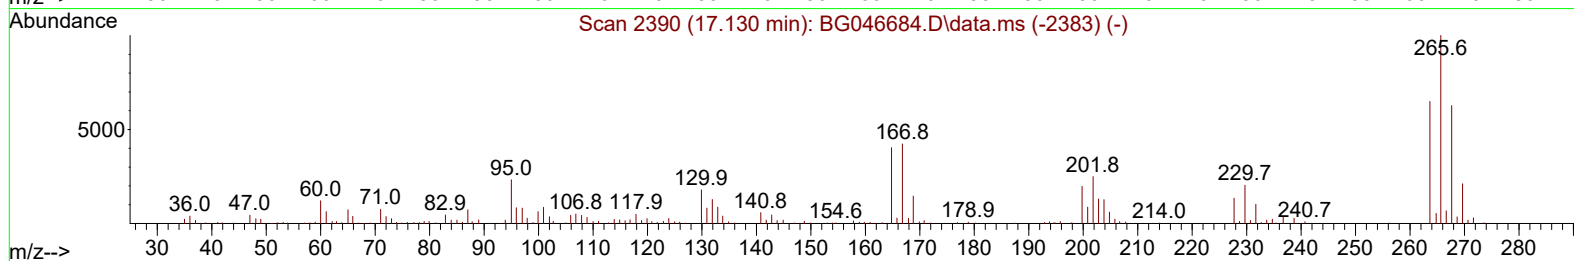
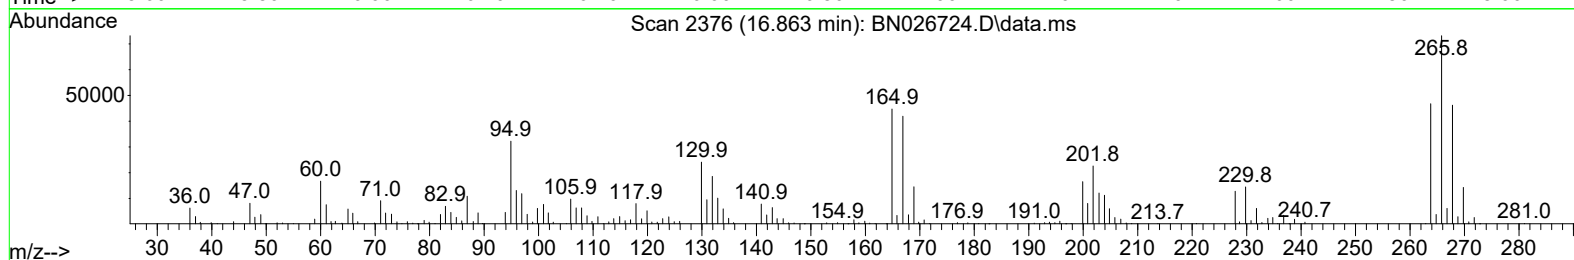


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026724.D
Acq On : 24 Jul 2023 22:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 04:18:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

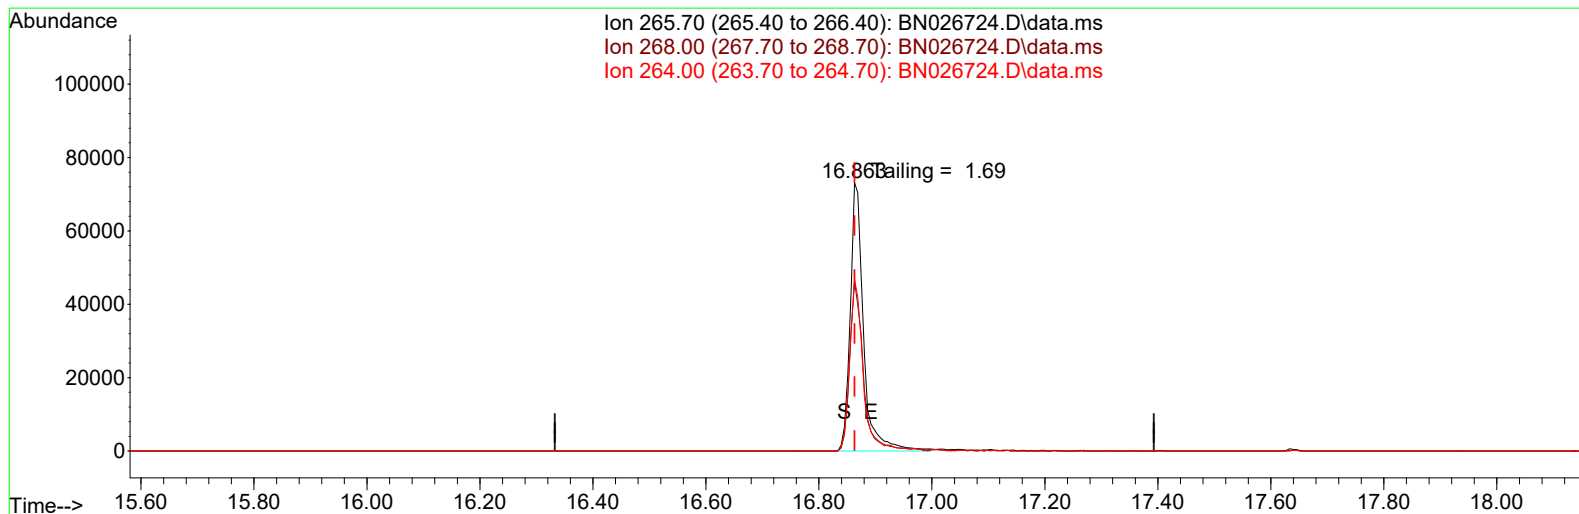

TIC: BN026724.D\data.ms

(70) Pentachlorophenol (C)




16.863min (0.000) 13247.60 ng

response 120598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026724.D
Acq On : 24 Jul 2023 22:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 04:18:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

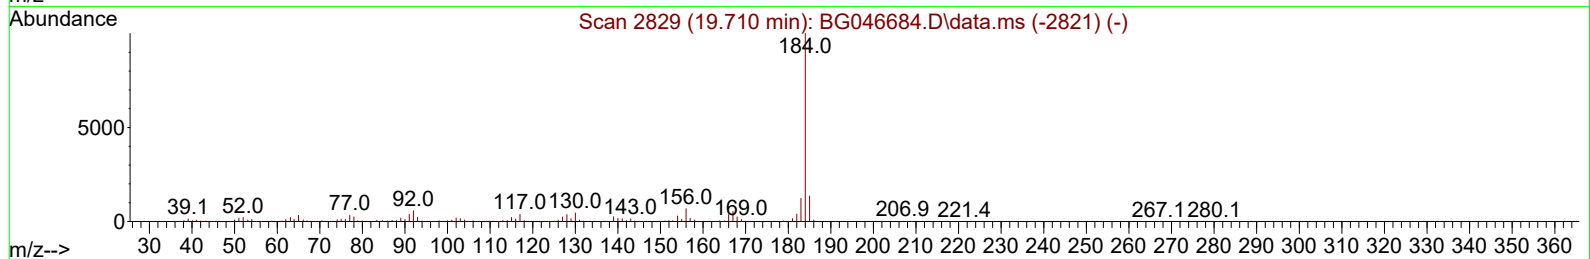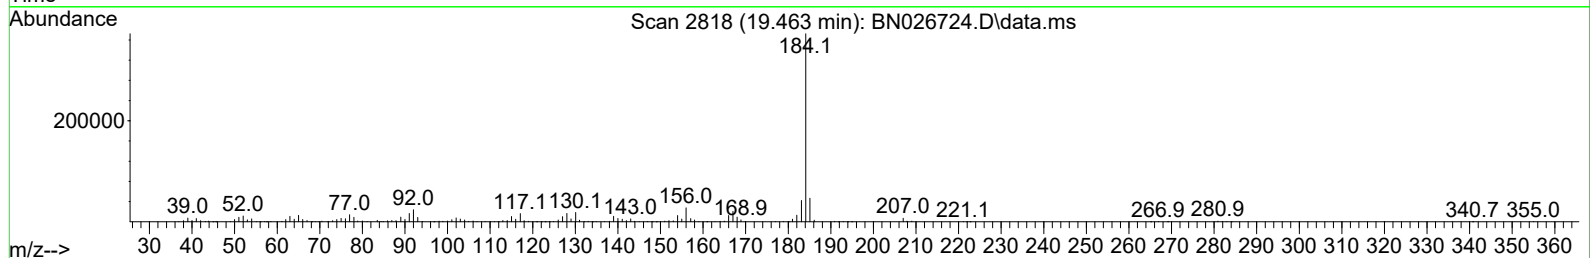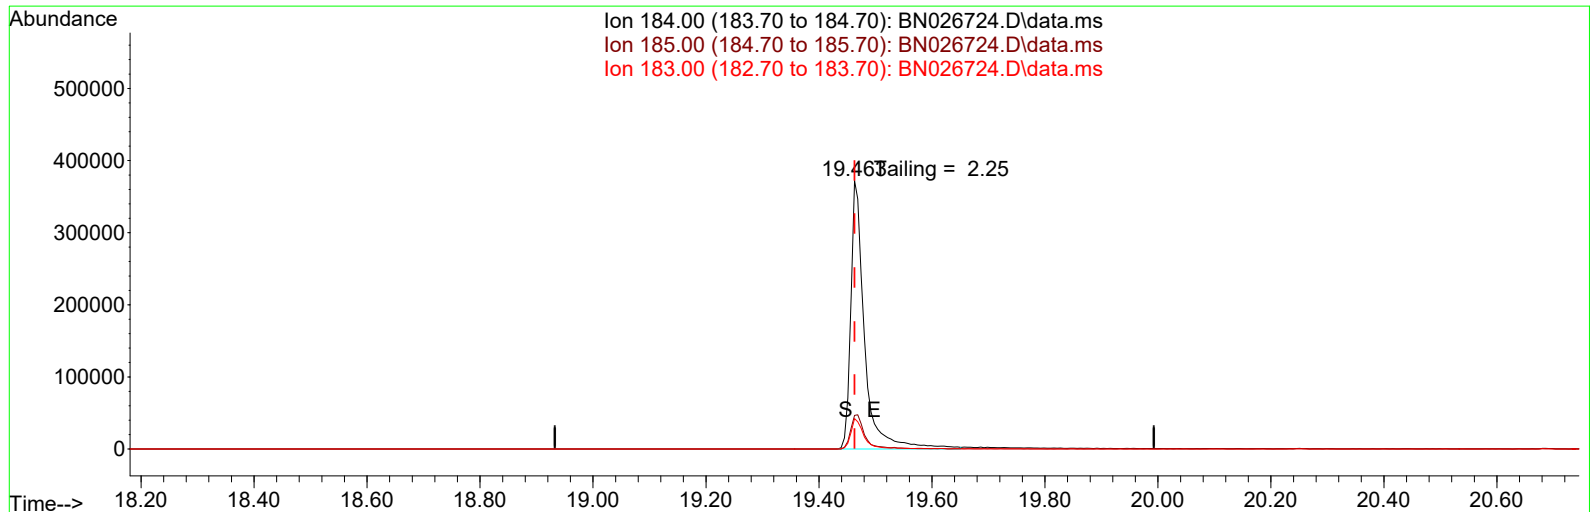

TIC: BN026724.D\data.ms

(77) Benzidine**19.463min (0.000) 374808.72 ng****response 635449**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.52
183.00	13.20	11.36
0.00	0.00	0.00