
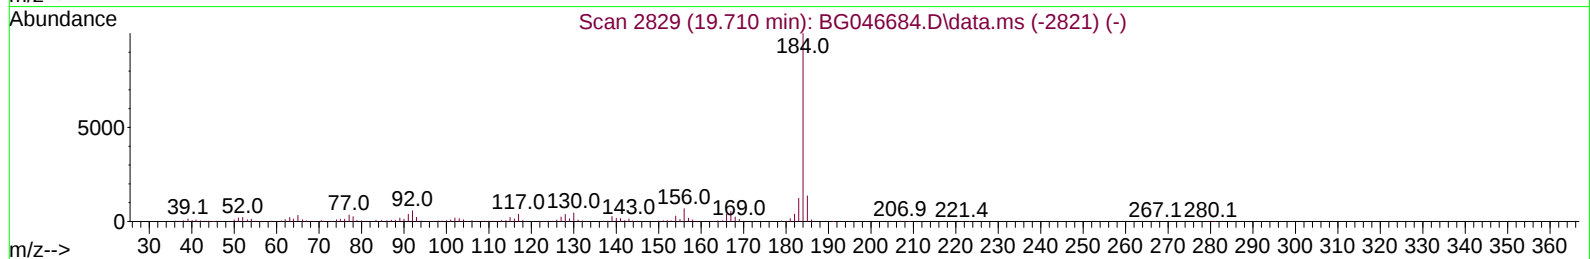
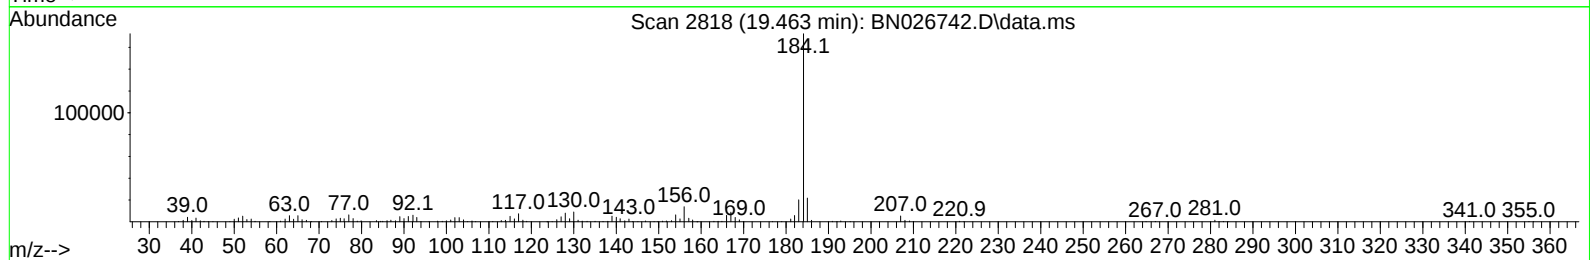


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026742.D
Acq On : 25 Jul 2023 11:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 05:31:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

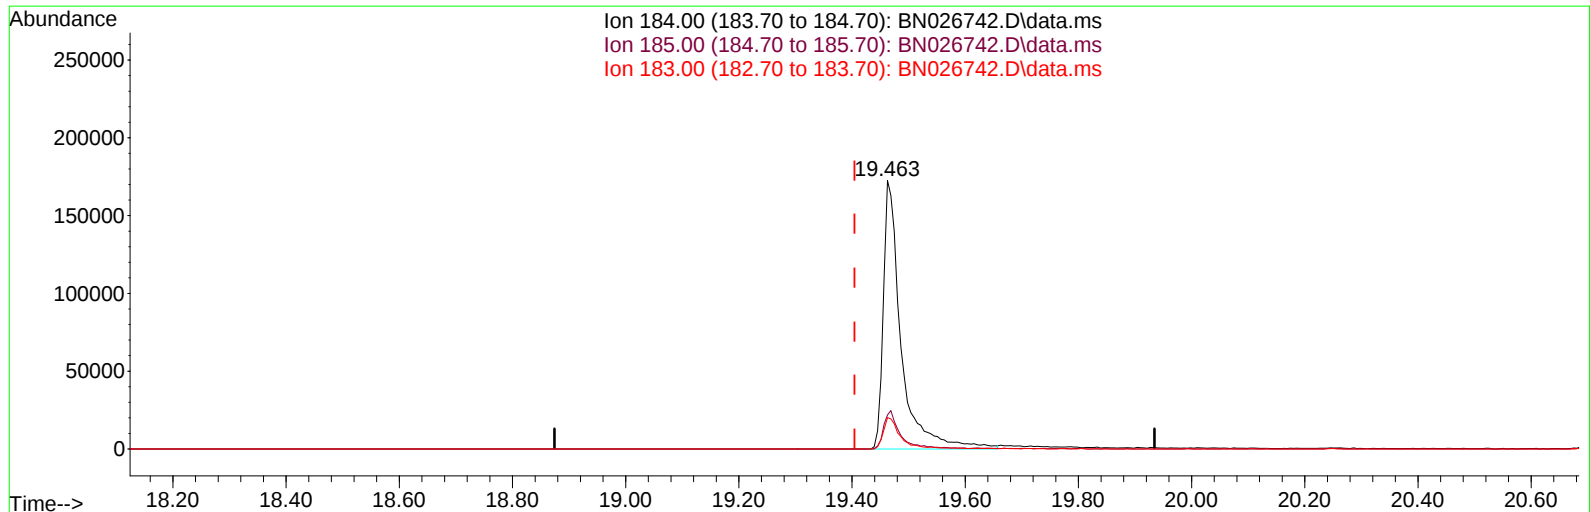

TIC: BN026742.D\data.ms

(77) Benzidine




19.463min (+ 0.059) 177210.04 ng

response 376917

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.67
183.00	13.20	11.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026742.D
Acq On : 25 Jul 2023 11:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 05:31:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

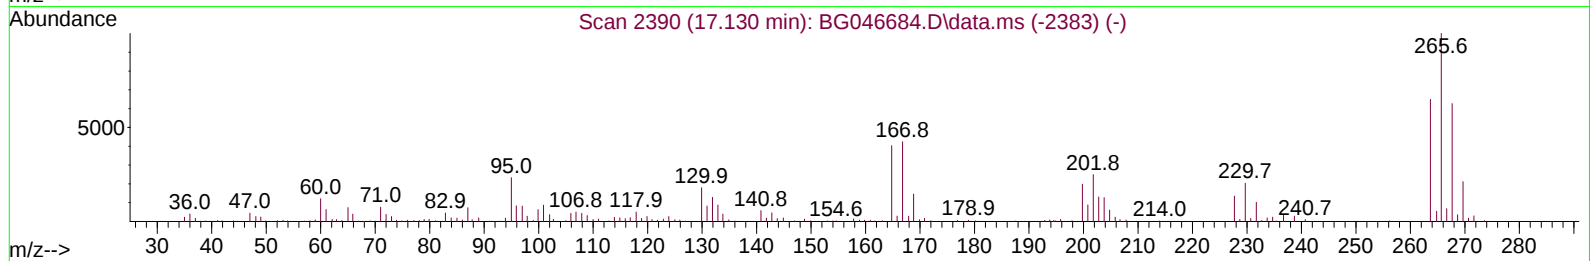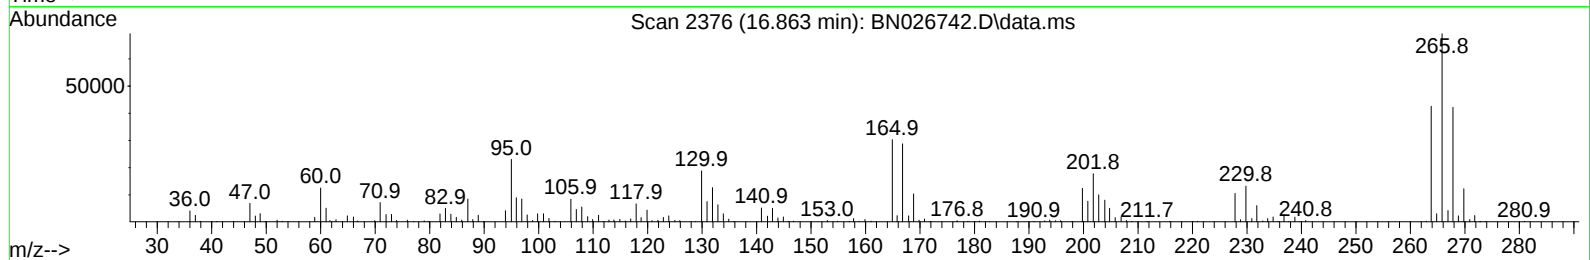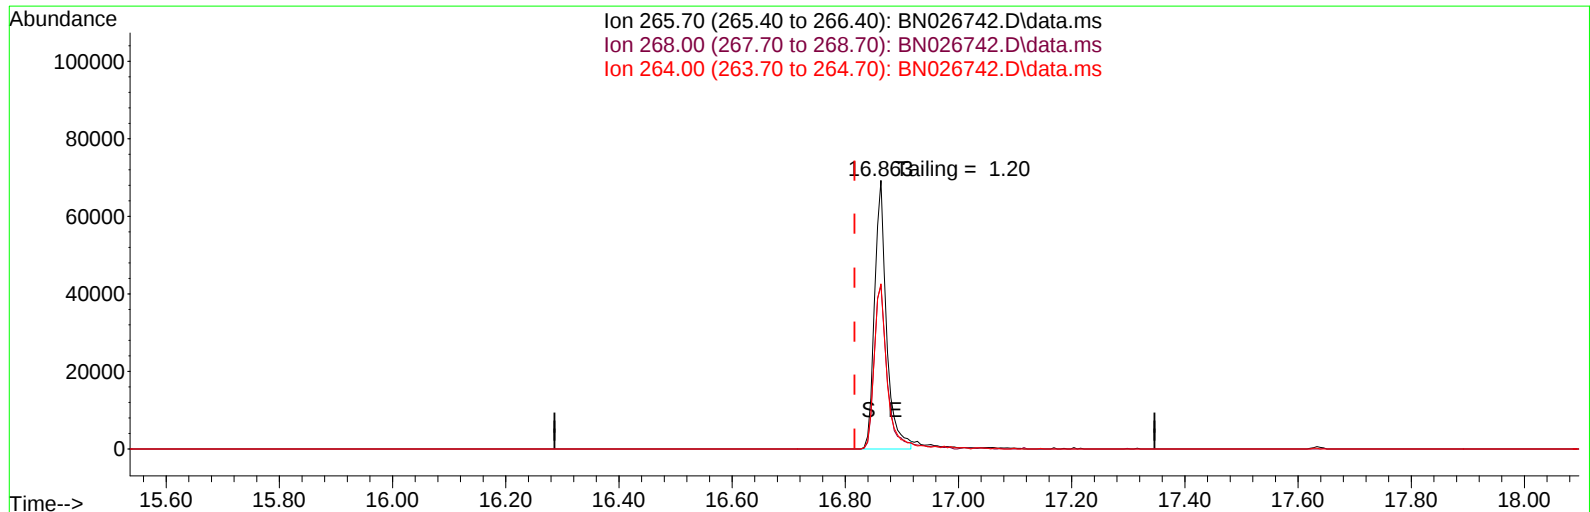

TIC: BN026742.D\data.ms

(70) Pentachlorophenol (C)**16.863min (+ 0.047) 12188.50 ng****response 106461**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.90
264.00	61.60	61.48
0.00	0.00	0.00