
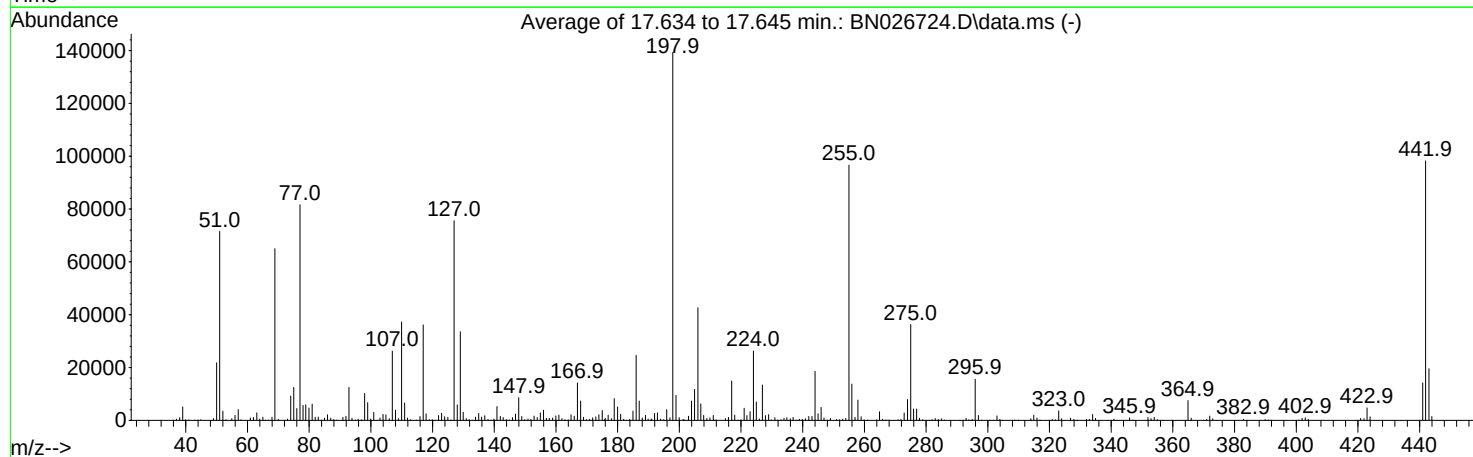


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026724.D
Acq On : 24 Jul 2023 22:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 24 23:51:48 2023

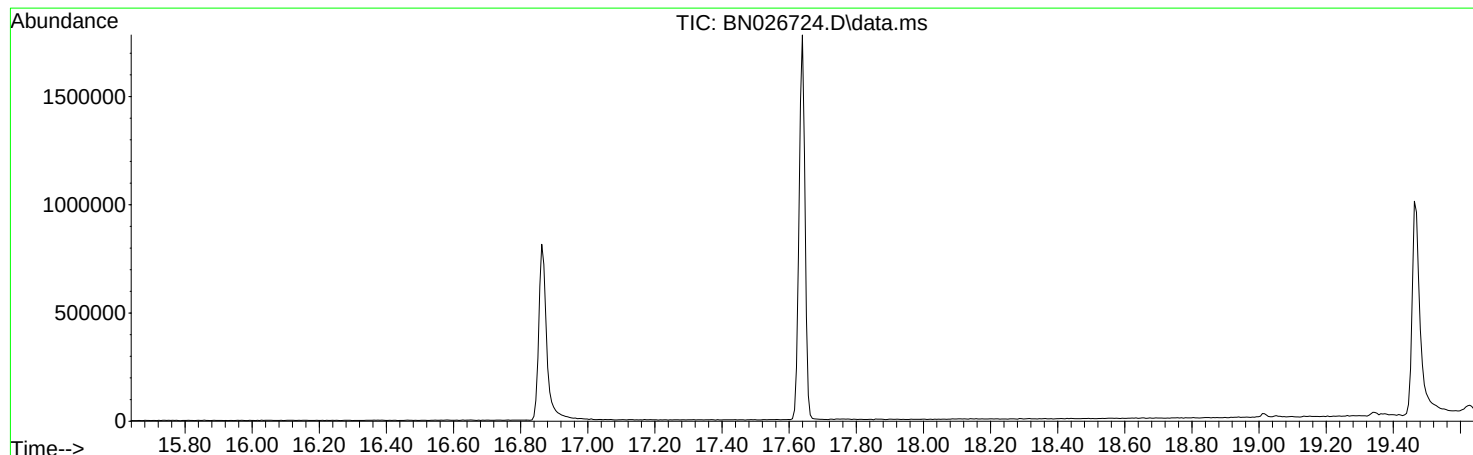

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	71528	PASS
68	69	0.00	2	1.9	1228	PASS
69	198	0.00	100	46.7	64981	PASS
70	69	0.00	2	0.6	379	PASS
127	198	10	80	54.3	75616	PASS
197	198	0.00	2	0.7	946	PASS
198	198	100	100	100.0	139251	PASS
199	198	5	9	6.8	9466	PASS
275	198	10	60	26.1	36291	PASS
365	198	1	100	5.4	7488	PASS
441	198	0.01	100	10.2	14203	PASS
442	442	50	100	100.0	98229	PASS
443	442	15	24	19.9	19589	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/24/2023	BNA_N	<u>BN026724.D</u>
Compound Name	Response	Retention Time
DDT	132307	20.686
DDD	184848	20.251
DDE	3096	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
187944	320251	58.69

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
 Data File : BN026724.D
 Acq On : 24 Jul 2023 22:03
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 25 04:18:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 04:17:57 2023
 Response via : Initial Calibration

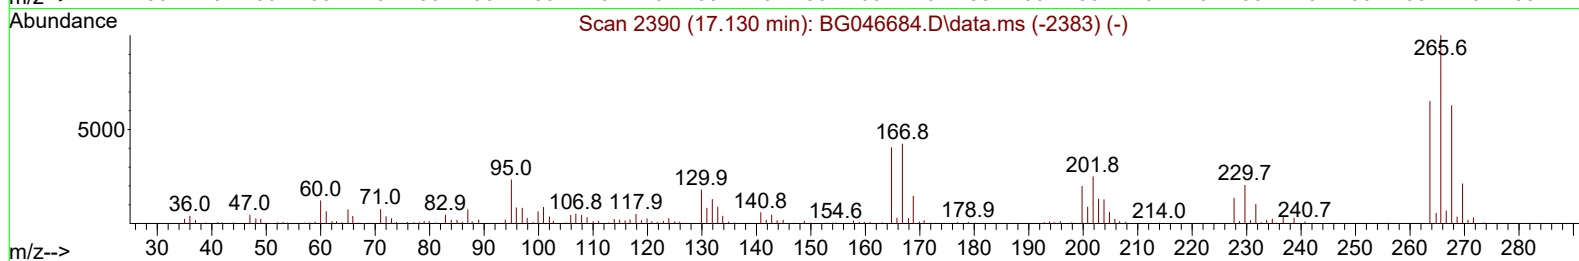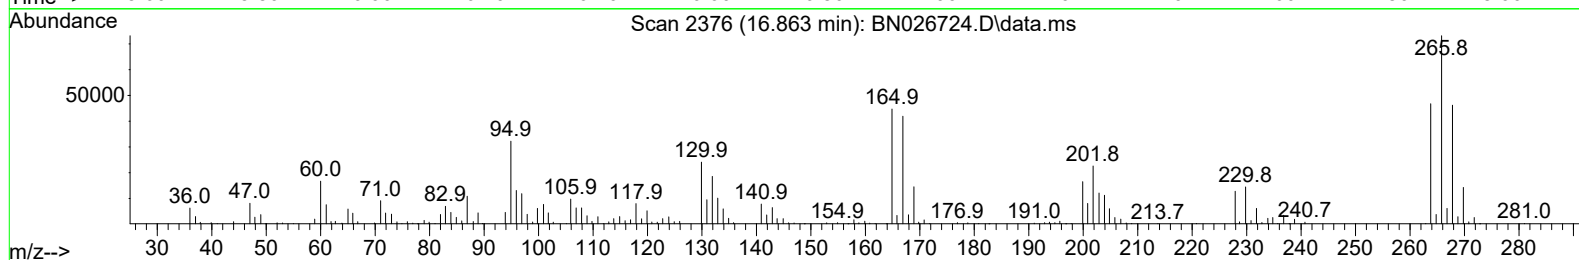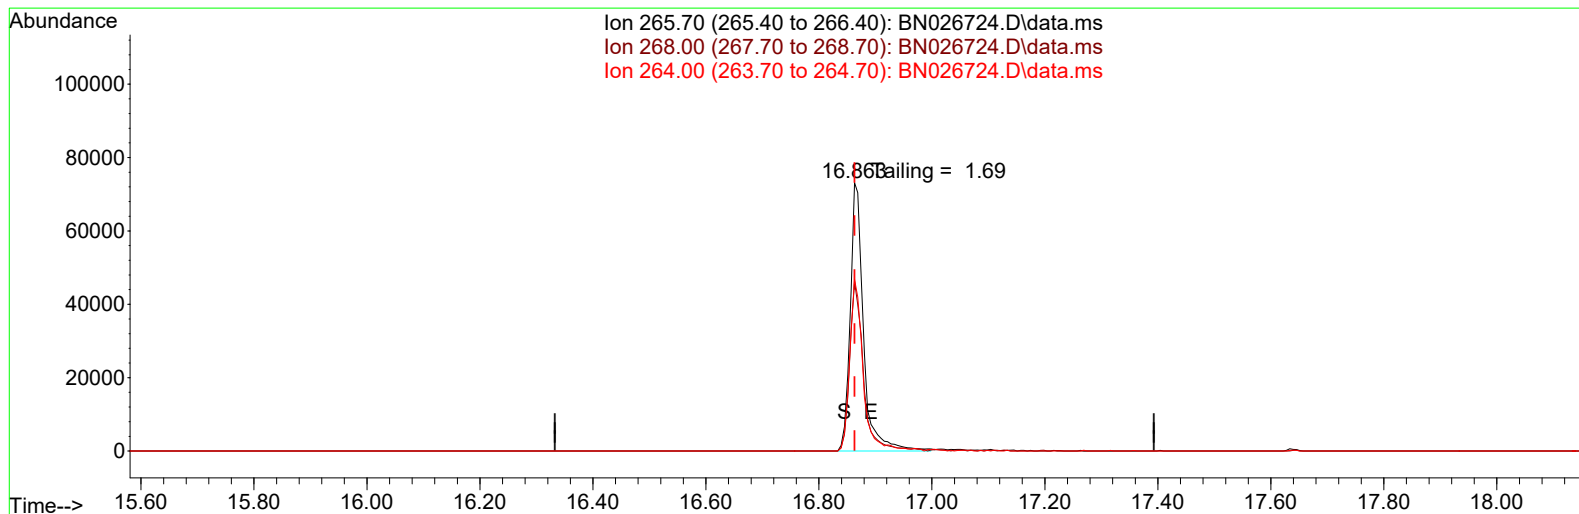

TIC: BN026724.D\data.ms

(70) Pentachlorophenol (C)

16.863min (0.000) 13247.60 ng




response 120598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026724.D
Acq On : 24 Jul 2023 22:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 25 04:18:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

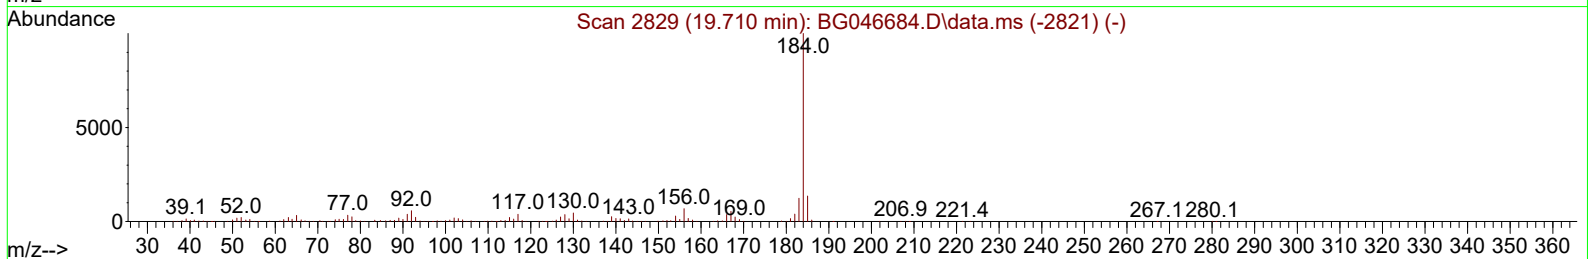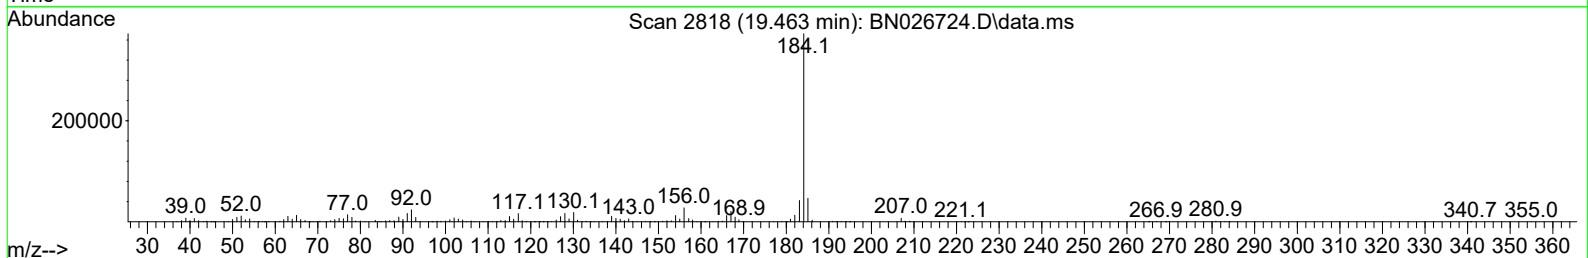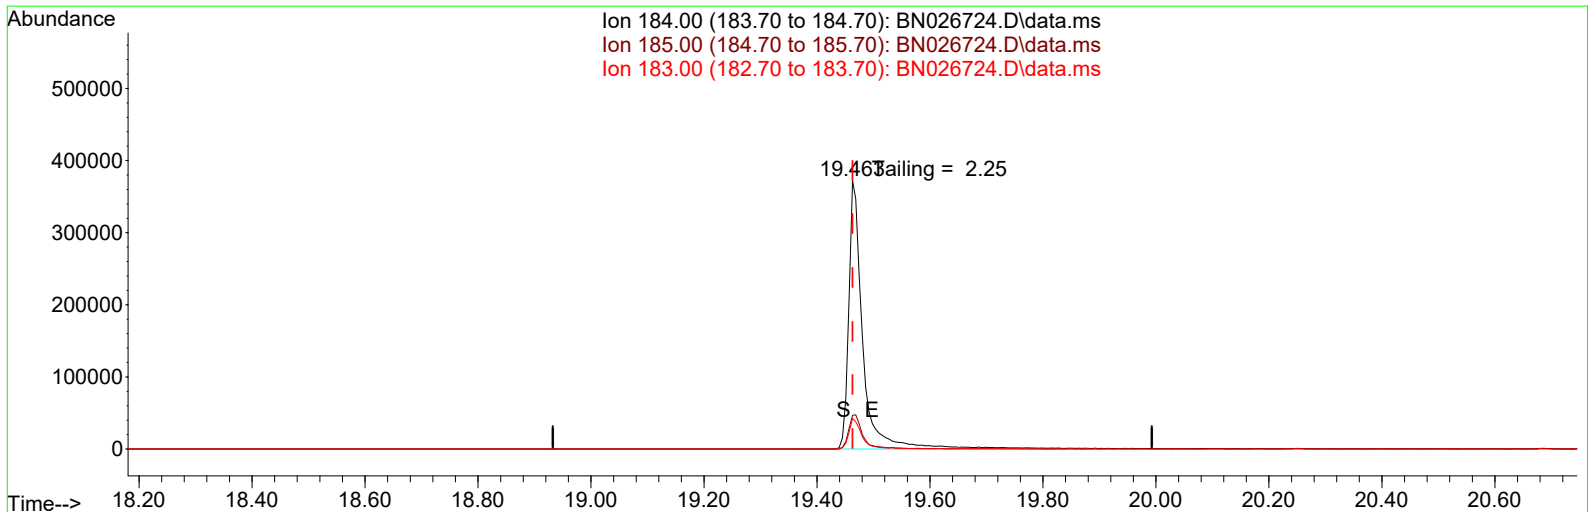

TIC: BN026724.D\data.ms

(77) Benzidine

19.463min (0.000) 374808.72 ng

response 635449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.52
183.00	13.20	11.36
0.00	0.00	0.00