
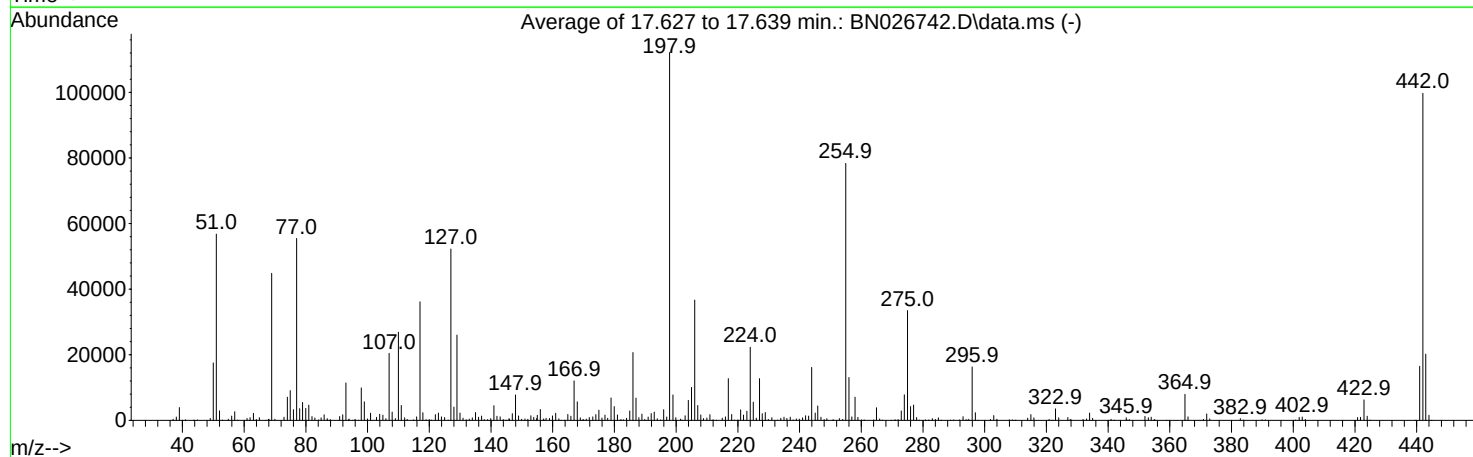


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026742.D
Acq On : 25 Jul 2023 11:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 24 23:51:48 2023

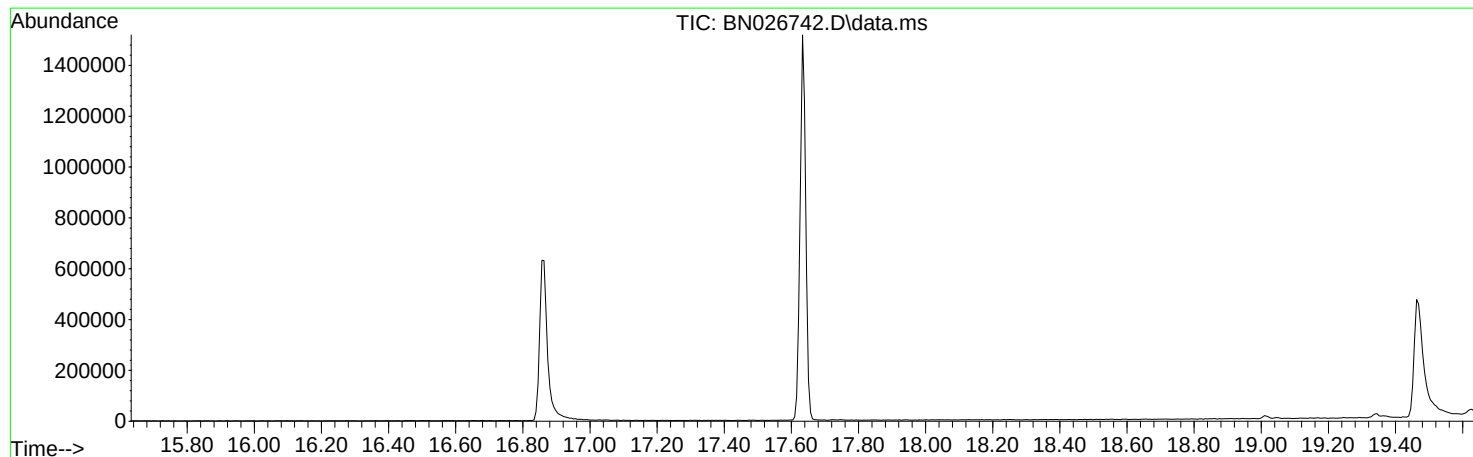




Spectrum Information: Average of 17.627 to 17.639 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	50.7	56813	PASS
68	69	0.00	2	0.8	341	PASS
69	198	0.00	100	40.0	44856	PASS
70	69	0.00	2	0.8	351	PASS
127	198	10	80	46.6	52229	PASS
197	198	0.00	2	0.9	1009	PASS
198	198	100	100	100.0	112160	PASS
199	198	5	9	6.9	7752	PASS
275	198	10	60	29.8	33459	PASS
365	198	1	100	7.1	7959	PASS
441	198	0.01	100	14.7	16498	PASS
442	442	50	100	100.0	99720	PASS
443	442	15	24	20.2	20177	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
Data File : BN026742.D
Acq On : 25 Jul 2023 11:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 26 05:31:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 04:17:57 2023
Response via : Initial Calibration

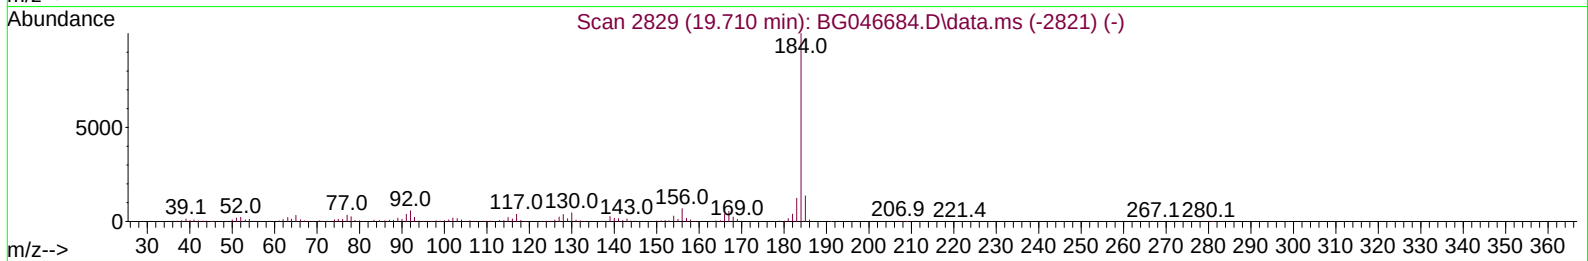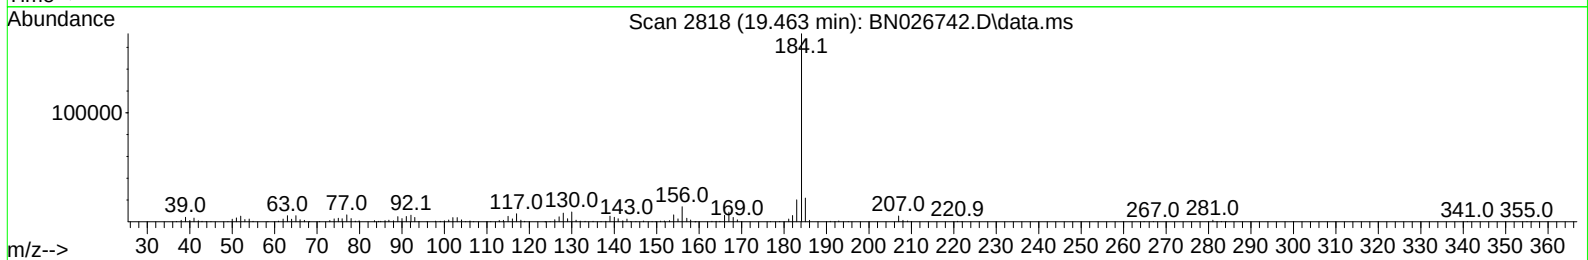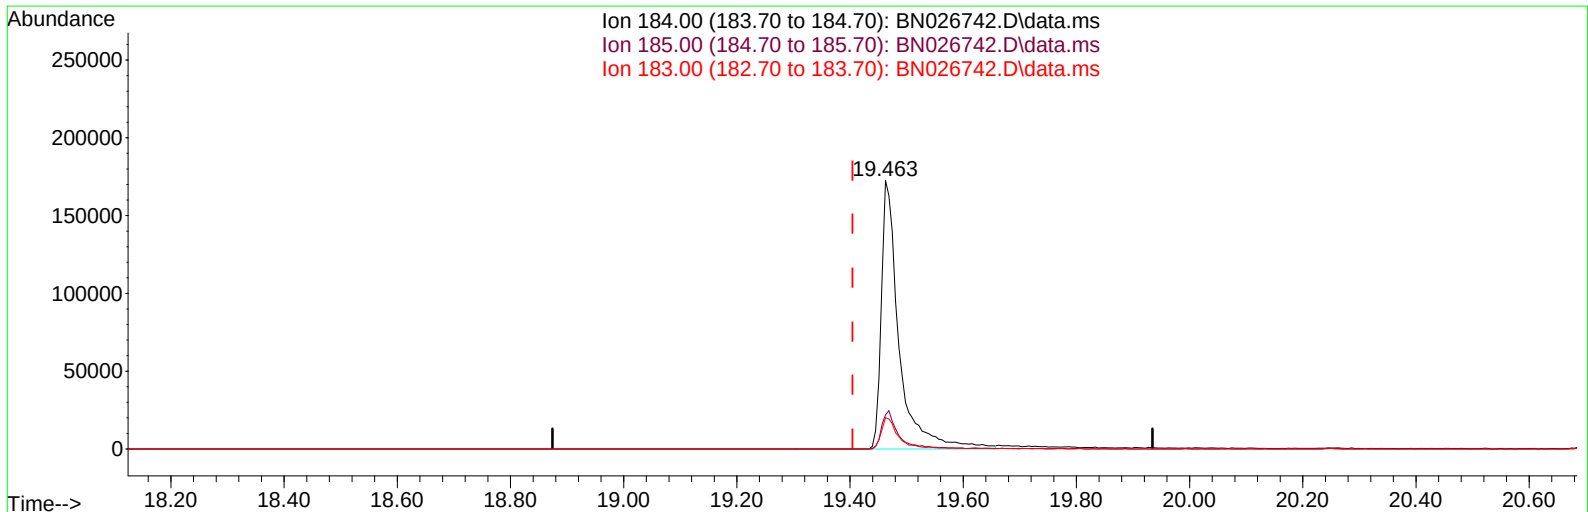

TIC: BN026742.D\data.ms

(77) Benzidine

19.463min (+ 0.059) 177210.04 ng




response 376917

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.67
183.00	13.20	11.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072423\
 Data File : BN026742.D
 Acq On : 25 Jul 2023 11:00
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 26 05:31:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 04:17:57 2023
 Response via : Initial Calibration

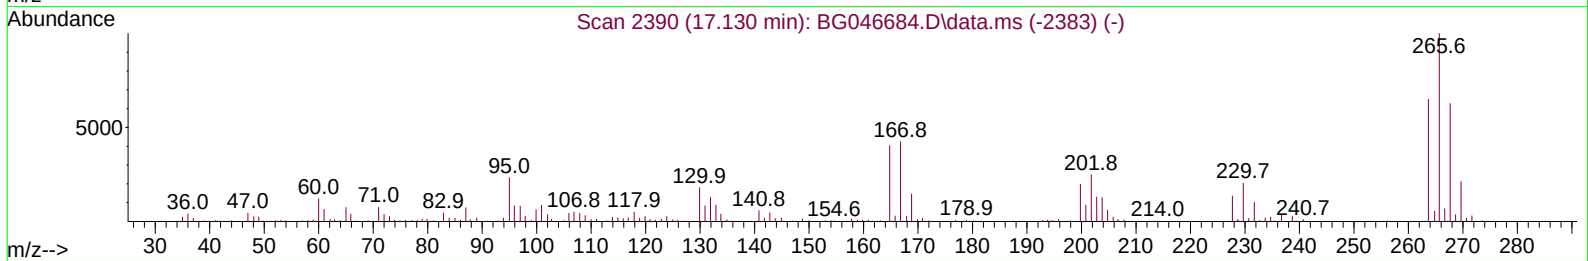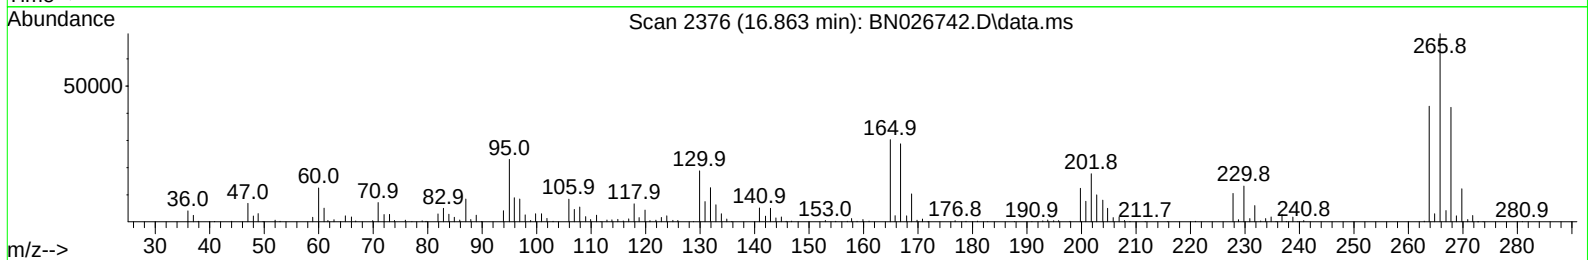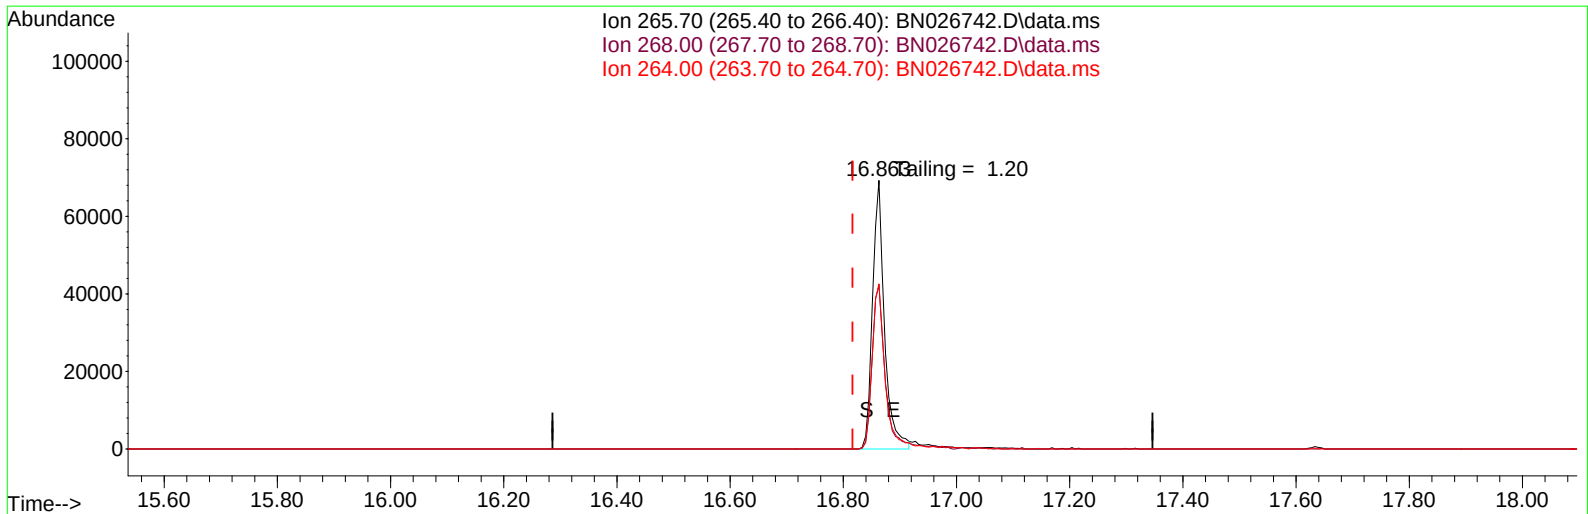

TIC: BN026742.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.047) 12188.50 ng

response 106461

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.90
264.00	61.60	61.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2023	BNA_N	<u>BN026742.D</u>
Compound Name	Response	Retention Time
DDT	149430	20.692
DDD	119956	20.251
DDE	4352	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
124308	273738	45.41

Instrument :
BNA_N
ClientSampleId :
DFTPP