


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072518\
 Data File : BN002140.D
 Acq On : 25 Jul 2018 17:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN072518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 25 20:08:02 2018

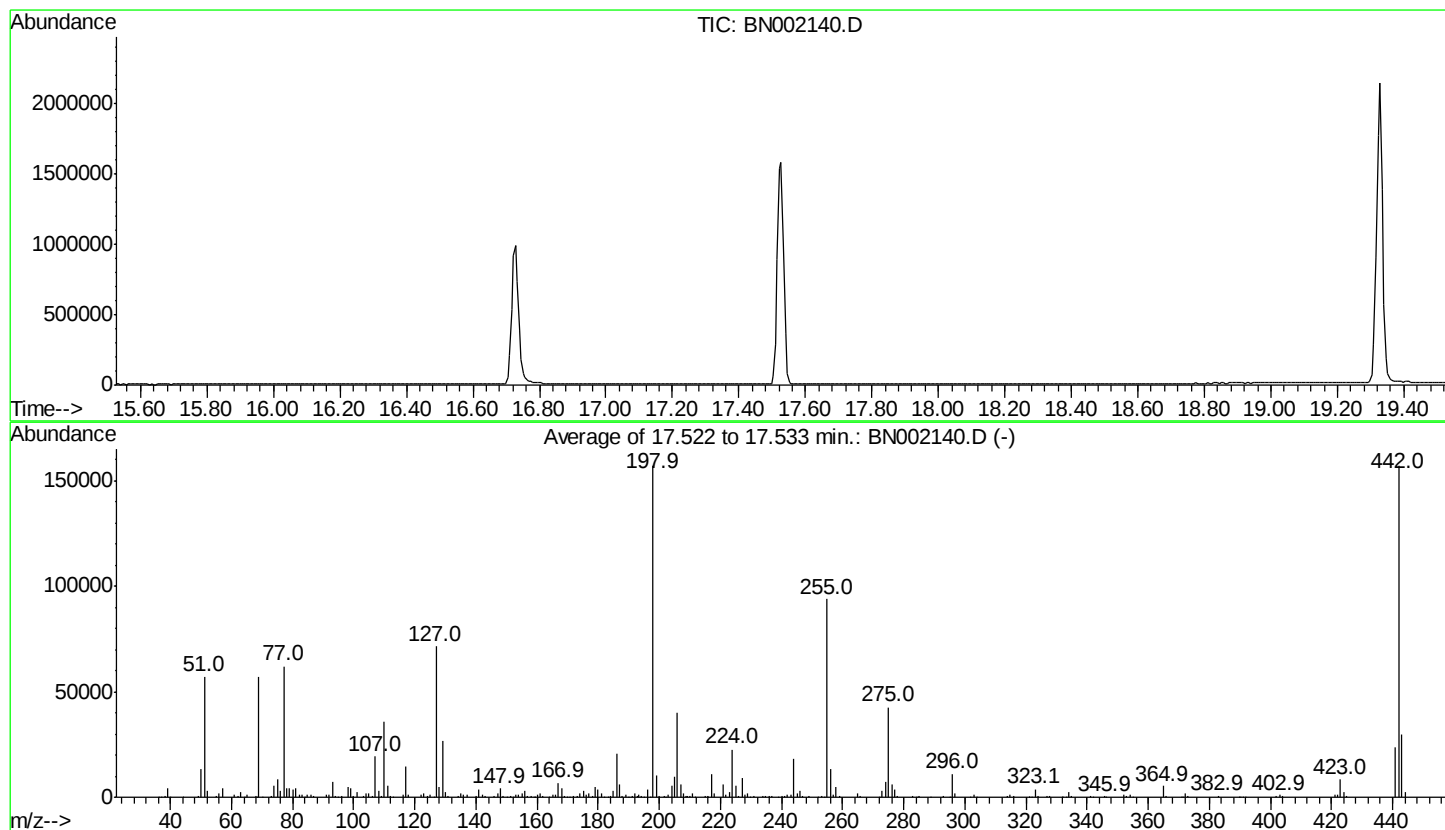

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	57253	PASS
68	69	0.00	2	1.6	901	PASS
69	198	0.00	100	36.3	57024	PASS
70	69	0.00	2	0.5	277	PASS
127	198	10	80	45.5	71469	PASS
197	198	0.00	2	0.2	238	PASS
198	198	100	100	100.0	157189	PASS
199	198	5	9	6.8	10636	PASS
275	198	10	60	27.2	42680	PASS
365	198	1	100	3.4	5420	PASS
441	198	0.01	100	15.1	23792	PASS
442	198	50	100	100.0	157184	PASS
443	442	15	24	18.8	29554	PASS