


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072518\
 Data File : BN002159.D
 Acq On : 26 Jul 2018 04:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN072518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 25 20:08:02 2018

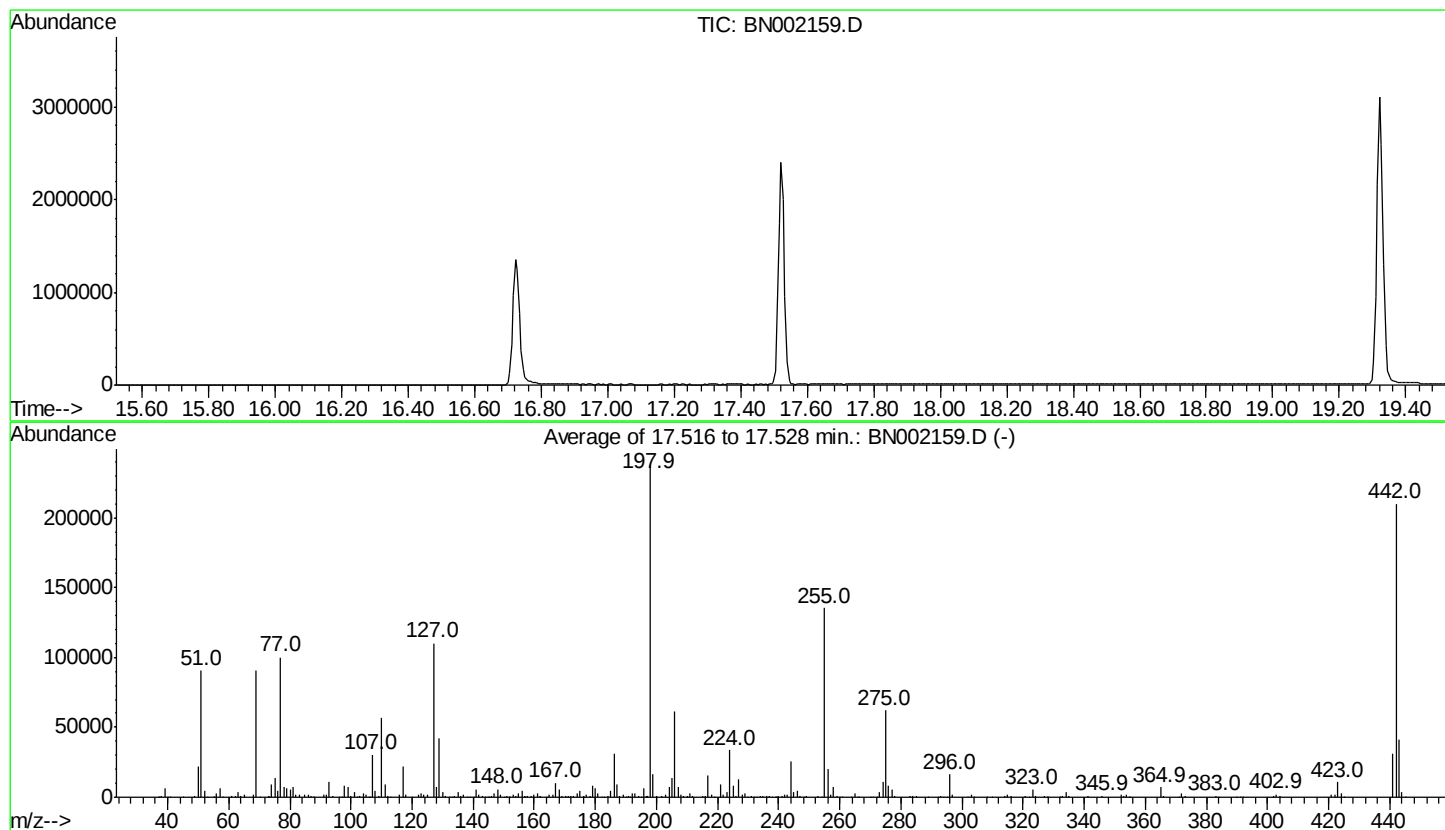

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	90533	PASS
68	69	0.00	2	1.8	1629	PASS
69	198	0.00	100	38.1	90424	PASS
70	69	0.00	2	0.5	436	PASS
127	198	10	80	46.4	110093	PASS
197	198	0.00	2	0.4	849	PASS
198	198	100	100	100.0	237184	PASS
199	198	5	9	6.8	16089	PASS
275	198	10	60	26.1	61858	PASS
365	198	1	100	3.0	7135	PASS
441	198	0.01	100	13.2	31349	PASS
442	198	50	100	88.6	210133	PASS
443	442	15	24	19.4	40834	PASS