
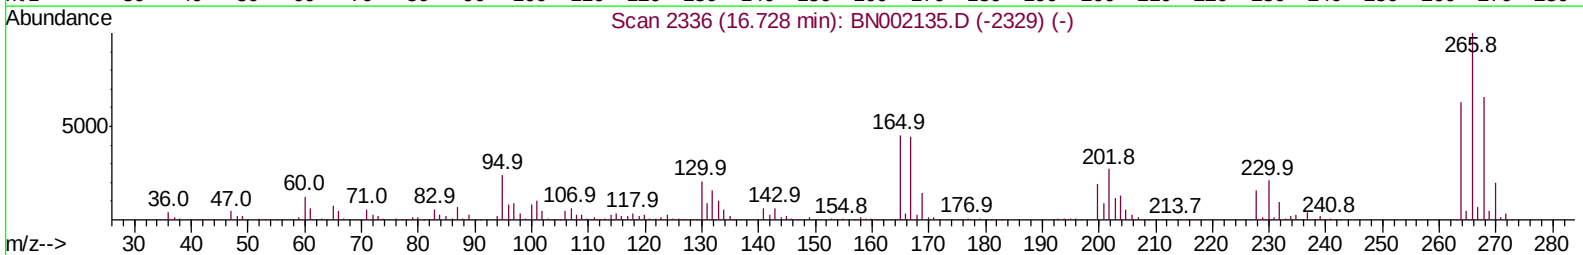
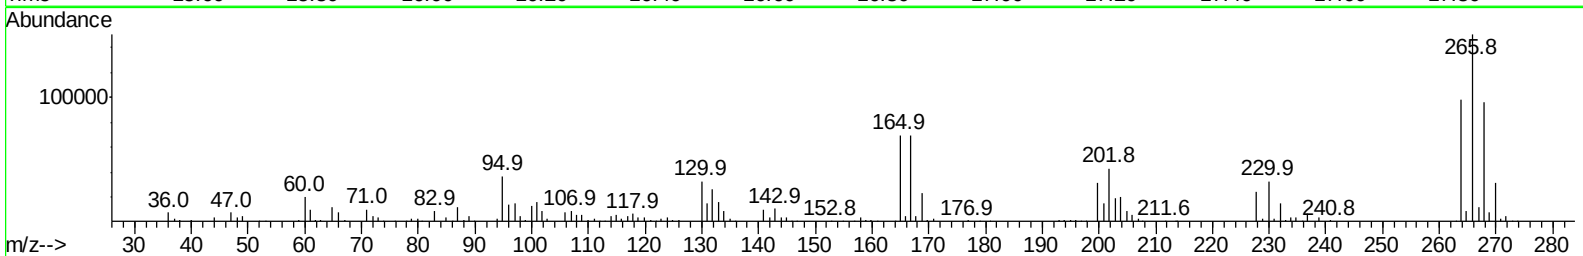


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072618\
Data File : BN002166.D
Acq On : 26 Jul 2018 09:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 09:19:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN072518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 26 18:27:25 2018
Response via : Initial Calibration

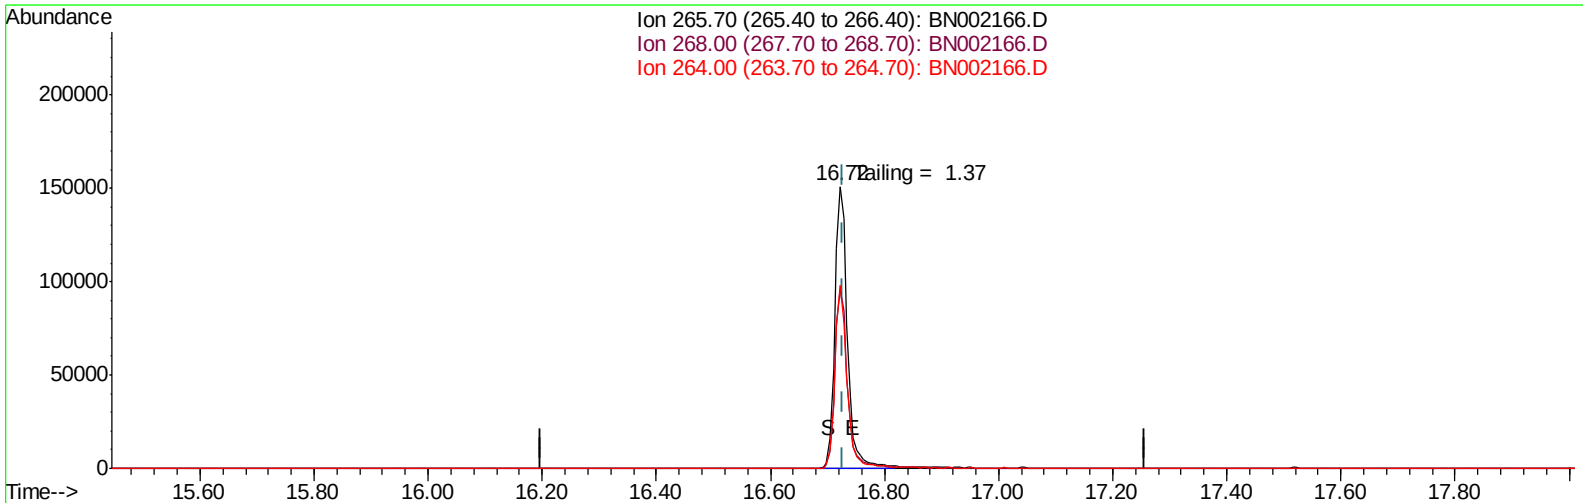

TIC: BN002166.D

(69) Pentachlorophenol (C)




16.722min (-0.006) 19475.09ng

response 229526

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.73
264.00	62.00	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072618\
 Data File : BN002166.D
 Acq On : 26 Jul 2018 09:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 09:19:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN072518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 26 18:27:25 2018
 Response via : Initial Calibration

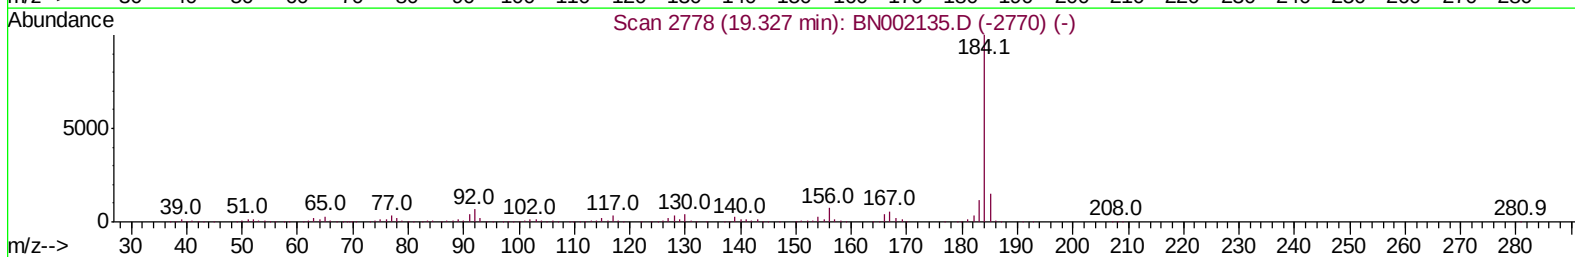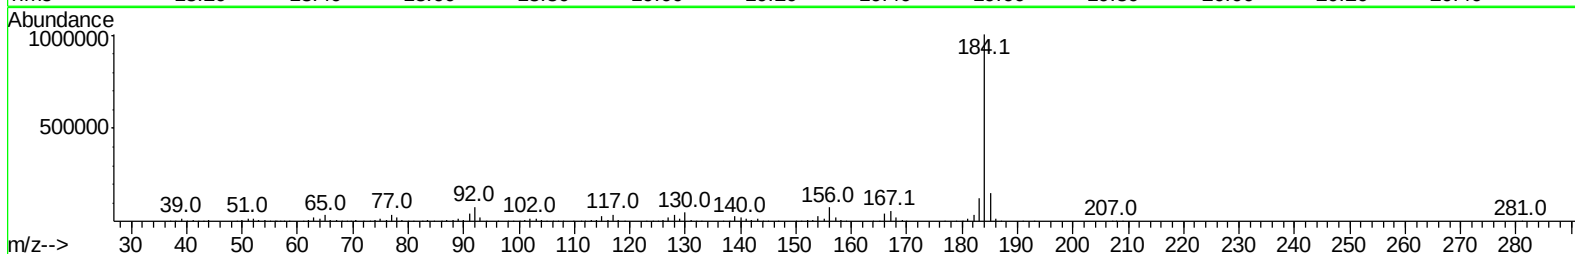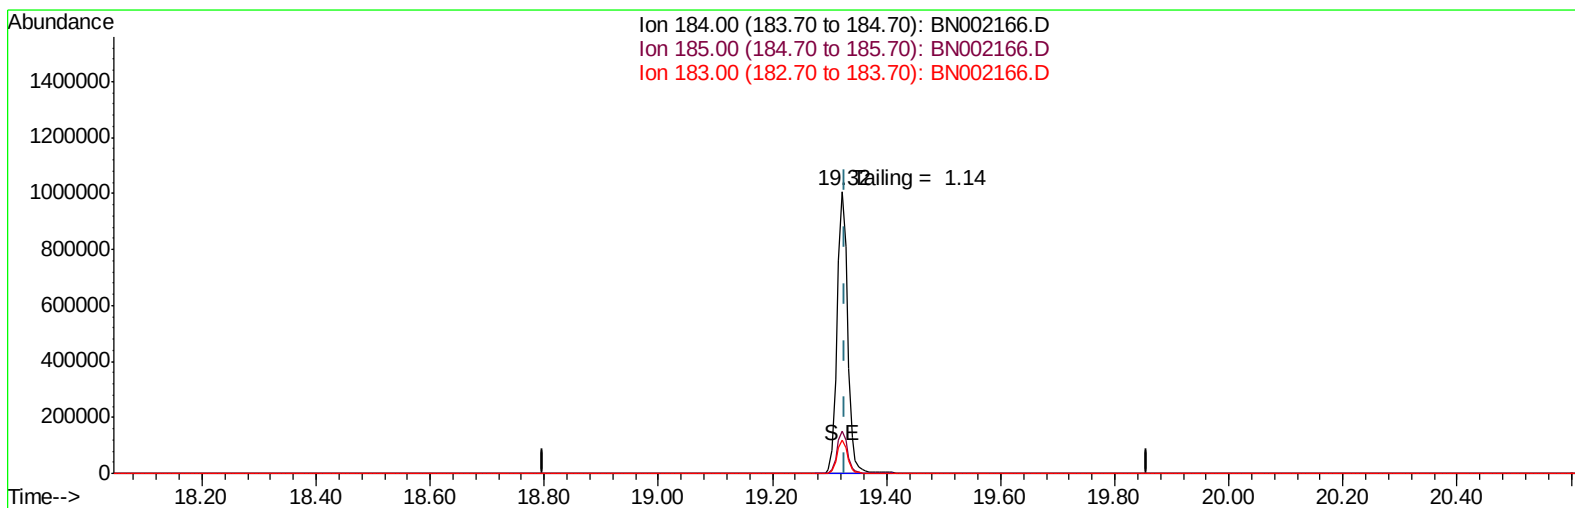

TIC: BN002166.D

(76) Benzidine

19.322min (-0.006) 0.00ng

response 1290329

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.97
183.00	13.30	12.04
0.00	0.00	0.00