


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072618\
 Data File : BN002166.D
 Acq On : 26 Jul 2018 09:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN072518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 26 18:27:25 2018

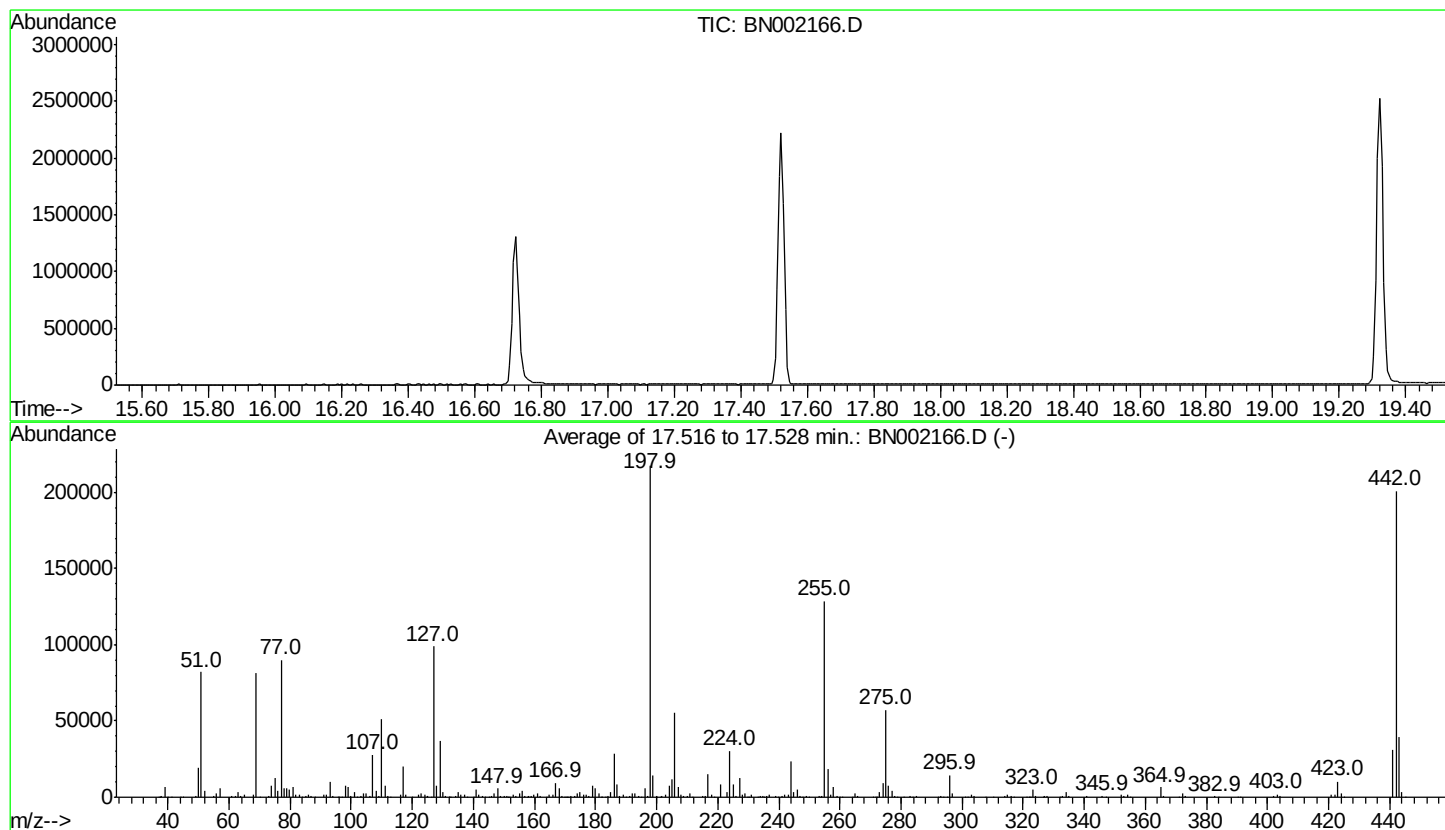

Spectrum Information: Average of 17.516 to 17.528 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	82050	PASS
68	69	0.00	2	1.7	1412	PASS
69	198	0.00	100	37.4	81405	PASS
70	69	0.00	2	0.5	380	PASS
127	198	10	80	45.5	99005	PASS
197	198	0.00	2	0.4	831	PASS
198	198	100	100	100.0	217472	PASS
199	198	5	9	6.6	14389	PASS
275	198	10	60	26.3	57298	PASS
365	198	1	100	3.1	6640	PASS
441	198	0.01	100	14.3	31178	PASS
442	198	50	100	92.3	200768	PASS
443	442	15	24	19.5	39096	PASS