




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072623\
 Data File : BN026758.D
 Acq On : 26 Jul 2023 16:09
 Operator : MA/JU
 Sample : PB154053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Quant Time: Jul 26 20:19:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/28/2023
 Supervised By :mohammad ahmed 07/28/2023

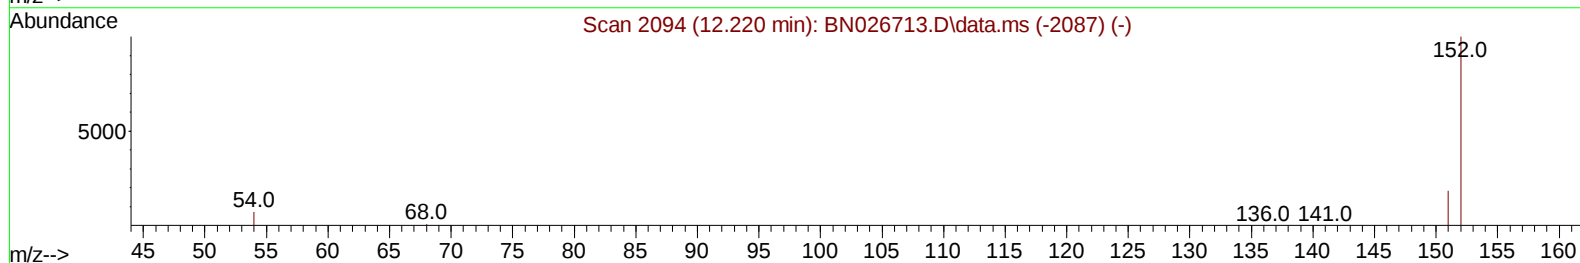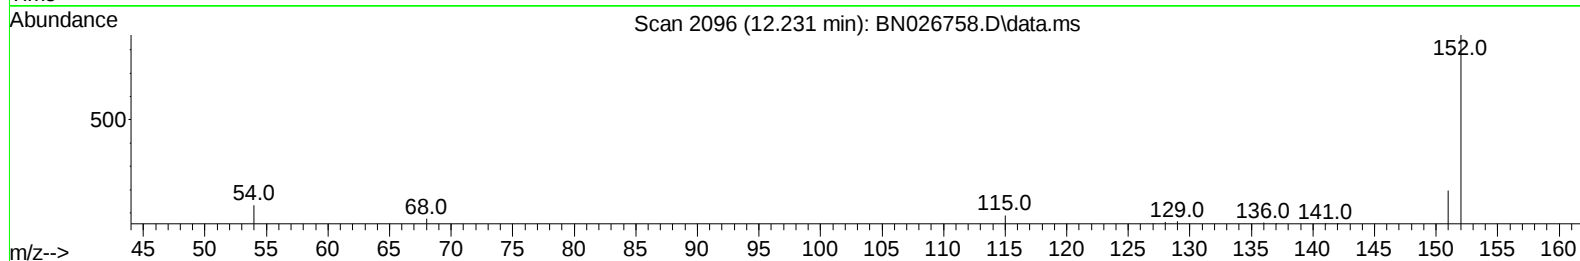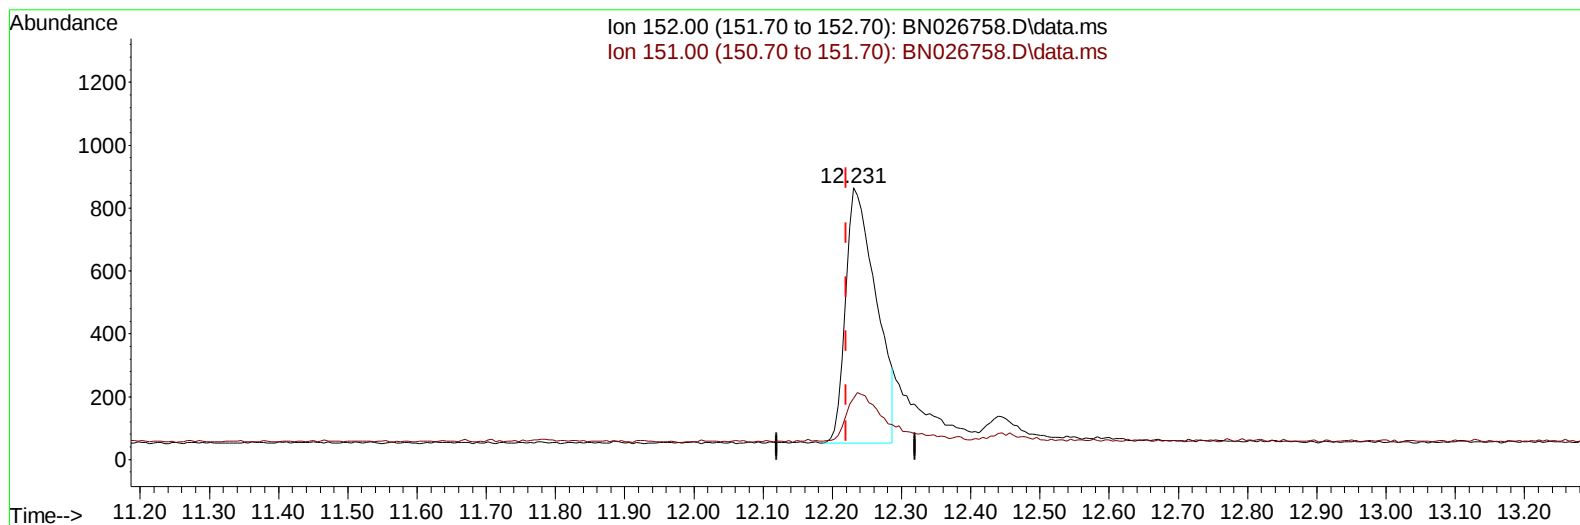

TIC: BN026758.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.231min (+ 0.011) 0.36 ng/u1

response 2454

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	19.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072623\
 Data File : BN026758.D
 Acq On : 26 Jul 2023 16:09
 Operator : MA/JU
 Sample : PB154053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Quant Time: Jul 26 20:19:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/28/2023
 Supervised By :mohammad ahmed 07/28/2023

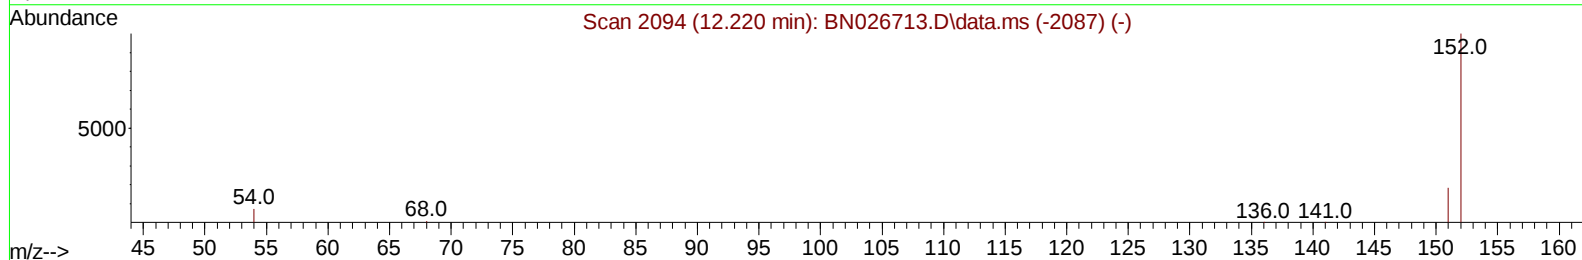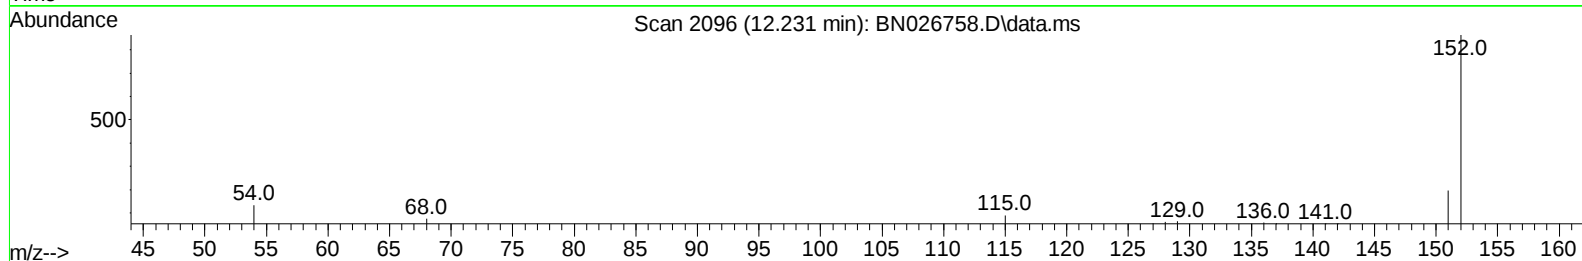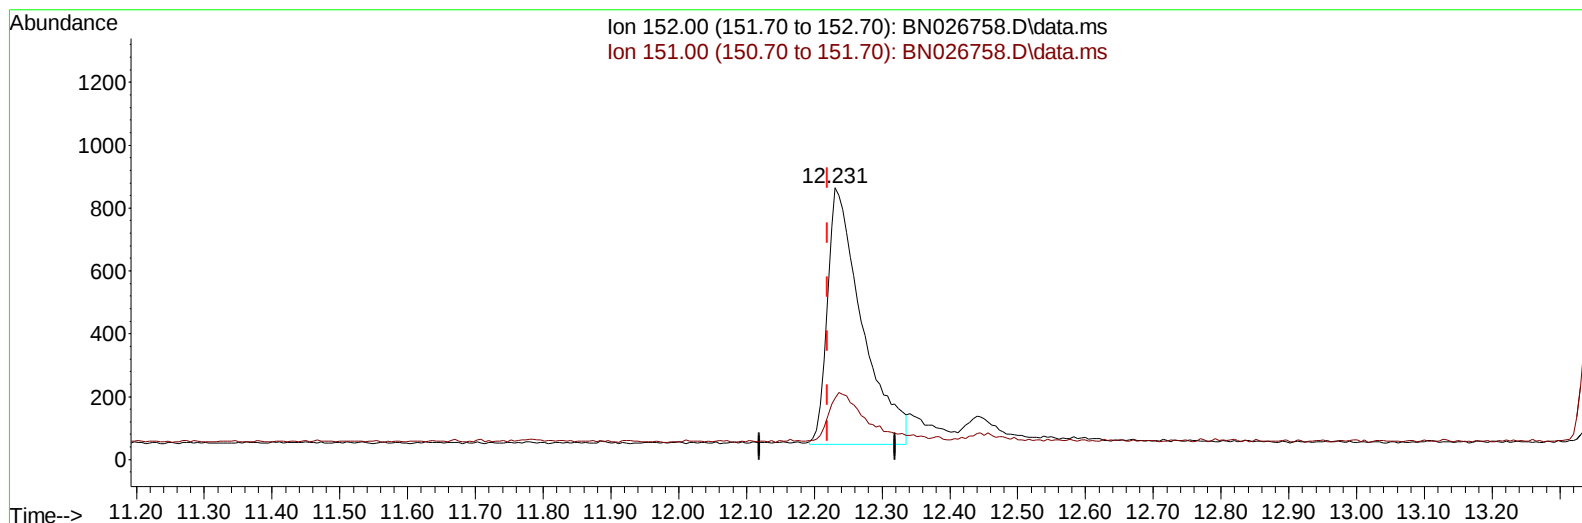

TIC: BN026758.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.231min (+ 0.011) 0.42 ng/ul m

response 2903

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	16.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072623\
 Data File : BN026758.D
 Acq On : 26 Jul 2023 16:09
 Operator : MA/JU
 Sample : PB154053BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK053

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/28/2023
 Supervised By :mohammad ahmed 07/28/2023

Quant Time: Jul 26 20:19:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 24 00:39:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.823	152	1772	0.400	ng/ul	0.00
4) Naphthalene-d8	10.614	136	5060	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.458	164	3582	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	8564	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.428	240	8372	0.400	ng/ul	# 0.01
23) Perylene-d12	23.784	264	12779	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	16593	7.110	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.231	152	2903m	0.422	ng/ul	0.01
18) Fluoranthene-d10	19.246	212	9481	0.327	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072623\
Data File : BN026758.D
Acq On : 26 Jul 2023 16:09
Operator : MA/JU
Sample : PB154053BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK053

Manual IntegrationsAPPROVED

Quant Time: Jul 26 20:19:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 24 00:39:11 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/28/2023
Supervised By :mohammad ahmed 07/28/2023

