
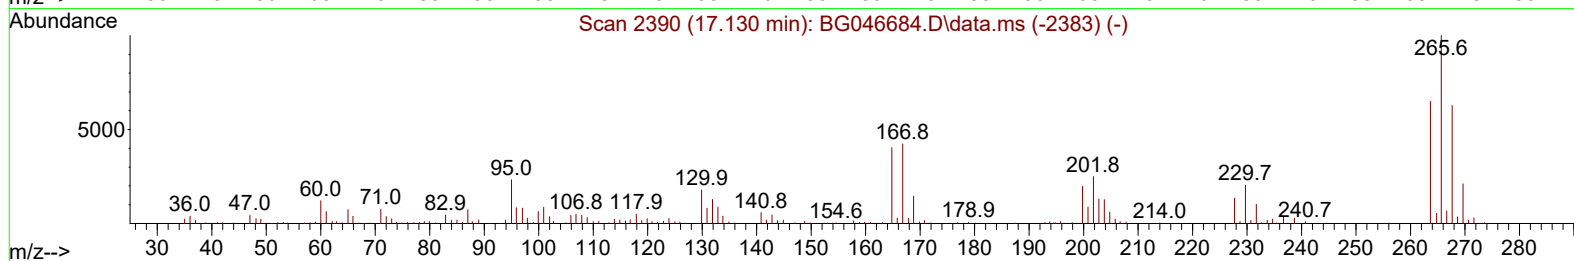
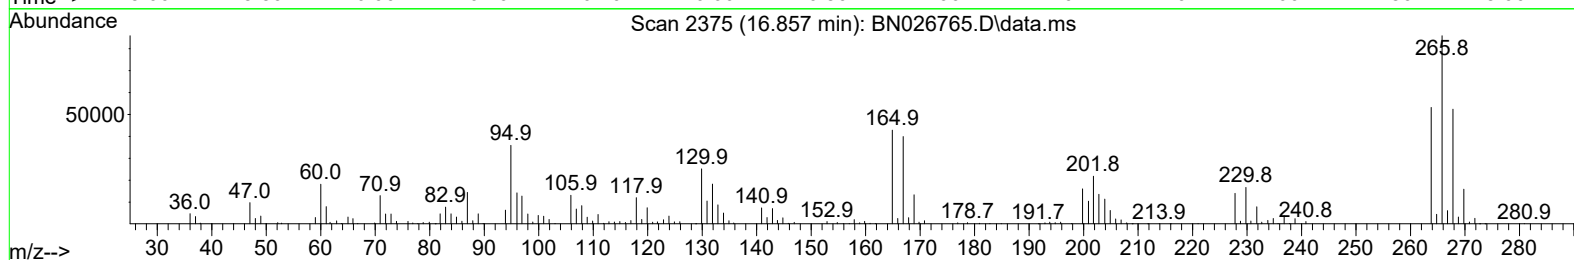


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072723\
Data File : BN026765.D
Acq On : 27 Jul 2023 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:59:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 04:59:07 2023
Response via : Initial Calibration

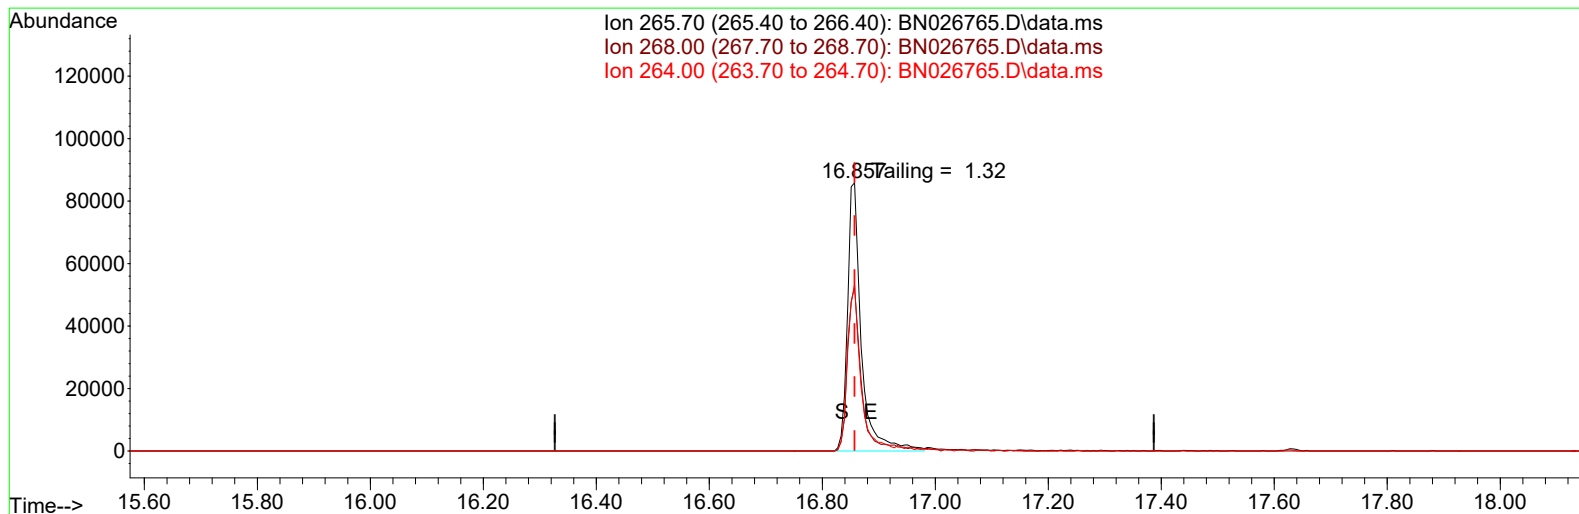

TIC: BN026765.D\data.ms

(70) Pentachlorophenol (C)




16.857min (0.000) 14480.09 ng

response 146136

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.98
264.00	61.60	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072723\
Data File : BN026765.D
Acq On : 27 Jul 2023 13:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:59:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 04:59:07 2023
Response via : Initial Calibration

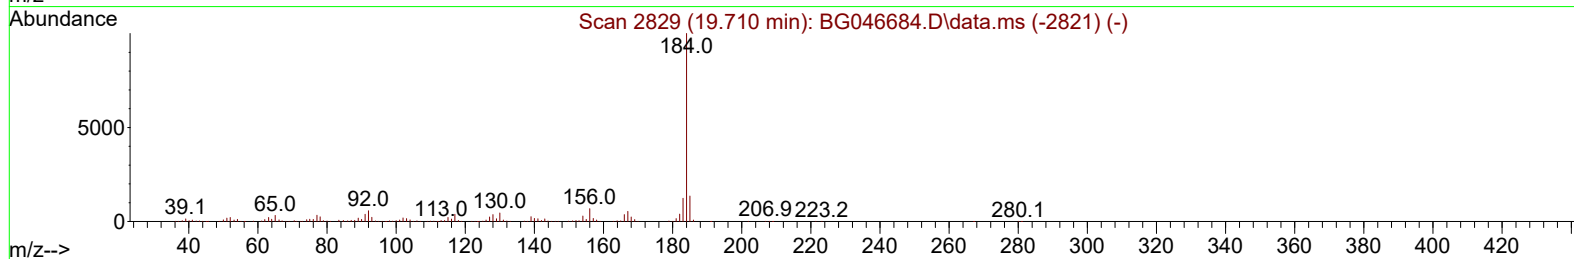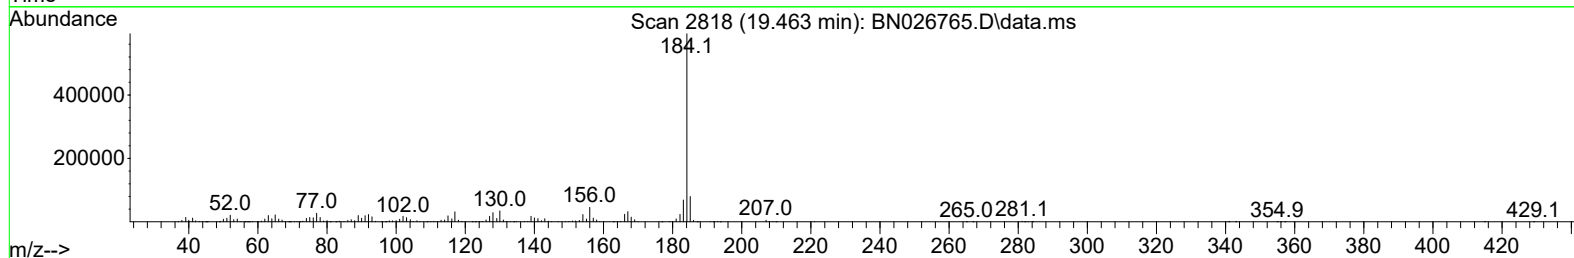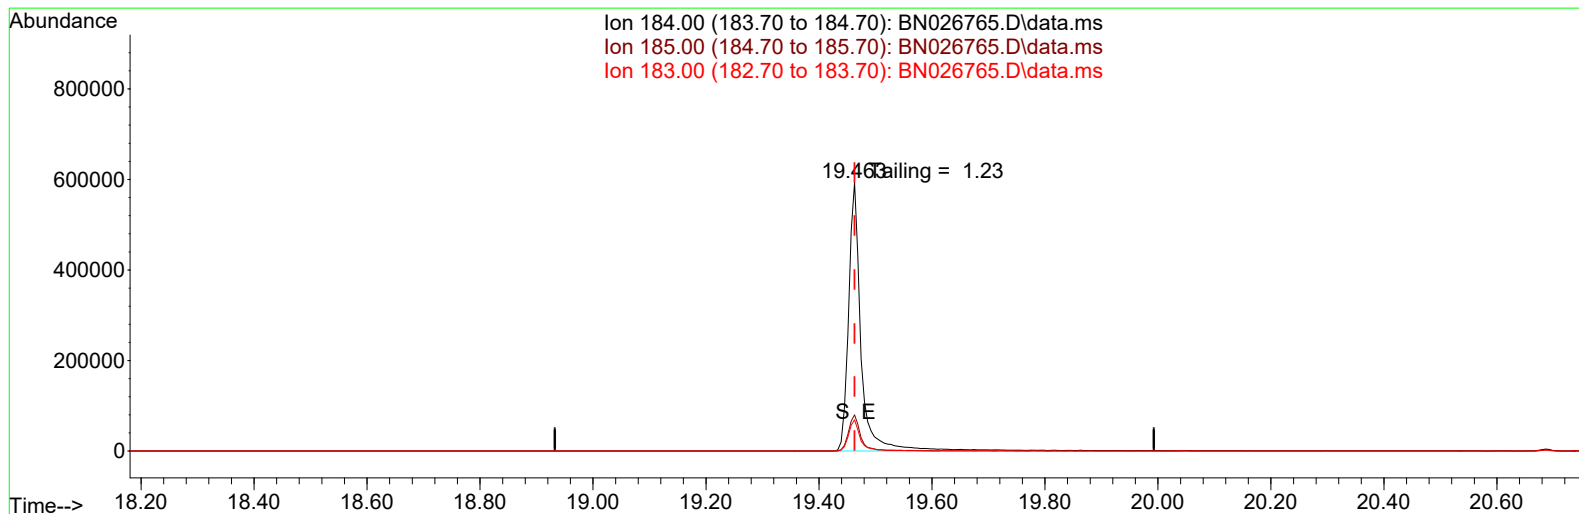

TIC: BN026765.D\data.ms

(77) Benzidine

19.463min (0.000) 0.00 ng

response 902039

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.46
183.00	13.20	11.62
0.00	0.00	0.00