
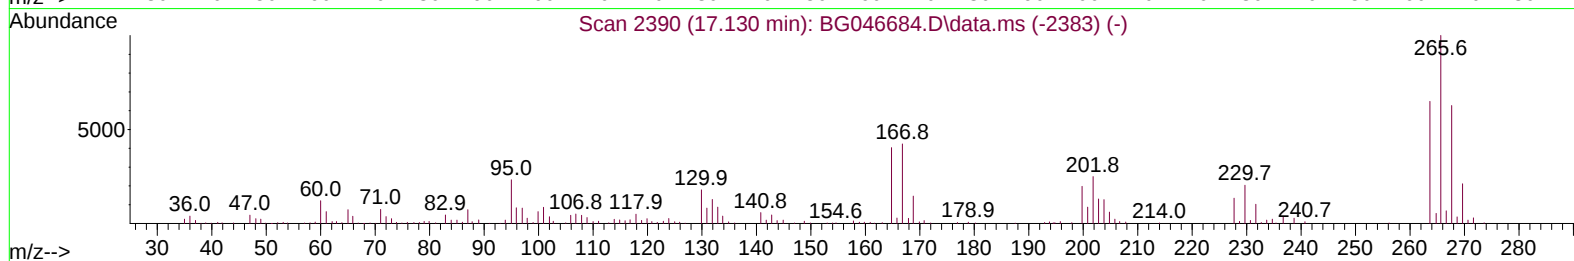
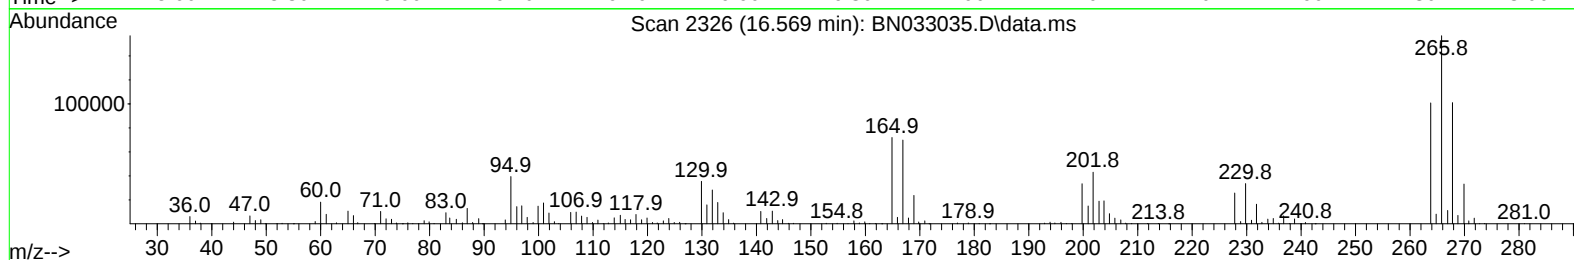


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033035.D
Acq On : 27 Jul 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jul 29 00:56:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

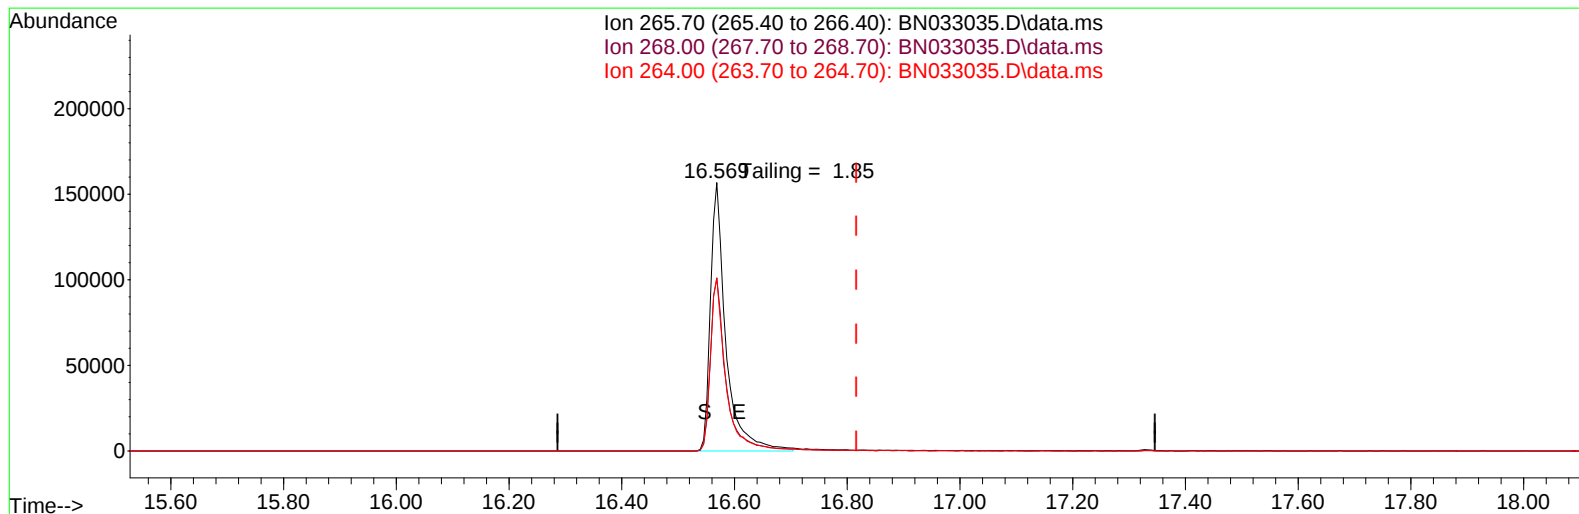

TIC: BN033035.D\data.ms

(70) Pentachlorophenol (C)




16.569min (-0.247) 21778.49 ng

response 301489

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033035.D
Acq On : 27 Jul 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Jul 29 00:56:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

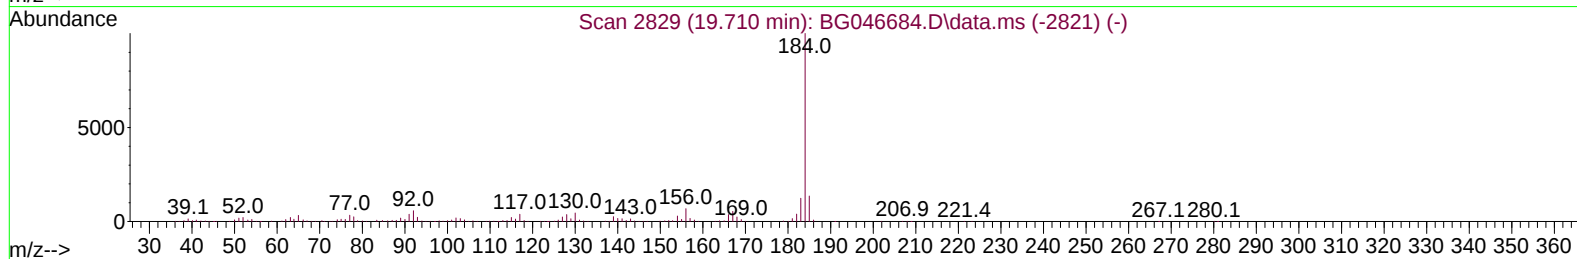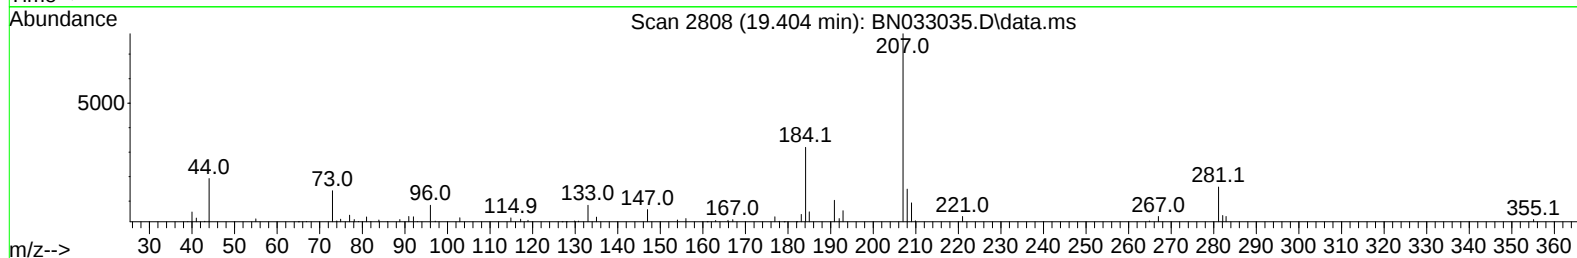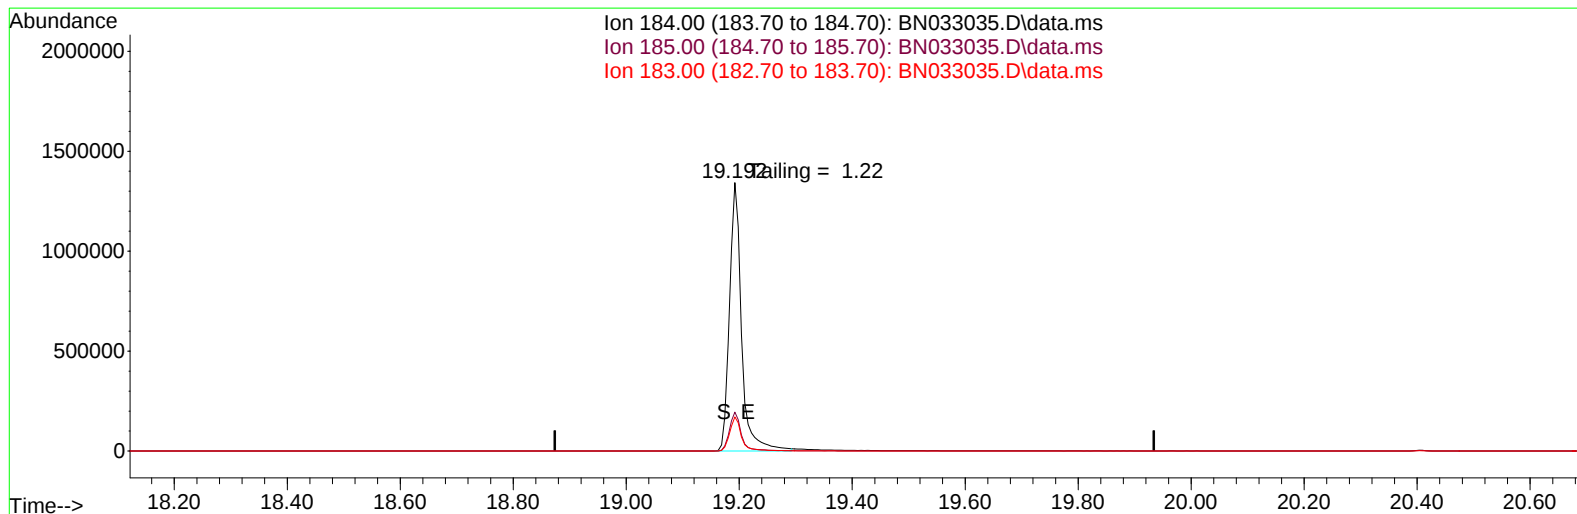

TIC: BN033035.D\data.ms

(77) Benzidine

19.404min (-19.404) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.50	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00