
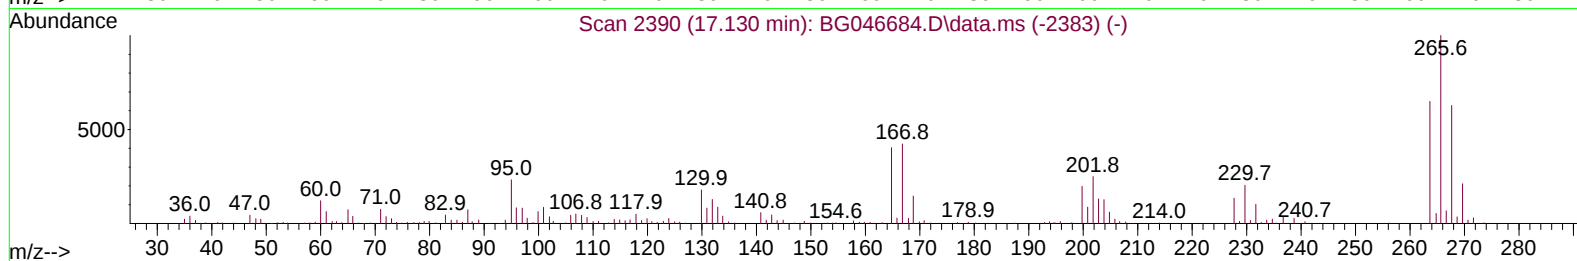
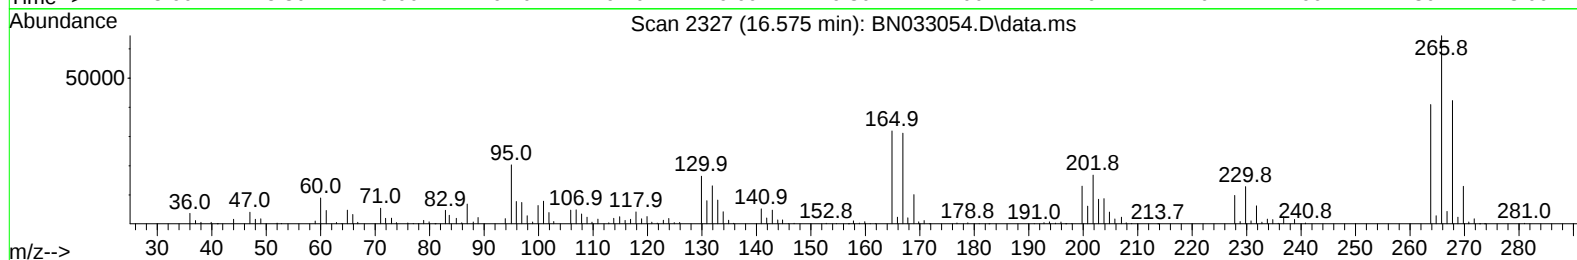


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033054.D
Acq On : 28 Jul 2024 04:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Quant Time: Jul 29 04:25:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

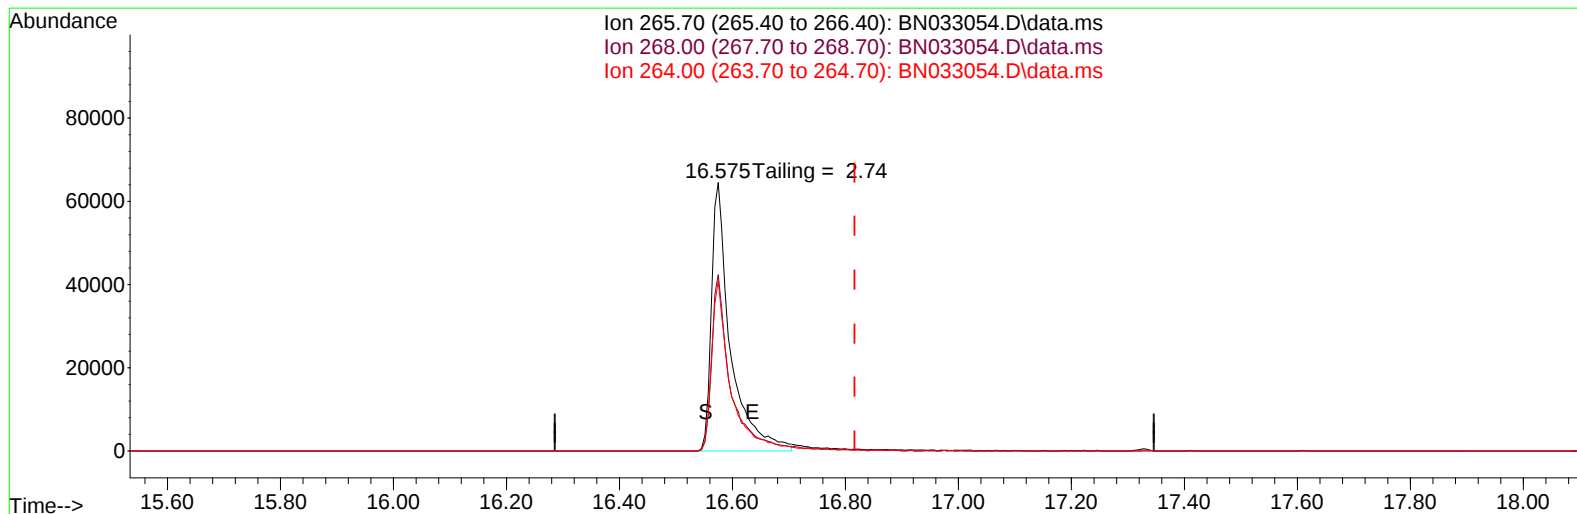

TIC: BN033054.D\data.ms

(70) Pentachlorophenol (C)




16.575min (-0.241) 16014.53 ng

response 154961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.65
264.00	61.60	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033054.D
Acq On : 28 Jul 2024 04:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Quant Time: Jul 29 04:25:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

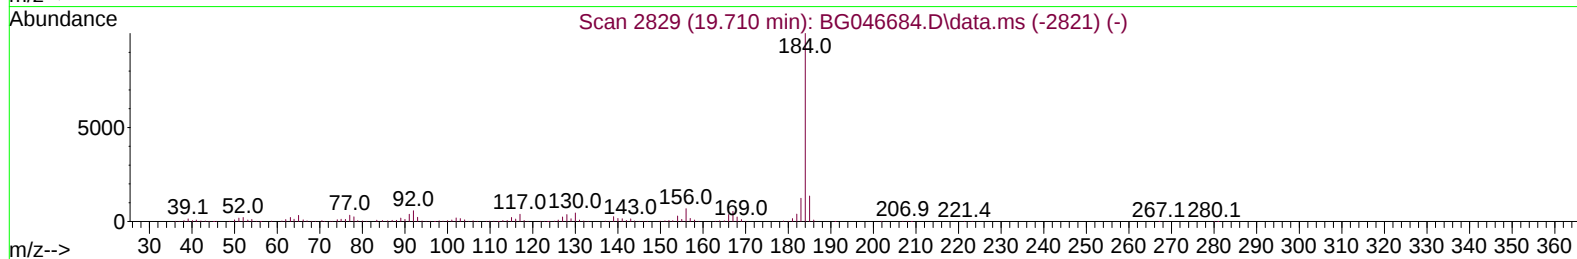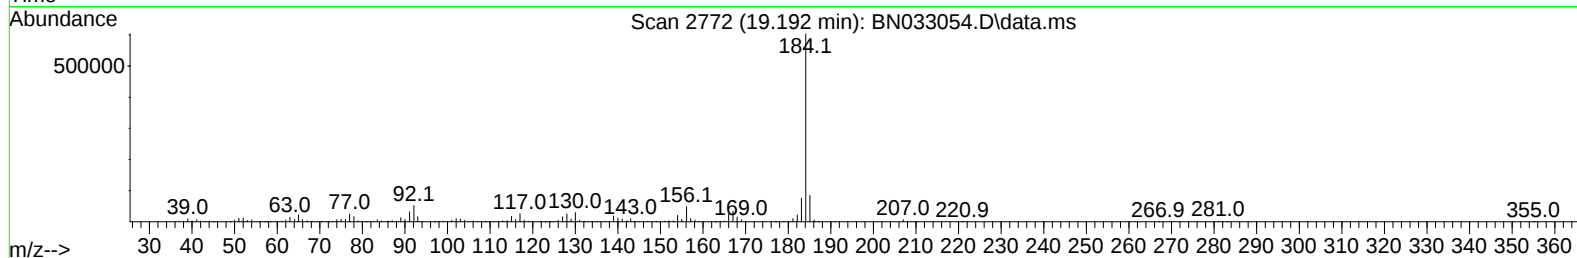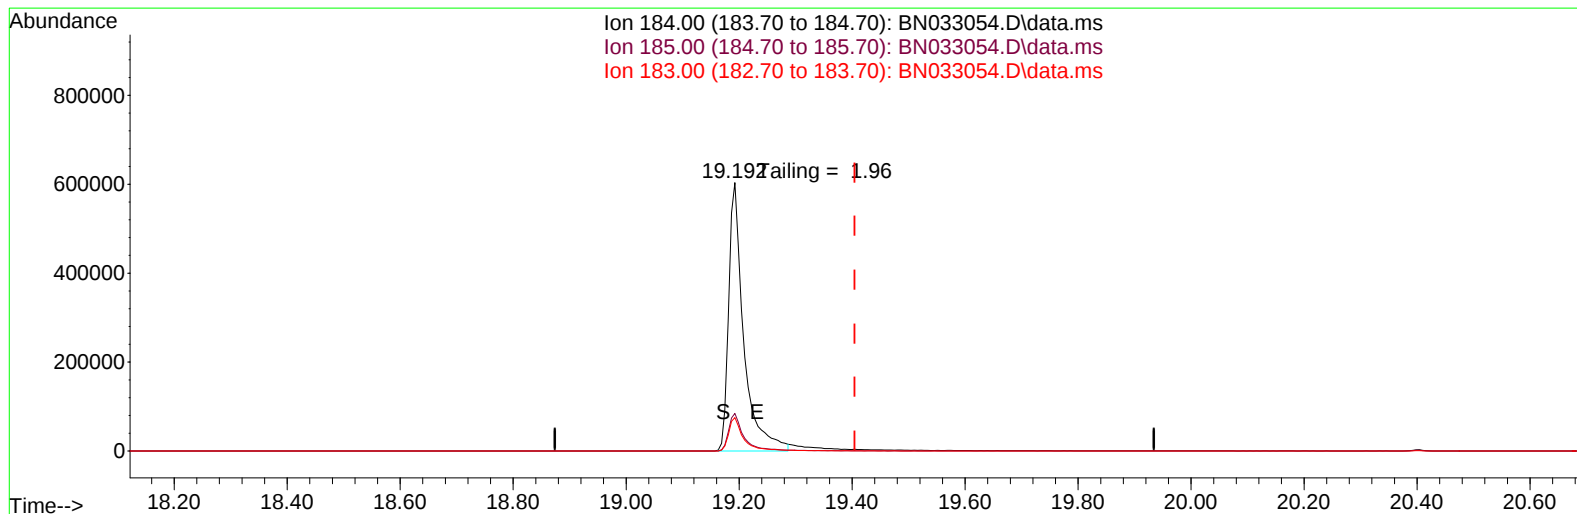

TIC: BN033054.D\data.ms

(77) Benzidine

19.192min (-0.212) 0.00 ng

response 1164515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	12.51
0.00	0.00	0.00