
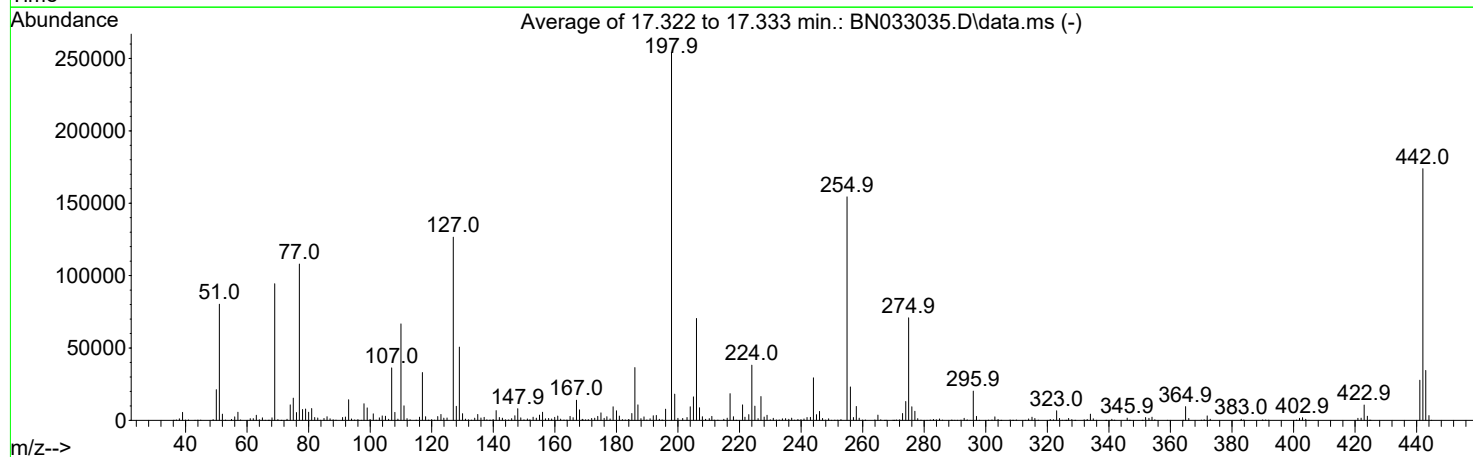


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033035.D
Acq On : 27 Jul 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Jul 21 23:33:21 2024

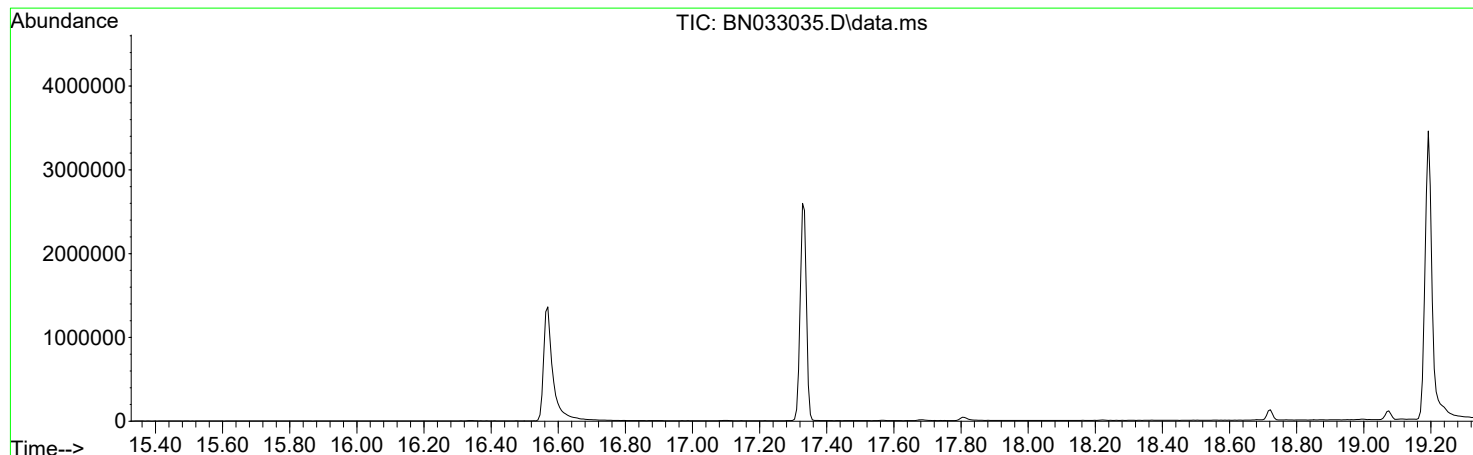

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	80192	PASS
68	69	0.00	2	1.9	1788	PASS
69	198	0.00	100	37.2	94456	PASS
70	69	0.00	2	0.5	515	PASS
127	198	10	80	49.8	126536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	254123	PASS
199	198	5	9	7.1	18145	PASS
275	198	10	60	27.9	70907	PASS
365	198	1	100	3.7	9459	PASS
441	198	0.01	100	10.9	27752	PASS
442	442	50	100	100.0	173899	PASS
443	442	15	24	19.8	34451	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/27/2024	BNA_N	<u>BN033035.D</u>
Compound Name	Response	Retention Time
DDT	1012469	20.404
DDD	45267	19.974
DDE	2039	19.451
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47306	1059775	4.46

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033035.D
Acq On : 27 Jul 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 00:56:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

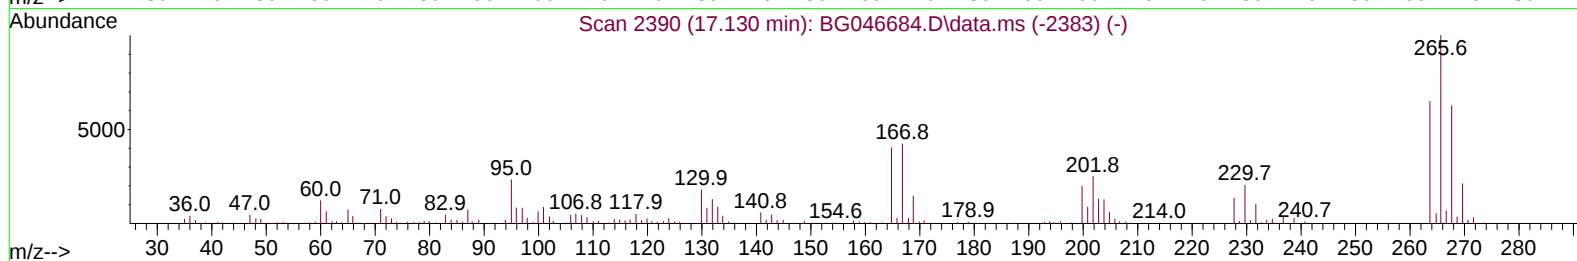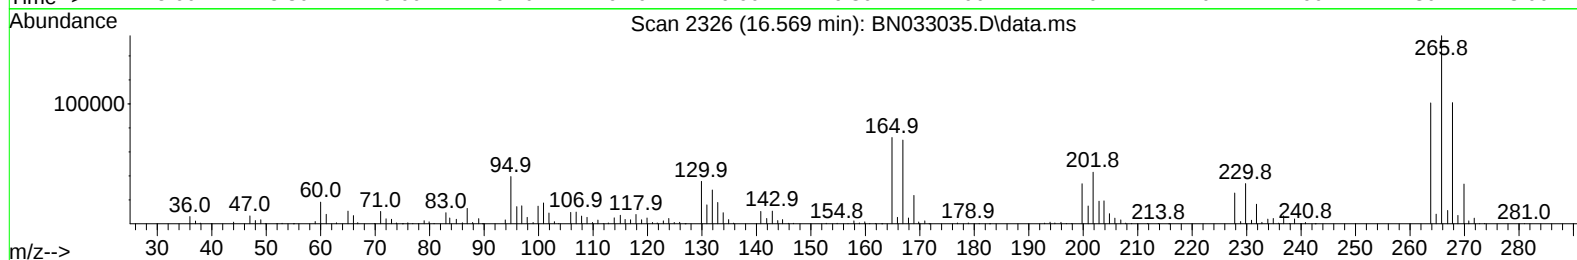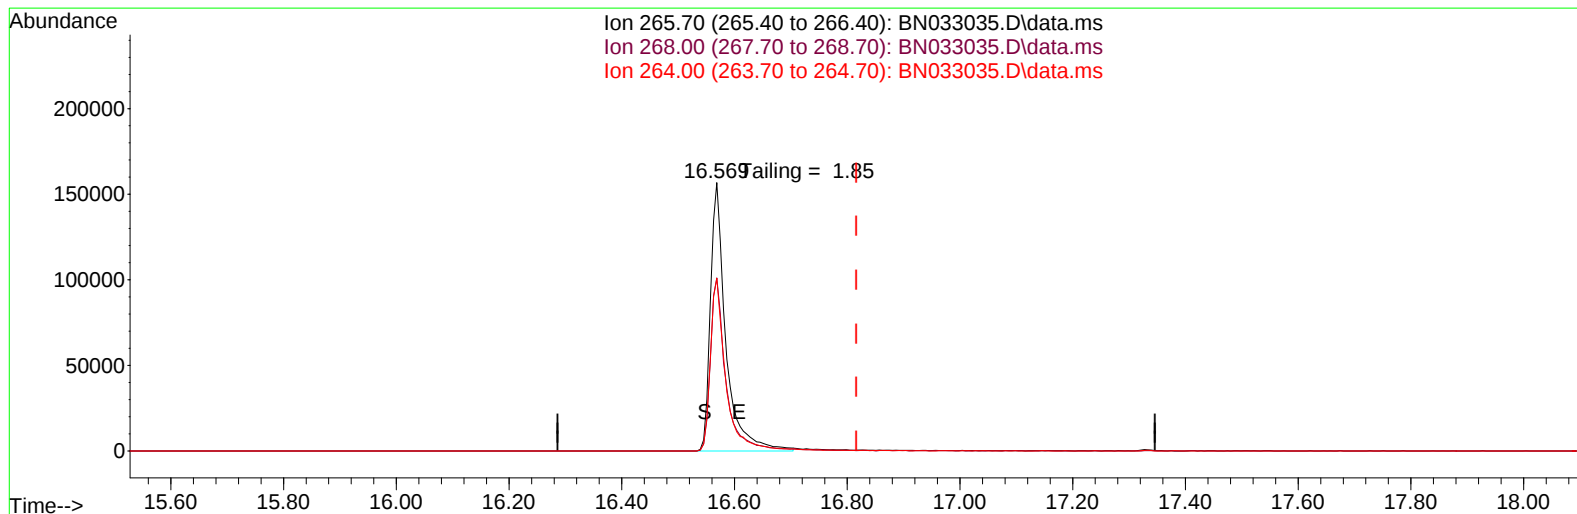

TIC: BN033035.D\data.ms

(70) Pentachlorophenol (C)

16.569min (-0.247) 21778.49 ng




response 301489

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.50
264.00	61.60	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033035.D
Acq On : 27 Jul 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 00:56:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

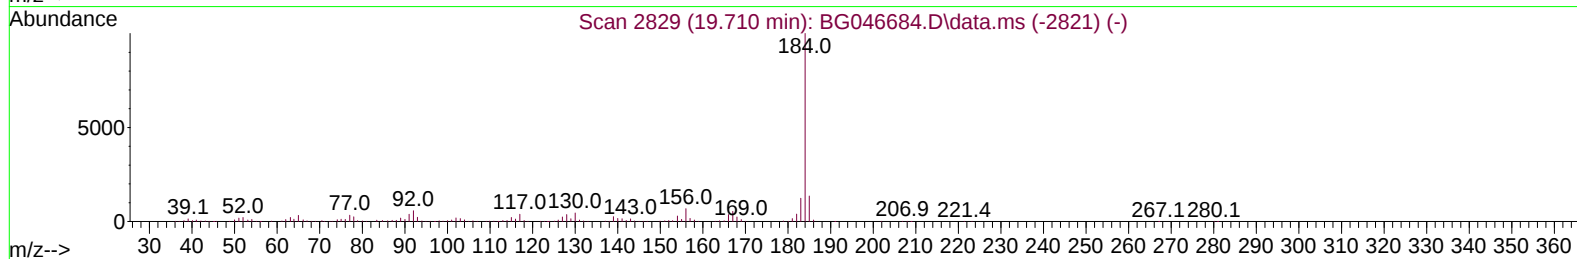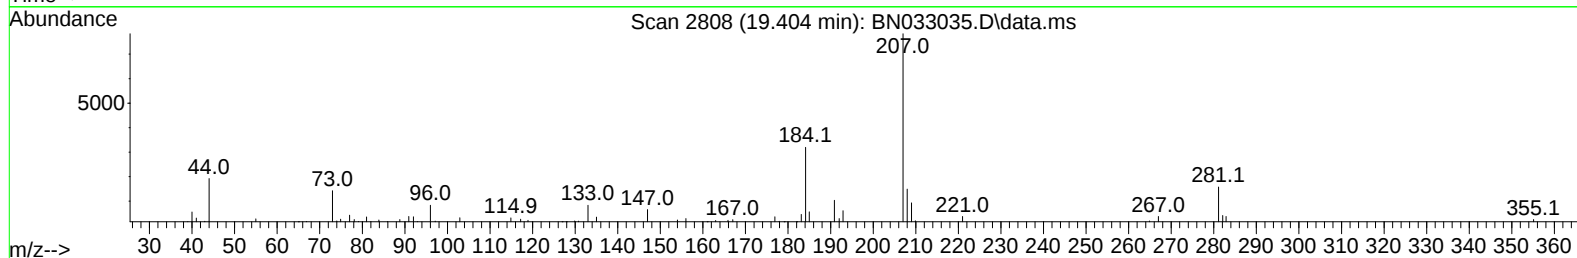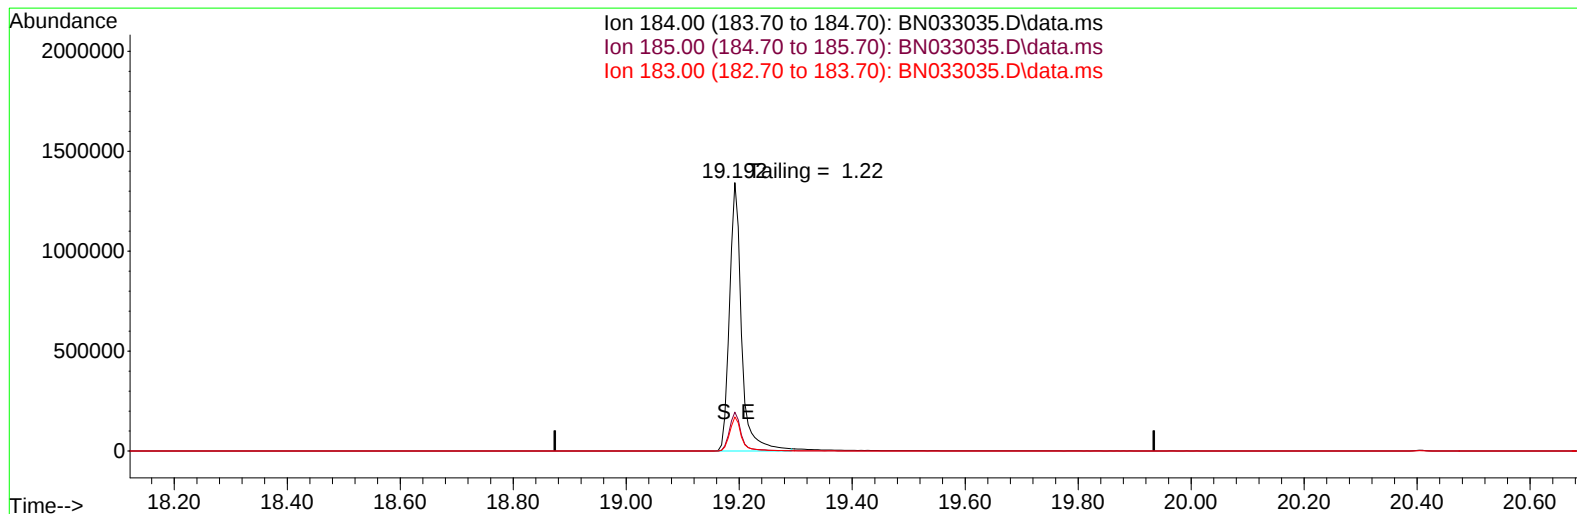

TIC: BN033035.D\data.ms

(77) Benzidine

19.404min (-19.404) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.50	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00