
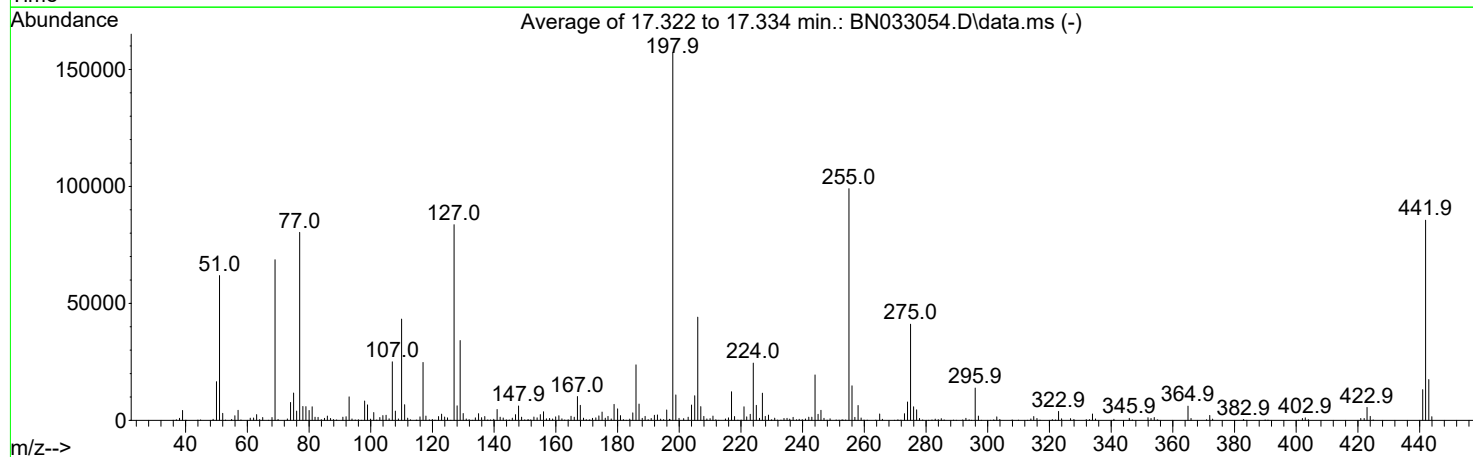


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033054.D
Acq On : 28 Jul 2024 04:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Jul 21 23:33:21 2024

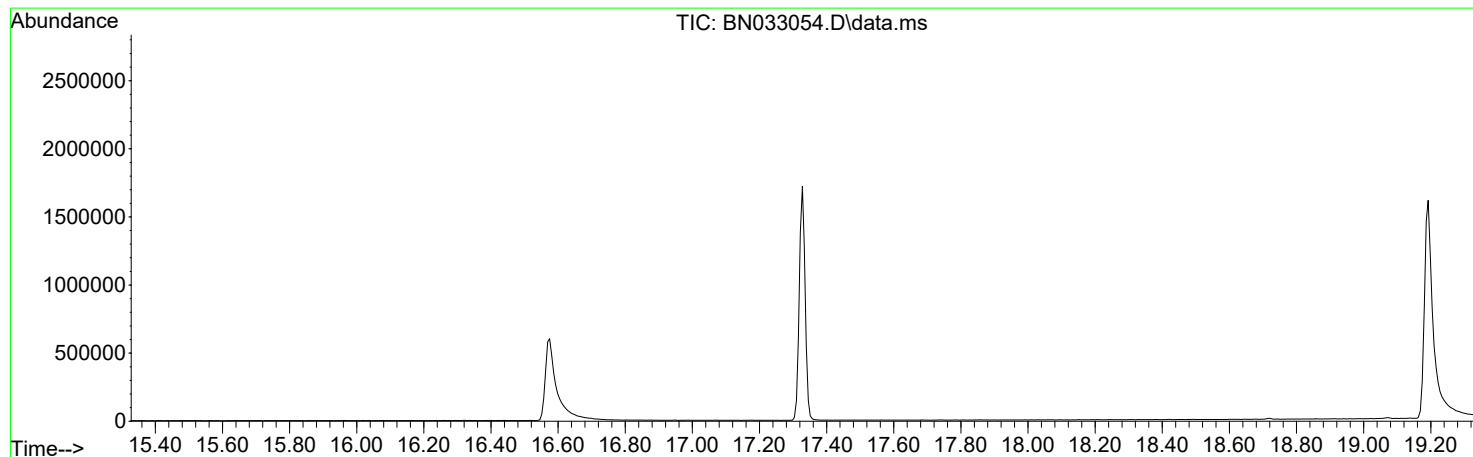

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	61920	PASS
68	69	0.00	2	1.8	1231	PASS
69	198	0.00	100	43.7	68653	PASS
70	69	0.00	2	0.6	425	PASS
127	198	10	80	53.2	83656	PASS
197	198	0.00	2	0.3	517	PASS
198	198	100	100	100.0	157227	PASS
199	198	5	9	6.9	10910	PASS
275	198	10	60	26.2	41128	PASS
365	198	1	100	3.9	6103	PASS
441	198	0.01	100	8.4	13136	PASS
442	442	50	100	100.0	85539	PASS
443	442	15	24	20.4	17456	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/27/2024	BNA_N	<u>BN033054.D</u>
Compound Name	Response	Retention Time
DDT	571367	20.404
DDD	25930	19.975
DDE	1488	19.451
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27418	598785	4.58

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033054.D
Acq On : 28 Jul 2024 04:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 04:25:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

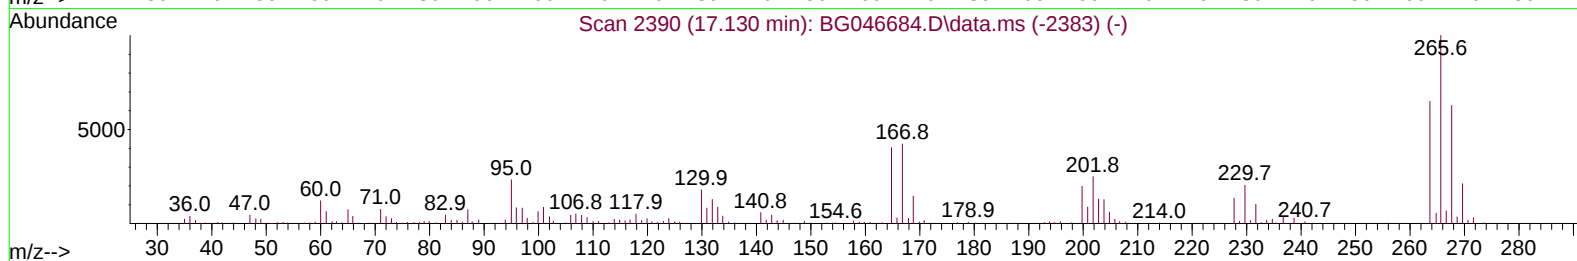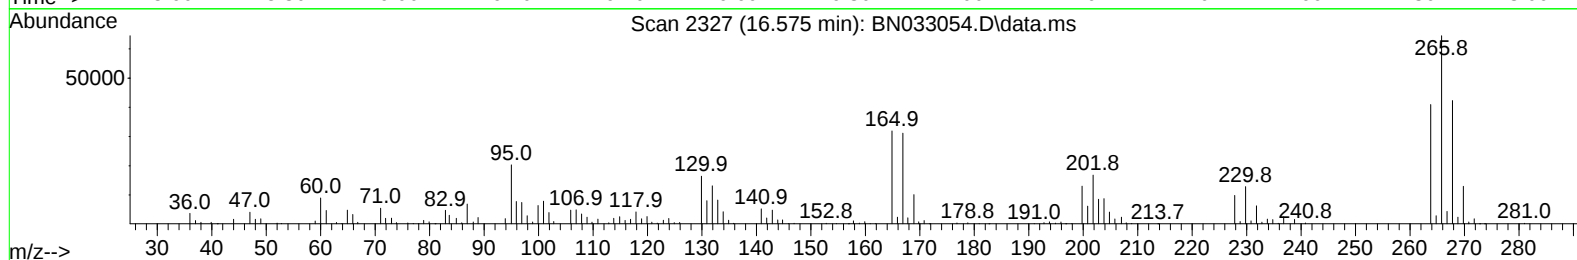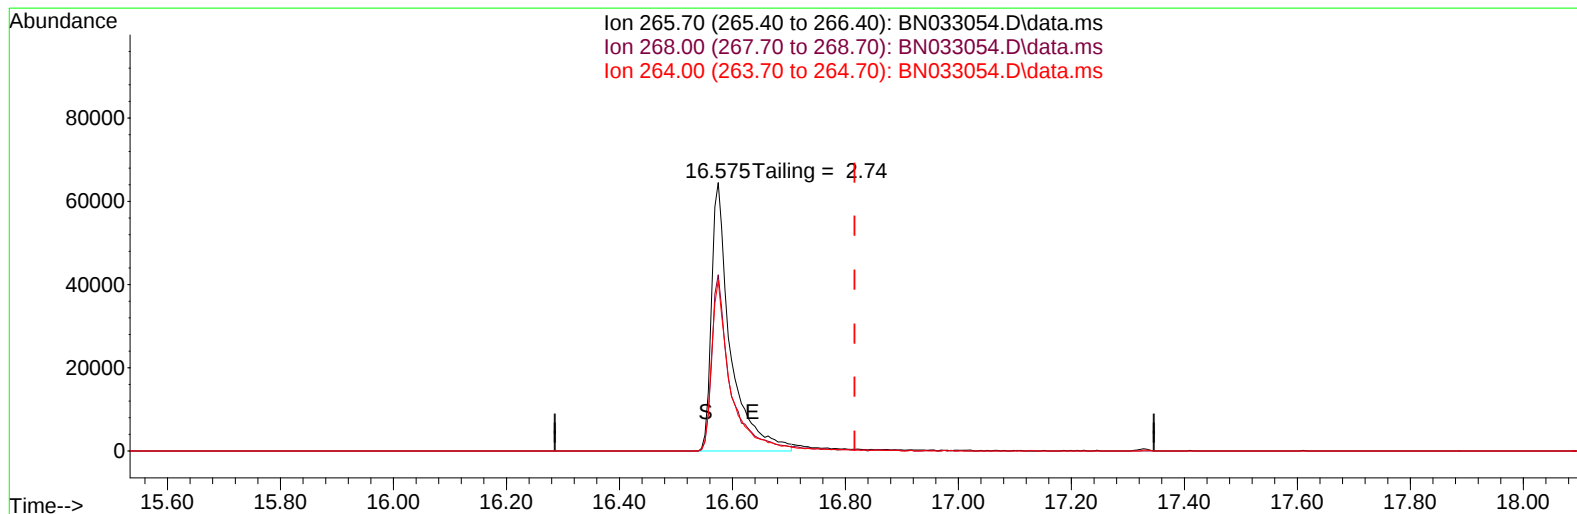

TIC: BN033054.D\data.ms

(70) Pentachlorophenol (C)

16.575min (-0.241) 16014.53 ng




response 154961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.65
264.00	61.60	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072724\
Data File : BN033054.D
Acq On : 28 Jul 2024 04:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 04:25:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

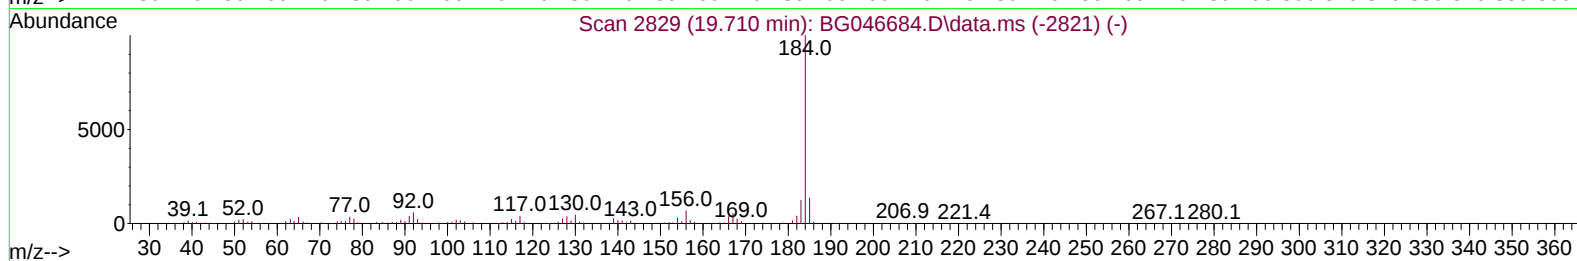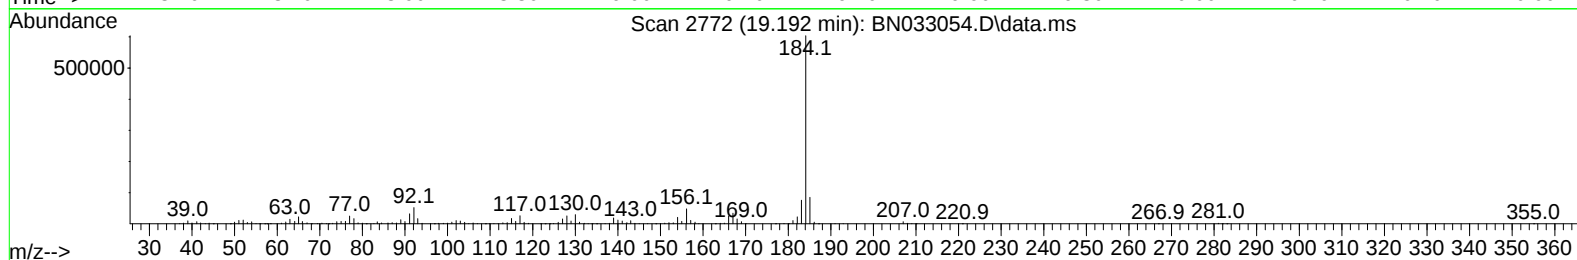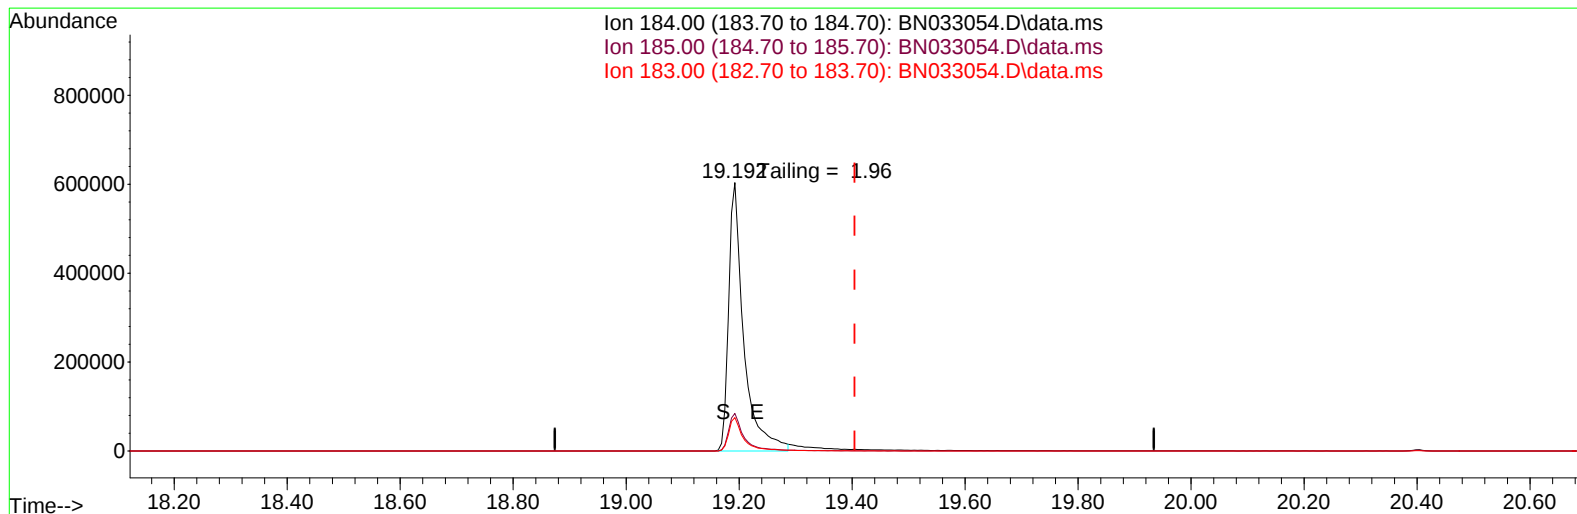

TIC: BN033054.D\data.ms

(77) Benzidine

19.192min (-0.212) 0.00 ng

response 1164515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	12.51
0.00	0.00	0.00