
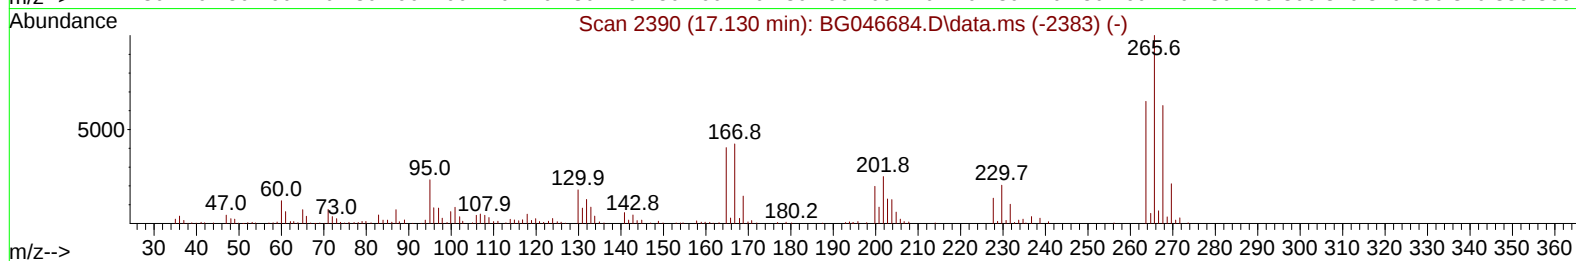
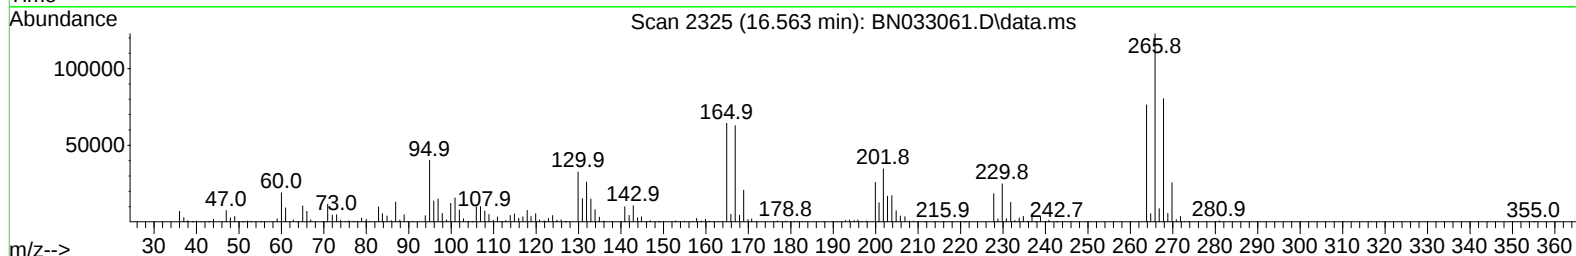


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072924\
Data File : BN033061.D
Acq On : 29 Jul 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 11:55:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

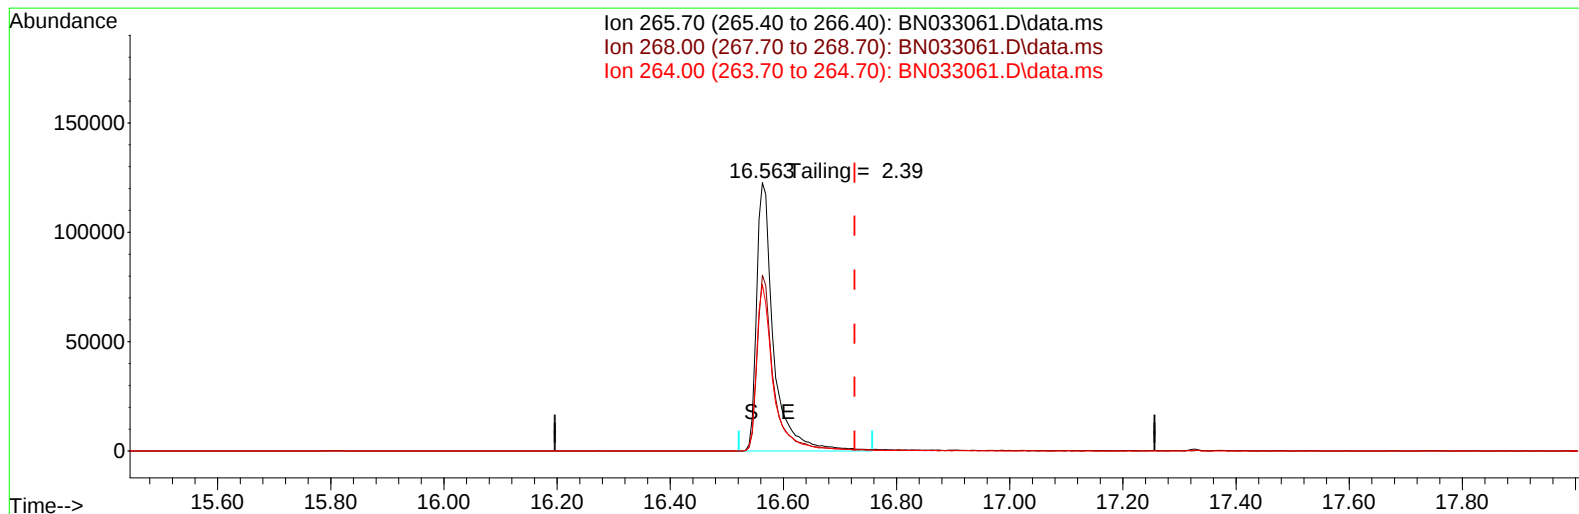

TIC: BN033061.D\data.ms

(70) Pentachlorophenol (C)




16.563min (-0.163) 20609.42 ng

response 255707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.52
264.00	61.60	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072924\
Data File : BN033061.D
Acq On : 29 Jul 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 11:55:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

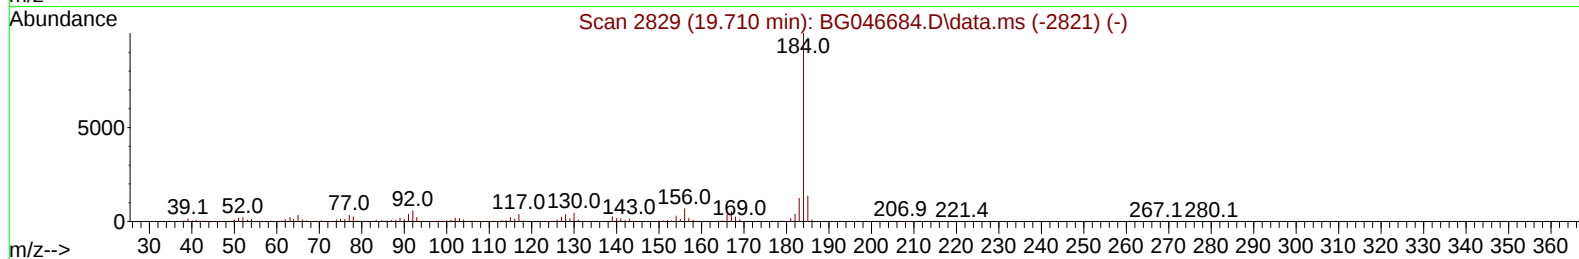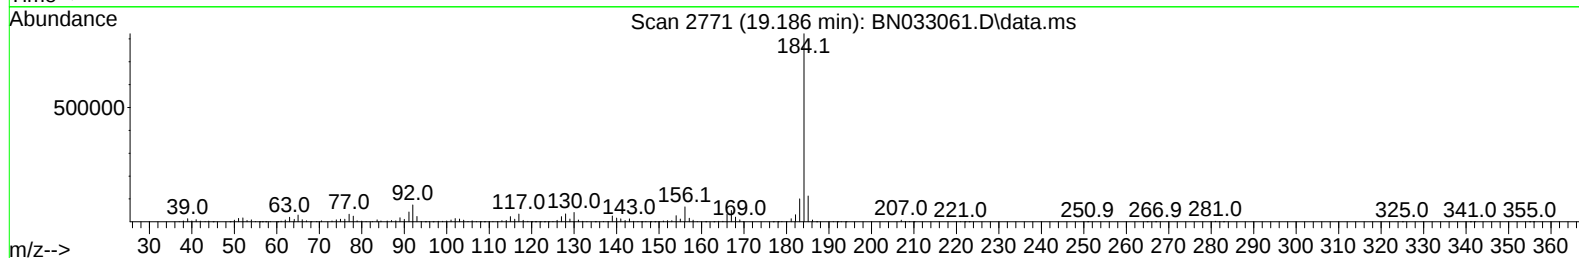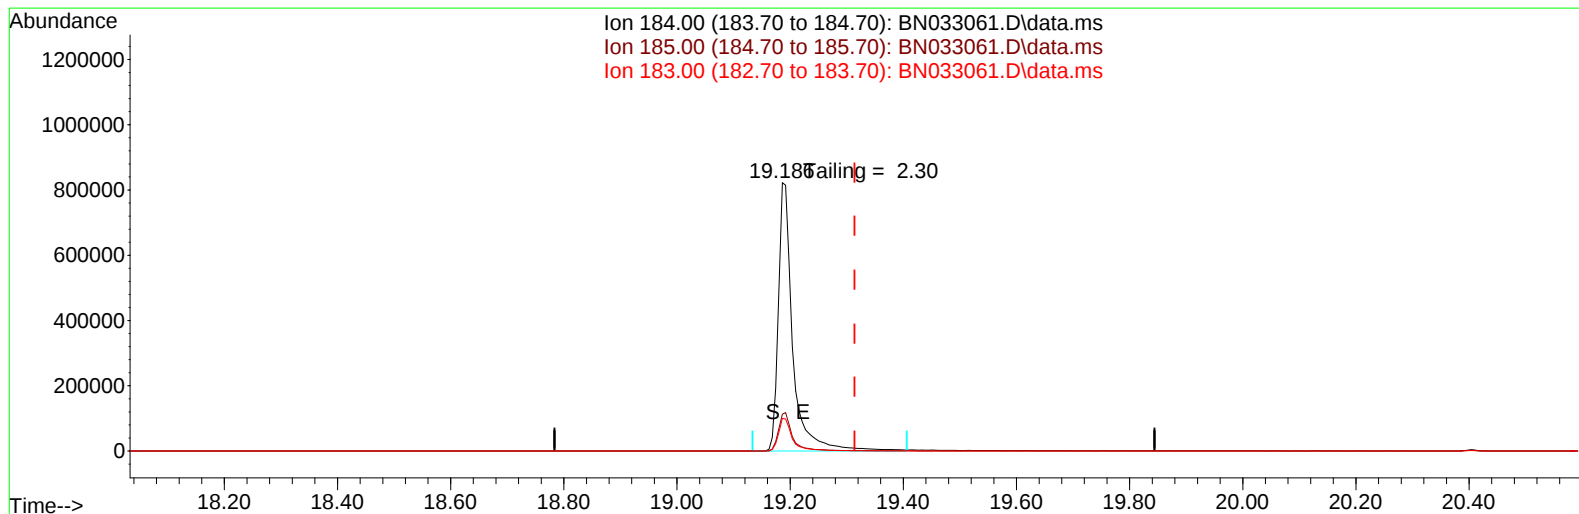

TIC: BN033061.D\data.ms

(77) Benzidine**19.186min (-0.128) 375687.56 ng m****response 1470750**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.72
183.00	13.20	12.17
0.00	0.00	0.00