


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072924\
Data File : BN033061.D
Acq On : 29 Jul 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 29 10:37:08 2024

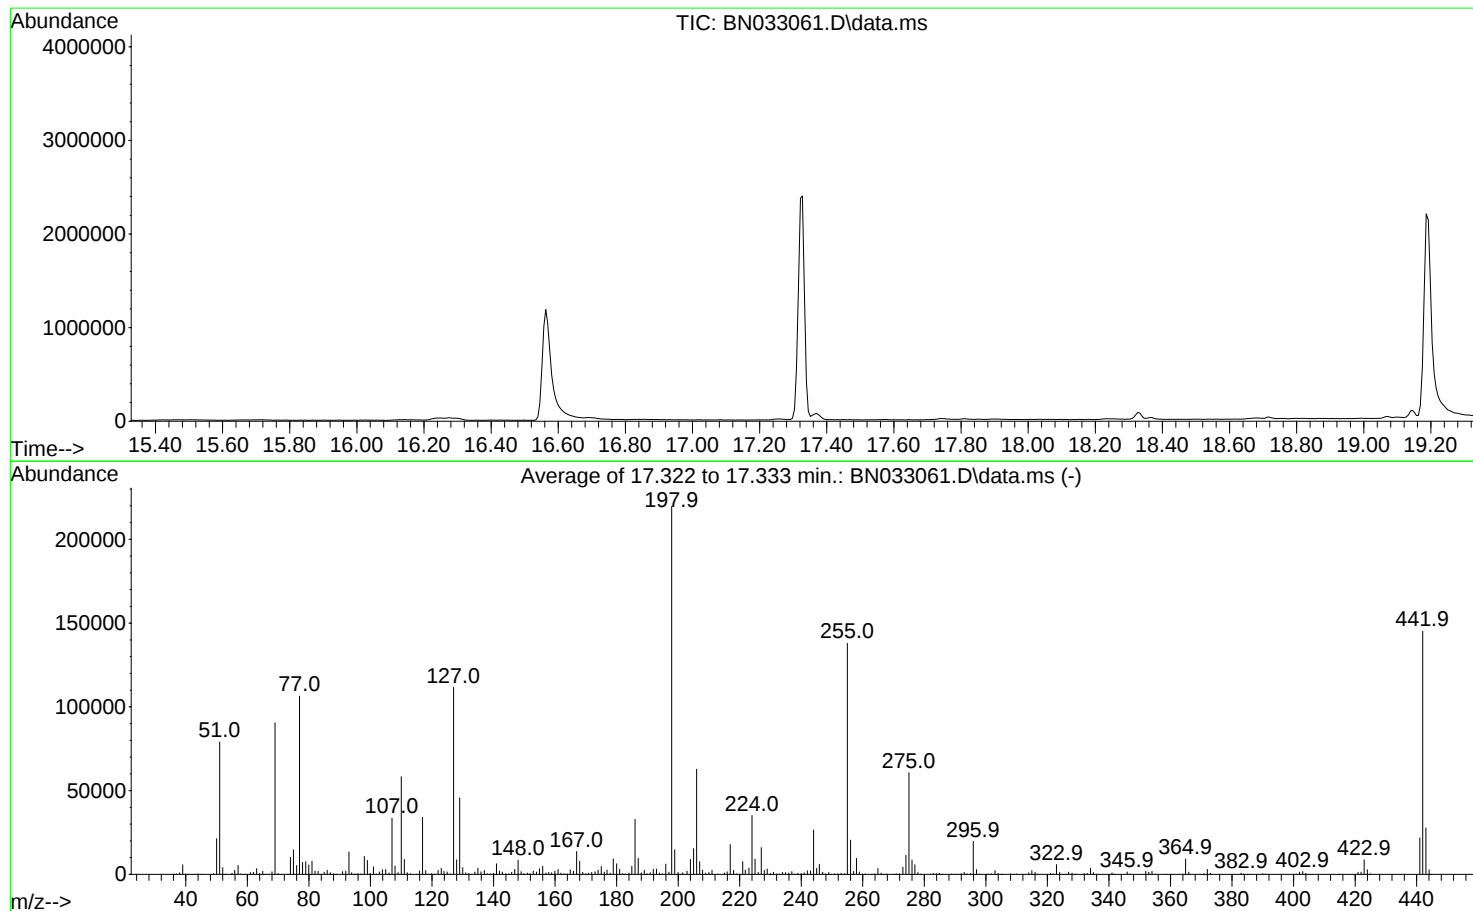

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	78965	PASS
68	69	0.00	2	1.7	1538	PASS
69	198	0.00	100	41.2	90560	PASS
70	69	0.00	2	0.7	606	PASS
127	198	10	80	50.8	111635	PASS
197	198	0.00	2	0.6	1344	PASS
198	198	100	100	100.0	219627	PASS
199	198	5	9	6.7	14765	PASS
275	198	10	60	27.7	60800	PASS
365	198	1	100	4.2	9223	PASS
441	198	0.01	100	9.9	21757	PASS
442	442	50	100	100.0	145232	PASS
443	442	15	24	19.1	27715	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/29/2024	BNA_N	<u>BN033061.D</u>
Compound Name	Response	Retention Time
DDT	838522	20.404
DDD	40748	19.974
DDE	2988	19.451
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43736	882258	4.96

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072924\
Data File : BN033061.D
Acq On : 29 Jul 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 11:55:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

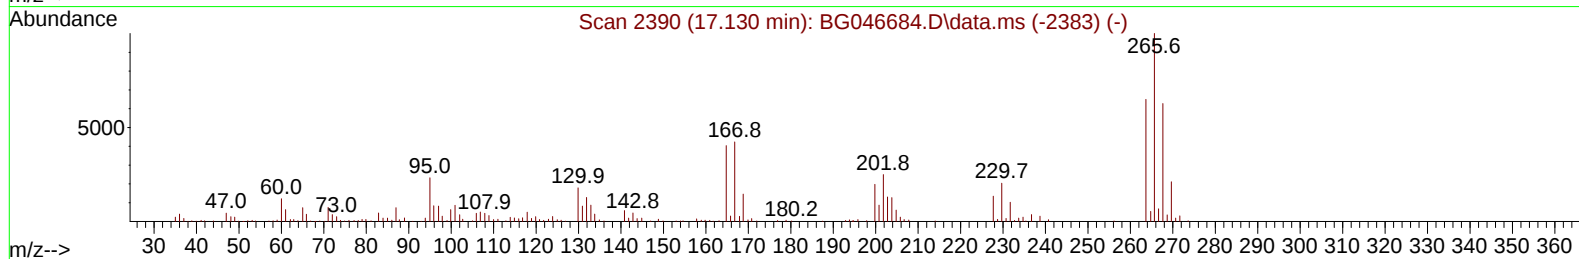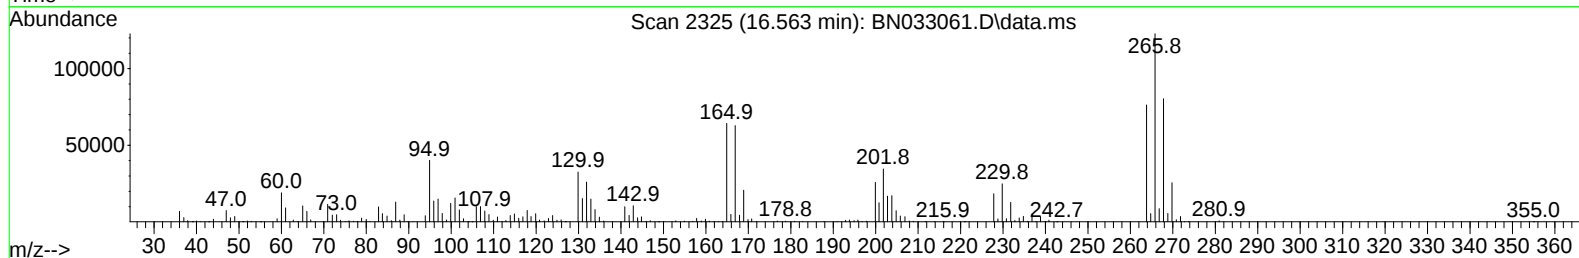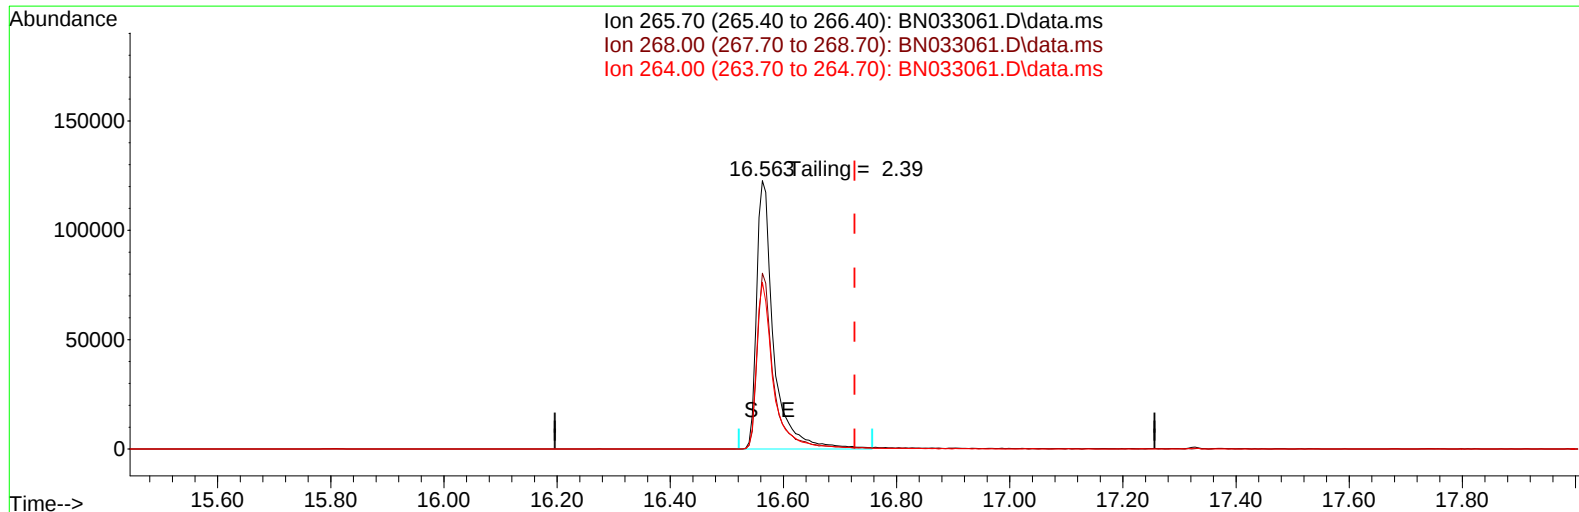

TIC: BN033061.D\data.ms

(70) Pentachlorophenol (C)

16.563min (-0.163) 20609.42 ng




response 255707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.52
264.00	61.60	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072924\
Data File : BN033061.D
Acq On : 29 Jul 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 29 11:55:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

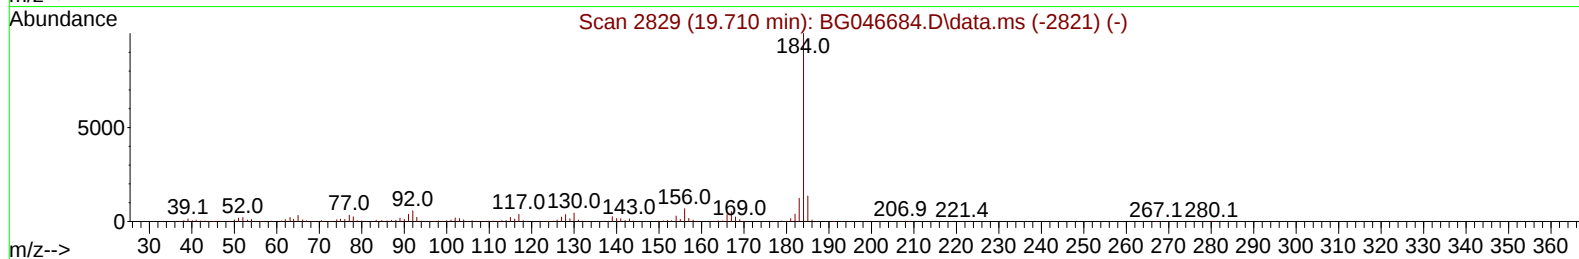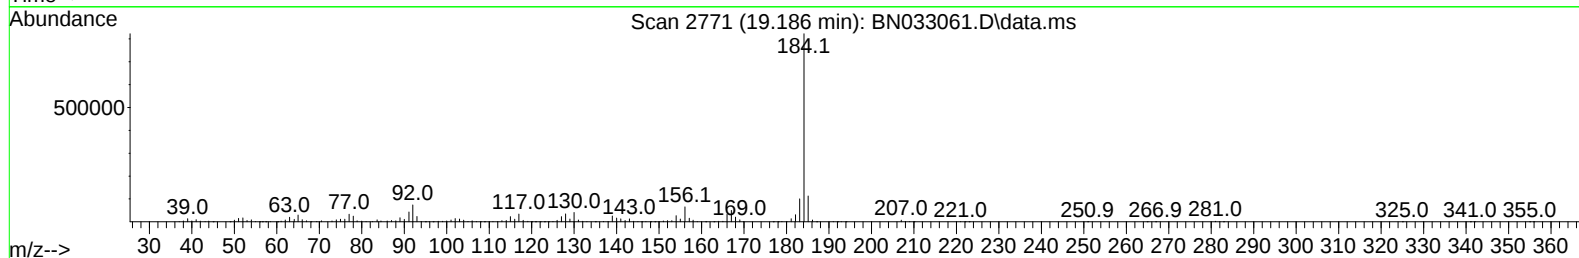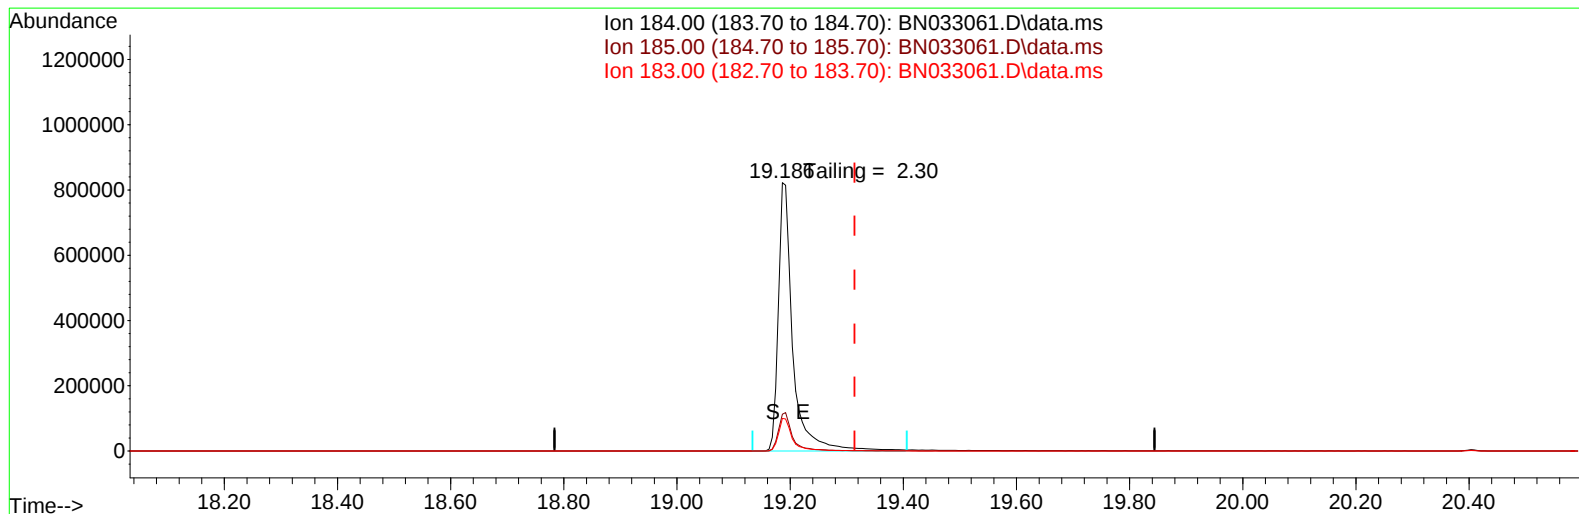

TIC: BN033061.D\data.ms

(77) Benzidine

19.186min (-0.128) 375687.56 ng m

response 1470750

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.72
183.00	13.20	12.17
0.00	0.00	0.00