
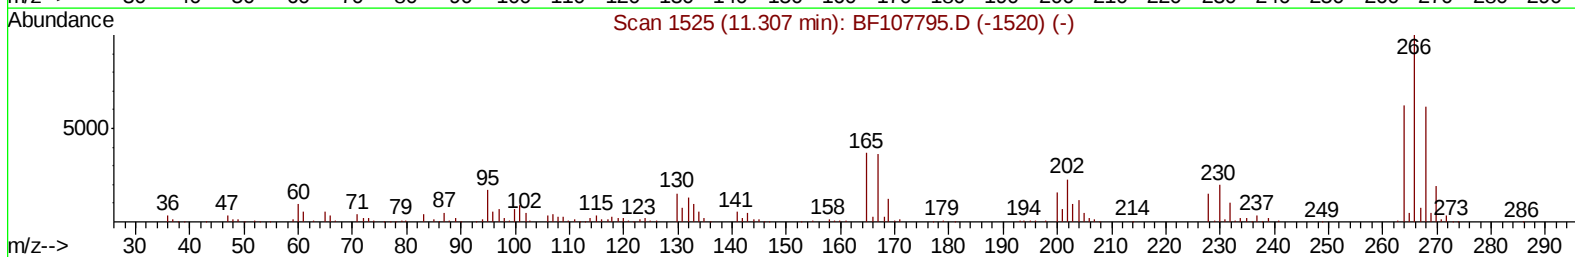
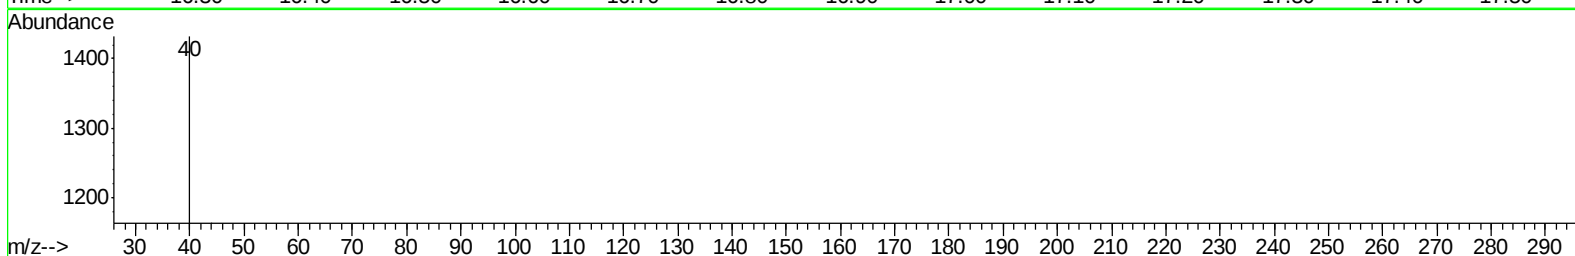


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073018\  
 Data File : BN002180.D  
 Acq On : 30 Jul 2018 09:22  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 02:18:48 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jul 30 17:48:53 2018  
 Response via : Initial Calibration

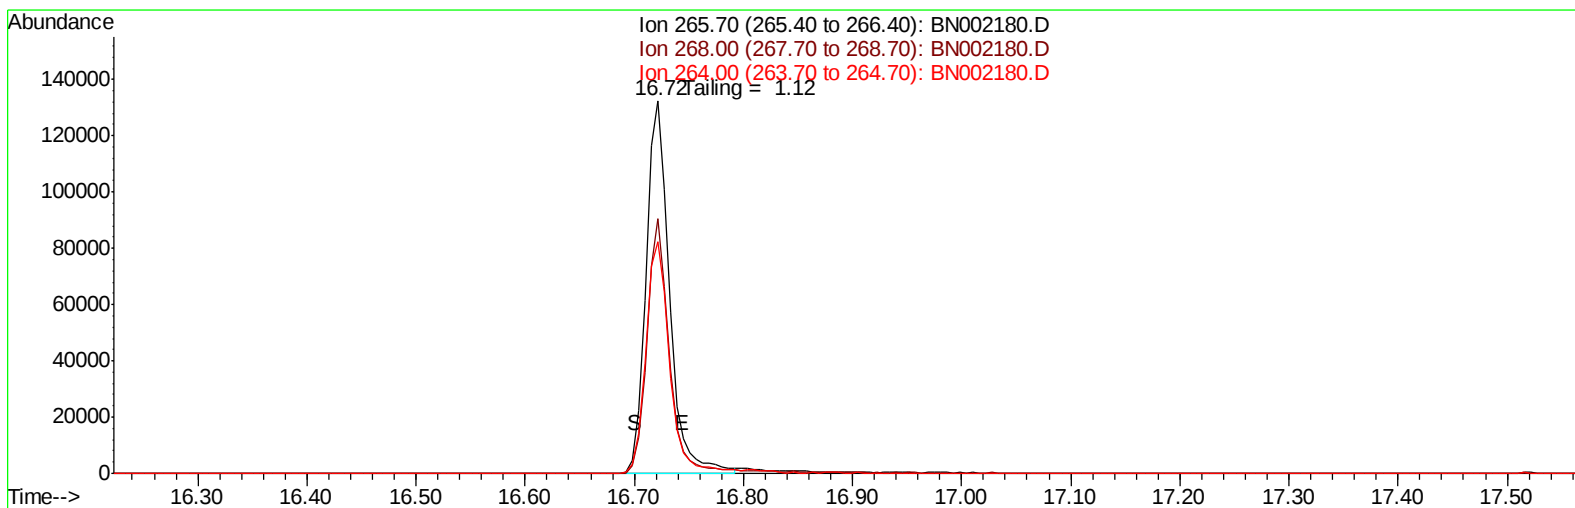

TIC: BN002180.D

(69) Pentachlorophenol (C)




11.307min (-11.307) 0.00ng

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 0.00  |
| 268.00 | 63.90 | 0.00# |
| 264.00 | 61.90 | 0.00# |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073018\  
 Data File : BN002180.D  
 Acq On : 30 Jul 2018 09:22  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 02:18:48 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jul 30 17:48:53 2018  
 Response via : Initial Calibration

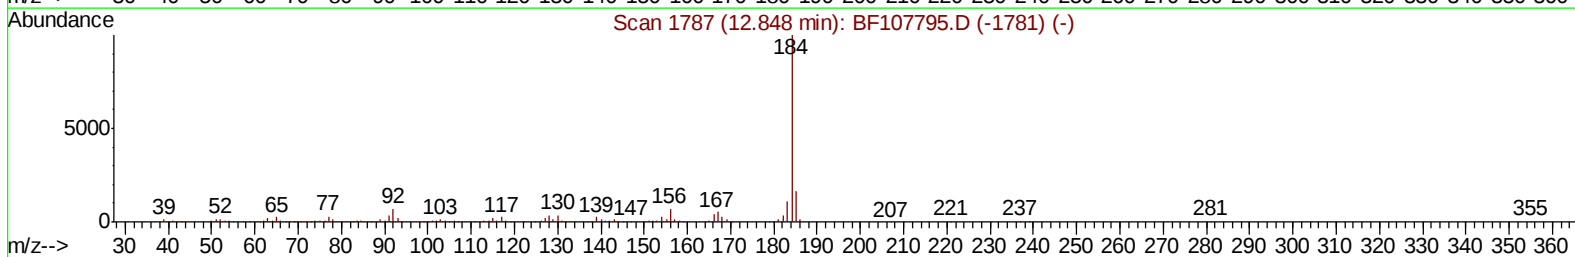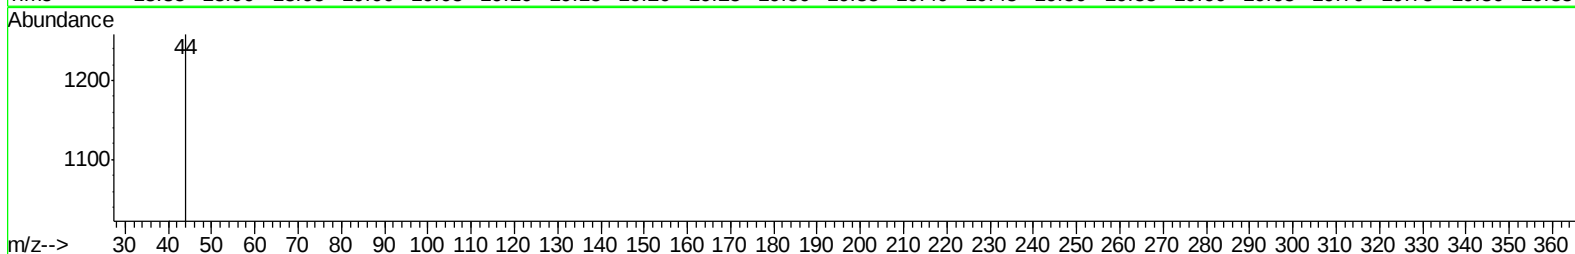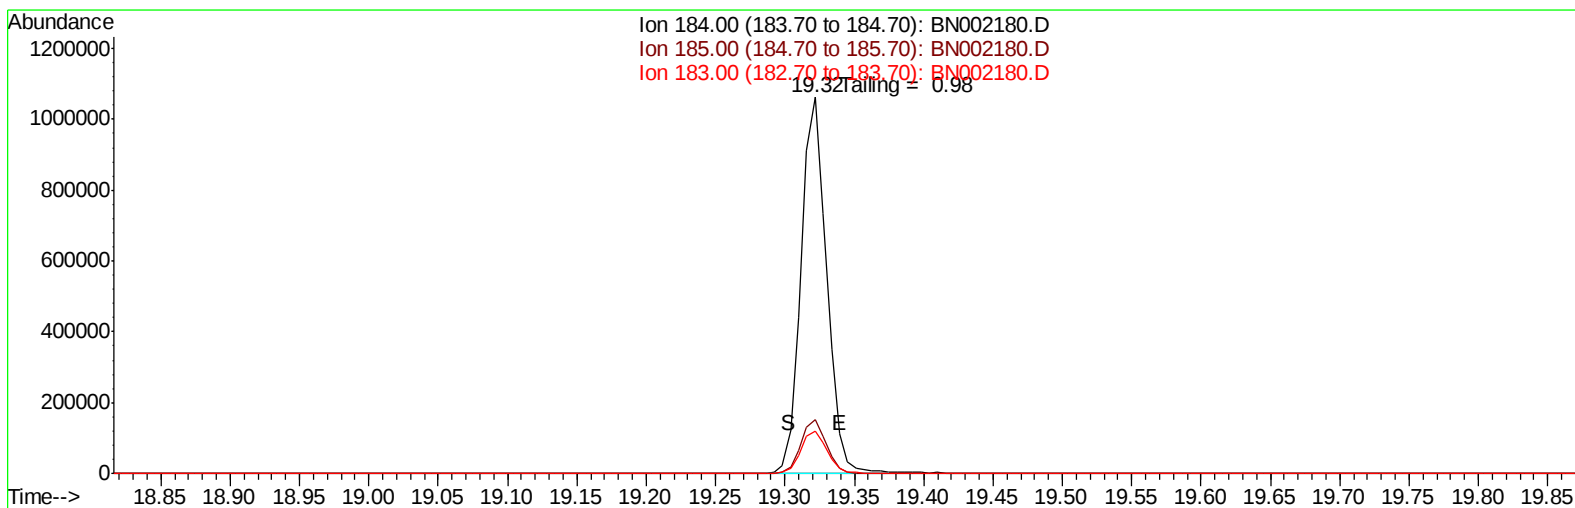

TIC: BN002180.D

(76) Benzidine

12.848min (-12.848) 0.00ng

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 0.00  |
| 185.00 | 15.70 | 0.00# |
| 183.00 | 11.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |