
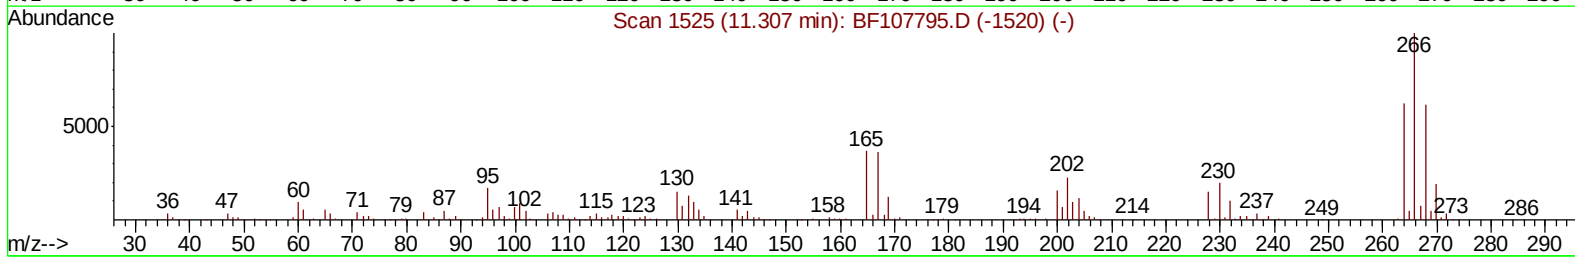
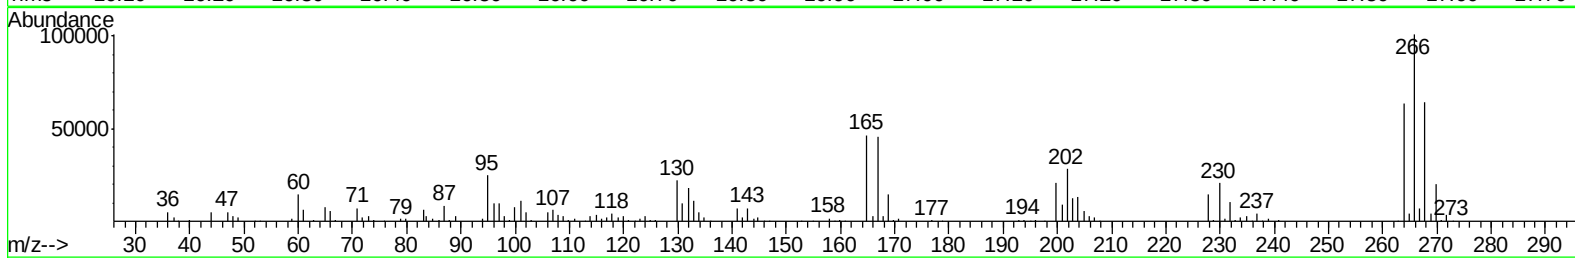


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073018\
Data File : BN002189.D
Acq On : 30 Jul 2018 17:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 02:20:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

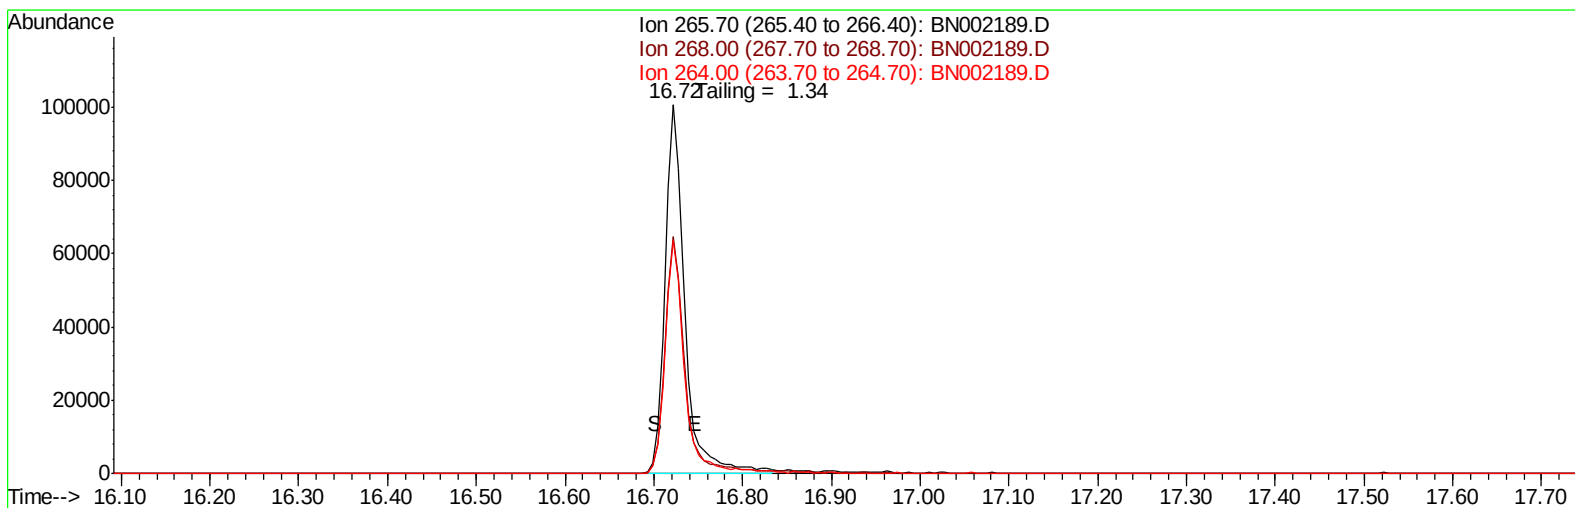

TIC: BN002189.D

(69) Pentachlorophenol (C)




16.722min (+5.415) 0.00ng m

response 157631

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.13
264.00	61.90	63.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN073018\
 Data File : BN002189.D
 Acq On : 30 Jul 2018 17:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 02:20:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 30 17:48:53 2018
 Response via : Initial Calibration

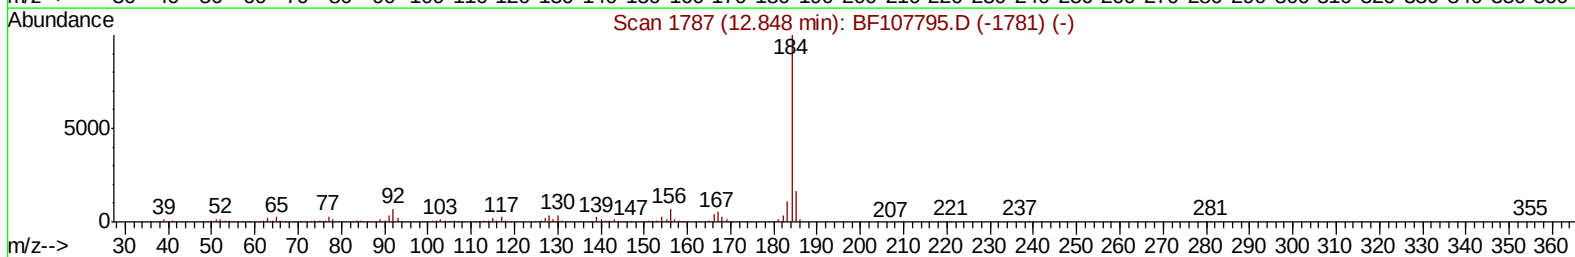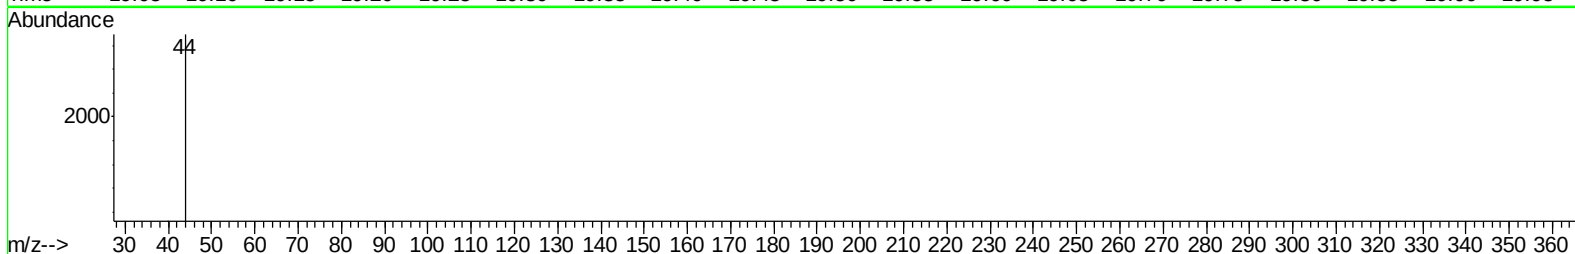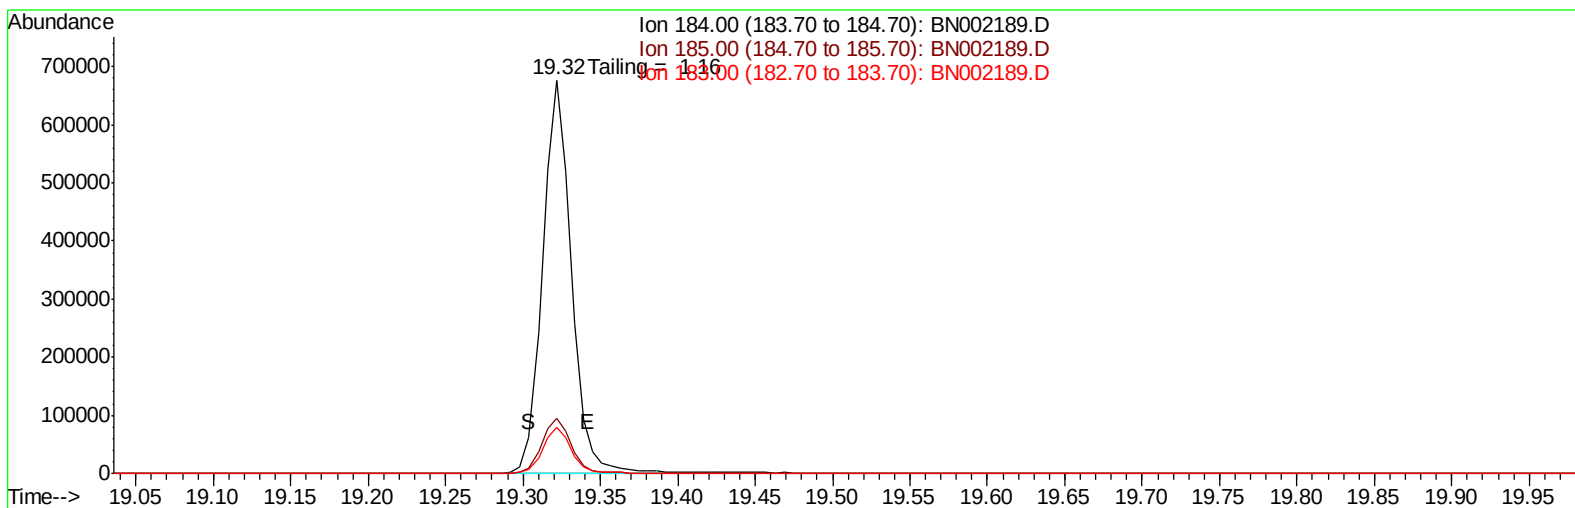

TIC: BN002189.D

(76) Benzidine

12.848min (-12.848) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00