


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN073018\
 Data File : BN002180.D
 Acq On : 30 Jul 2018 09:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 16:17:29 2018

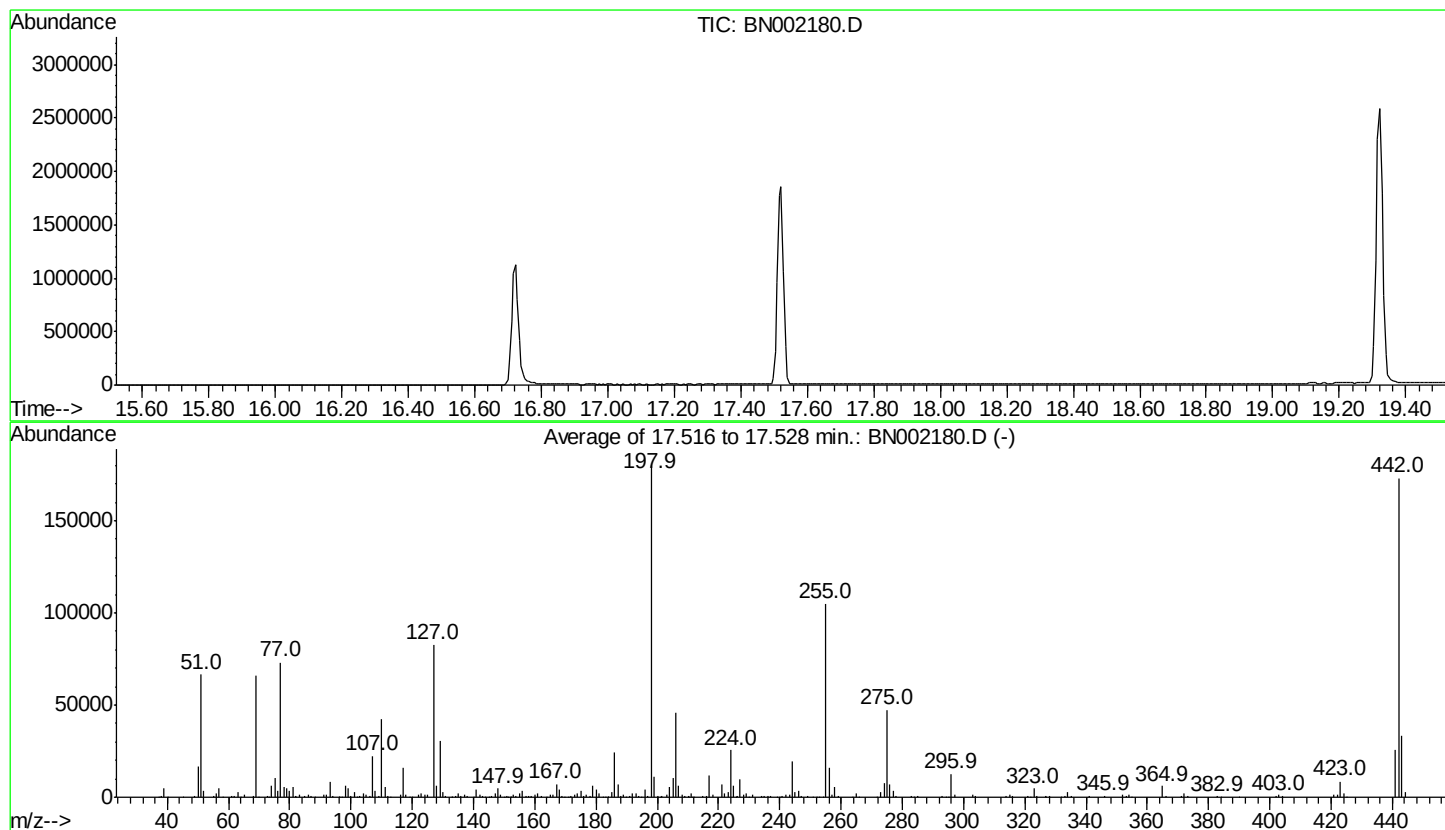

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	66560	PASS
68	69	0.00	2	1.5	966	PASS
69	198	0.00	100	36.9	66322	PASS
70	69	0.00	2	0.5	320	PASS
127	198	10	80	46.0	82794	PASS
197	198	0.00	2	0.5	840	PASS
198	198	100	100	100.0	179928	PASS
199	198	5	9	6.4	11477	PASS
275	198	10	60	26.4	47530	PASS
365	198	1	100	3.3	6023	PASS
441	198	0.01	100	14.5	26029	PASS
442	198	50	100	96.2	173013	PASS
443	442	15	24	19.3	33464	PASS