


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN073018\
 Data File : BN002189.D
 Acq On : 30 Jul 2018 17:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 16:17:29 2018

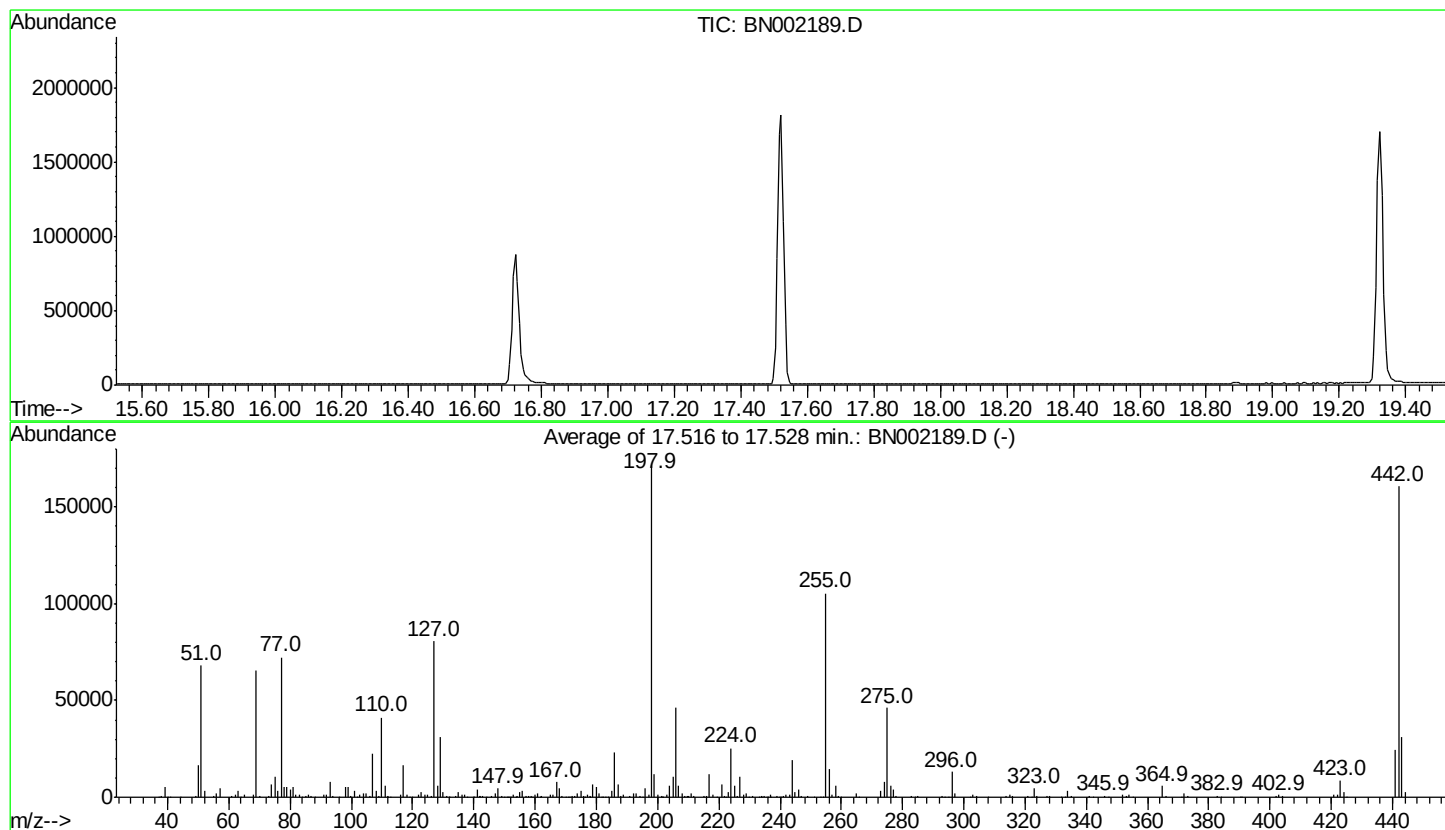

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	67941	PASS
68	69	0.00	2	1.7	1129	PASS
69	198	0.00	100	38.4	65821	PASS
70	69	0.00	2	0.6	376	PASS
127	198	10	80	47.0	80658	PASS
197	198	0.00	2	0.6	1025	PASS
198	198	100	100	100.0	171437	PASS
199	198	5	9	7.1	12186	PASS
275	198	10	60	26.9	46082	PASS
365	198	1	100	3.4	5781	PASS
441	198	0.01	100	14.2	24280	PASS
442	198	50	100	93.8	160725	PASS
443	442	15	24	19.2	30808	PASS